


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051519\
 Data File : VU032015.D
 Acq On : 15 May 2019 08:35
 Operator : JC/SP
 Sample : BFB43
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB43

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM051419WMA.M
 Title : VOC Analysis
 Last Update : Thu May 16 04:24:16 2019

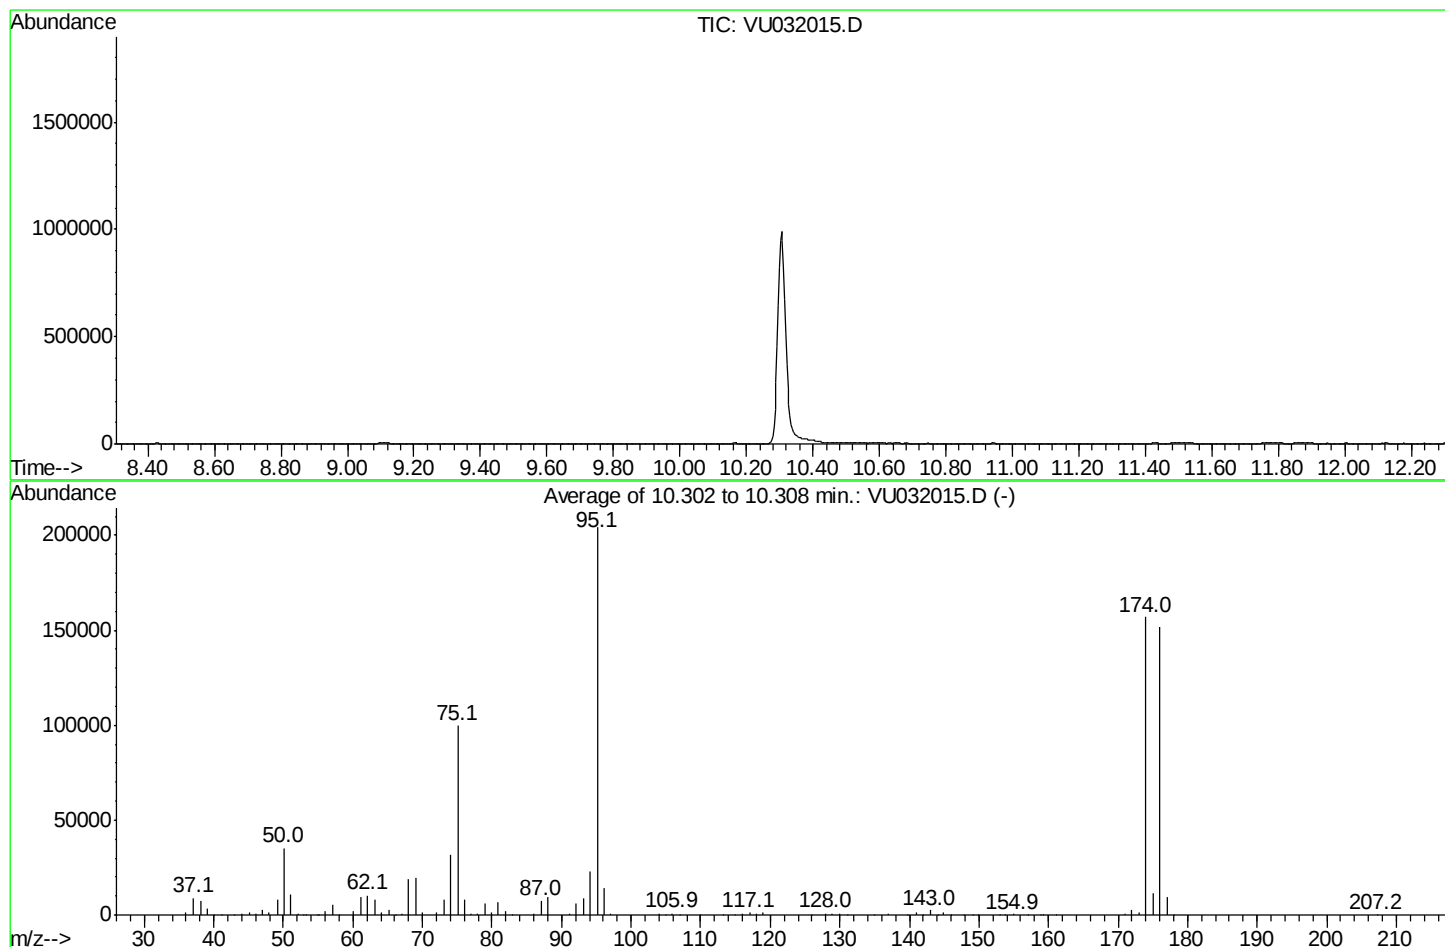

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	35274	PASS
75	95	30	80	48.8	99597	PASS
95	95	100	100	100.0	204202	PASS
96	95	5	9	6.9	13995	PASS
173	174	0.00	2	0.9	1389	PASS
174	95	50	120	76.8	156842	PASS
175	174	5	9	7.5	11701	PASS
176	174	95	101	96.7	151701	PASS
177	176	5	9	6.2	9462	PASS

Scan 2853 (10.263 min): VU032015.D
BFB43

m/z	Abundance
40.00	705.0
44.00	1298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	1672.0
37.10	8801.0
38.10	7560.0
39.00	3724.0
40.00	996.0
44.00	1862.0
45.00	1502.0
46.00	402.0
47.00	2629.0
47.90	1541.0
49.10	8270.0
50.00	34848.0
51.10	10798.0
52.10	732.0
52.80	224.0
53.20	166.0
54.80	441.0
56.00	2299.0
57.00	5469.0
58.00	266.0
60.00	1664.0
61.10	9371.0
62.10	11113.0
63.10	8213.0
64.10	1661.0
65.10	2234.0
66.10	110.0
67.10	433.0
68.00	19584.0
69.10	19736.0
70.00	1572.0
72.10	1175.0
73.10	8170.0
74.10	31760.0
75.10	99784.0
76.00	7545.0
77.00	900.0
77.90	812.0
79.00	6018.0
80.00	1555.0
80.90	6108.0
82.00	1794.0
82.80	274.0
85.90	356.0
87.00	7549.0
88.00	9591.0
91.10	786.0
92.00	5229.0
93.10	8858.0
94.10	22360.0
95.10	201280.0
96.10	13444.0
97.00	463.0
104.00	745.0
105.00	245.0
105.90	862.0
107.00	203.0
109.90	142.0
113.20	133.0
114.90	173.0
115.90	694.0
117.10	1314.0
118.00	704.0
118.90	1267.0
125.90	135.0
128.00	716.0
128.90	486.0
129.90	696.0
131.00	169.0
134.80	225.0
136.90	453.0
141.00	1307.0
141.90	165.0
143.00	2388.0
144.10	255.0
144.90	1170.0
145.90	376.0
147.80	237.0
149.00	136.0
149.90	143.0
152.90	104.0
153.80	236.0
155.00	379.0
157.00	255.0
171.00	635.0
172.00	2609.0
174.00	151744.0
175.00	12258.0
176.00	147392.0
177.00	9477.0
178.00	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	1736.0
37.10	9542.0
38.00	7528.0
39.00	3810.0
40.00	1056.0
41.10	115.0
44.00	1969.0
45.00	1458.0
46.00	427.0
47.00	2703.0
47.90	1447.0
49.10	8615.0
50.10	36464.0
51.10	11051.0
52.10	760.0
52.90	155.0
55.00	408.0
56.00	2380.0
57.00	5651.0
58.00	271.0
60.00	1933.0
61.10	10049.0
62.10	10665.0
63.10	8536.0
64.10	1710.0
65.10	2566.0
66.10	212.0
67.10	531.0
68.00	18936.0
69.10	20344.0
70.00	1584.0
72.00	1246.0
73.10	8304.0
74.10	32664.0
75.10	102584.0
76.10	8274.0
77.00	902.0
78.00	828.0
79.00	6187.0
80.00	1537.0
80.90	6653.0
82.00	1846.0
82.80	282.0
85.90	561.0
87.00	7833.0
88.00	9807.0
91.10	862.0
92.00	6216.0
93.10	9049.0
94.10	23208.0
95.10	210880.0
96.10	14530.0
97.00	524.0
104.10	761.0
105.00	237.0
105.90	923.0
107.10	195.0
110.00	119.0
113.20	101.0
114.80	245.0
115.90	832.0
117.10	1311.0
117.90	703.0
118.90	1302.0
125.90	126.0
128.00	881.0
128.90	523.0
130.00	709.0
131.00	234.0
134.90	297.0
136.90	443.0
139.70	114.0
141.00	1290.0
141.90	145.0
143.00	2710.0
144.00	245.0
144.90	1325.0
145.90	316.0
147.80	273.0
149.00	189.0
149.90	168.0
153.70	263.0
155.00	382.0
156.90	253.0
159.20	115.0
161.00	140.0
171.00	628.0
172.00	2926.0
173.00	2063.0
174.00	161792.0
175.00	12030.0
176.00	156544.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

177.00	9850.0
178.00	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

m/z	Abundance
36.00	1685.0
37.10	8980.0
38.00	7006.0
39.10	3526.0
39.90	1103.0
43.00	108.0
44.00	2106.0
45.10	1309.0
46.00	418.0
47.00	2621.0
47.90	1162.0
49.10	7988.0
50.10	34512.0
51.10	10374.0
52.10	617.0
52.90	170.0
55.10	487.0
56.00	2353.0
57.10	4992.0
58.00	199.0
60.00	2135.0
61.10	9358.0
62.10	9569.0
63.10	8215.0
64.10	1526.0
65.10	2409.0
66.10	247.0
67.00	548.0
68.00	17216.0
69.10	19400.0
70.00	1240.0
72.00	1175.0
73.10	7873.0
74.10	31032.0
75.10	96424.0
76.10	7922.0
77.00	828.0
78.00	730.0
79.00	5929.0
80.00	1541.0
80.90	6618.0
82.00	1626.0
82.90	250.0
85.90	652.0
87.00	7514.0
88.00	8838.0
91.10	758.0
92.00	5839.0
93.10	8903.0
94.10	22288.0
95.10	200448.0
96.10	14013.0
97.10	478.0
104.10	852.0
104.90	186.0
105.90	859.0
107.10	166.0
110.00	106.0
114.80	297.0
115.90	758.0
117.00	1271.0
117.90	671.0
119.00	1287.0
127.90	771.0
129.00	478.0
130.00	750.0
131.00	316.0
135.00	370.0
136.90	350.0
139.70	140.0
141.00	1303.0
141.90	130.0
143.00	2645.0
144.00	217.0
144.90	1270.0
145.90	211.0
147.80	403.0
149.10	184.0
149.90	161.0
153.80	174.0
154.90	413.0
156.90	231.0
158.80	142.0
159.20	112.0
161.00	208.0
170.90	526.0
172.00	2815.0
173.00	2105.0
174.00	156992.0
175.00	10816.0
176.00	151168.0
177.00	9061.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43

178.00207.20

220.0108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB43