


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051520\
 Data File : VU038186.D
 Acq On : 15 May 2020 08:57
 Operator : JC/MD
 Sample : BFB24
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat May 16 03:30:00 2020

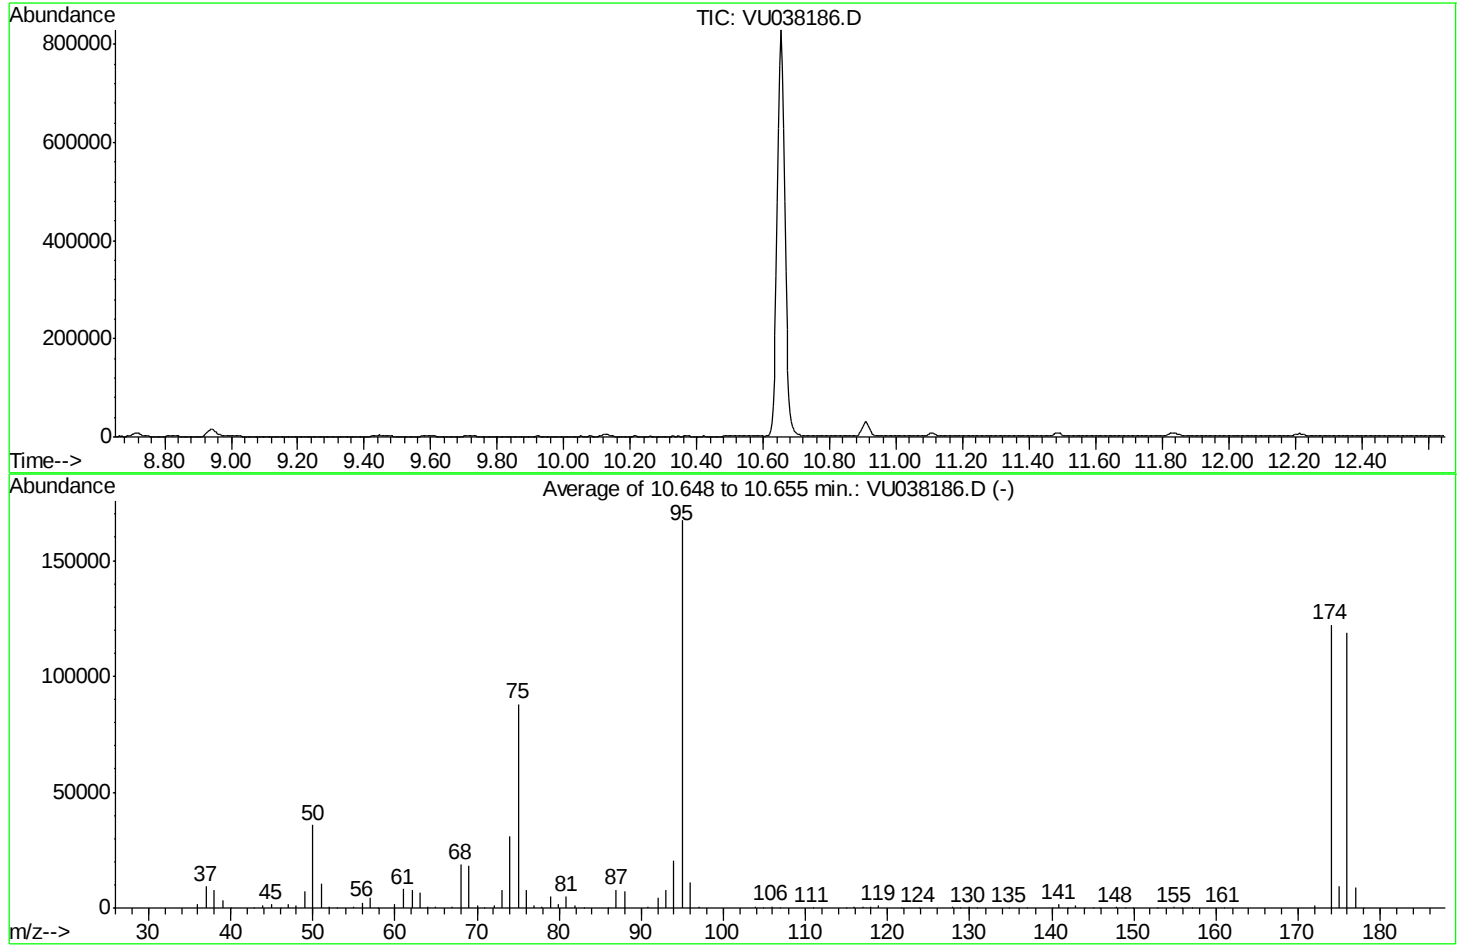

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	35770	PASS
75	95	30	80	52.6	88064	PASS
95	95	100	100	100.0	167338	PASS
96	95	5	9	6.6	11040	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.0	122234	PASS
175	174	5	9	7.7	9447	PASS
176	174	95	101	97.3	118925	PASS
177	176	5	9	7.2	8597	PASS

Scan 2881 (10.603 min): VU038186.D
BFB24

m/z	Abundance
36.00	325.0
40.00	230.0
43.90	845.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	1801.0
37.00	8872.0
38.00	7698.0
39.00	3122.0
40.00	470.0
42.90	182.0
44.00	2098.0
44.90	1281.0
47.00	1949.0
47.90	962.0
49.00	7221.0
50.00	34104.0
51.00	10397.0
52.00	469.0
53.00	103.0
54.90	337.0
56.00	2294.0
57.00	4562.0
57.90	246.0
60.00	1351.0
61.00	7900.0
62.00	7827.0
63.00	6368.0
64.00	595.0
65.00	770.0
66.90	518.0
68.00	17352.0
69.00	17752.0
70.00	1253.0
72.10	901.0
73.00	7453.0
74.00	29128.0
75.00	83904.0
76.00	7728.0
76.90	916.0
77.80	576.0
78.90	4896.0
79.90	1499.0
80.90	4832.0
81.90	1154.0
83.00	123.0
85.90	200.0
86.90	7405.0
87.90	6880.0
90.80	433.0
92.00	3972.0
93.00	7293.0
94.00	19464.0
95.00	157440.0
96.00	10811.0
97.00	333.0
103.90	565.0
104.80	175.0
105.90	610.0
106.90	187.0
110.80	214.0
114.90	124.0
115.90	425.0
116.90	826.0
118.00	515.0
118.90	778.0
128.00	342.0
128.90	223.0
129.90	375.0
130.90	127.0
134.90	252.0
136.90	236.0
139.90	107.0
140.90	1345.0
142.00	162.0
143.00	1170.0
145.00	175.0
145.80	226.0
147.80	298.0
149.00	142.0
149.90	119.0
152.90	107.0
155.00	329.0
155.90	110.0
157.00	184.0
160.90	169.0
172.00	973.0
174.00	111800.0
175.00	8840.0
176.00	109848.0
177.00	8227.0
177.90	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	1866.0
37.00	9436.0
38.00	8199.0
39.00	3477.0
40.00	475.0
42.90	196.0
44.00	2072.0
45.00	1425.0
47.00	1917.0
47.90	1039.0
49.00	7511.0
50.00	37088.0
51.00	10749.0
51.90	502.0
53.00	128.0
54.90	411.0
56.00	2488.0
57.00	4832.0
58.00	184.0
60.00	1548.0
61.00	8464.0
62.00	8221.0
63.00	7135.0
64.00	766.0
65.00	801.0
67.00	506.0
68.00	19176.0
69.00	18952.0
70.00	1349.0
72.10	1011.0
73.00	7994.0
74.00	32024.0
75.00	90840.0
76.00	8000.0
76.90	904.0
77.90	650.0
78.90	5394.0
79.90	1685.0
80.90	4959.0
81.90	1239.0
83.00	139.0
85.90	224.0
86.90	8044.0
87.90	7297.0
90.90	563.0
92.00	4605.0
93.00	7899.0
94.00	21440.0
95.00	172544.0
96.00	11305.0
97.00	317.0
103.90	568.0
104.80	209.0
105.90	645.0
106.90	164.0
110.90	187.0
114.90	113.0
115.90	525.0
117.00	753.0
118.00	644.0
118.90	855.0
123.80	112.0
128.00	384.0
128.90	227.0
129.90	407.0
131.00	163.0
134.80	248.0
136.90	201.0
140.00	149.0
140.90	1533.0
141.90	145.0
143.00	1316.0
145.00	197.0
145.90	251.0
147.80	364.0
149.00	176.0
152.90	115.0
154.90	316.0
155.90	159.0
157.00	228.0
160.90	194.0
172.00	844.0
174.00	125792.0
175.00	9676.0
176.00	122600.0
177.00	8909.0
177.90	210.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
35.90	1889.0
37.00	9119.0
38.00	7886.0
39.00	3544.0
40.00	406.0
42.80	141.0
44.00	1910.0
45.00	1507.0
46.00	221.0
47.00	1807.0
47.90	1105.0
49.00	7377.0
50.00	36120.0
51.00	10196.0
51.90	534.0
52.90	133.0
54.90	433.0
56.00	2453.0
57.00	4743.0
58.00	135.0
60.00	1618.0
61.00	8419.0
62.10	7895.0
63.00	7145.0
64.00	848.0
65.00	735.0
67.00	496.0
68.00	19168.0
69.00	18576.0
70.00	1337.0
70.90	124.0
72.10	820.0
73.00	7934.0
74.00	31624.0
75.00	89448.0
76.00	7461.0
77.00	955.0
77.90	683.0
78.90	5256.0
80.00	1569.0
80.90	4805.0
81.90	1294.0
82.90	159.0
85.90	247.0
87.00	8065.0
88.00	7344.0
90.90	641.0
92.00	4800.0
93.00	7477.0
94.00	21312.0
95.00	172032.0
96.00	11004.0
97.10	299.0
103.90	569.0
104.90	214.0
105.90	577.0
106.80	149.0
110.90	123.0
114.90	107.0
115.90	545.0
117.00	704.0
118.00	706.0
118.90	929.0
121.70	106.0
123.80	129.0
127.90	470.0
128.90	208.0
129.90	431.0
131.00	172.0
134.90	231.0
136.90	184.0
140.10	174.0
140.90	1485.0
141.80	159.0
142.90	1378.0
143.90	120.0
145.00	218.0
145.90	263.0
147.80	382.0
148.90	164.0
152.80	100.0
154.90	348.0
155.80	151.0
157.00	249.0
160.90	184.0
172.00	756.0
174.00	129112.0
175.00	9826.0
176.00	124328.0
177.00	8655.0
178.00	195.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24