

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
 Data File : VU043768.D
 Acq On : 14 May 2021 20:39
 Operator : SY/MD
 Sample : M2376-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: May 15 01:20:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 15 00:49:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	231176	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	233069	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	108224	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	86596	5.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.60%
7) Chloroethane-d5	1.919	69	61756	5.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.80%
11) 1,1-Dichloroethene-d2	2.575	65	36623	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	103.60%
20) 2-Butanone-d5	4.642	46	158035	48.76	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.52%
24) Chloroform-d	5.073	84	140841	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
26) 1,2-Dichloroethane-d4	5.710	65	72525	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
32) Benzene-d6	5.735	84	296760	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.20%
36) 1,2-Dichloropropane-d6	6.700	67	93893	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.906	98	249543	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
43) trans-1,3-Dichloroprop...	8.185	79	32385	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.642	63	151829	48.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.28%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	72030	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
66) 1,2-Dichlorobenzene-d4	12.201	152	92599	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%
Target Compounds						
16) Methylene chloride	3.054	84	8271	0.37	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
Data File : VU043768.D
Acq On : 14 May 2021 20:39
Operator : SY/MD
Sample : M2376-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: May 15 01:20:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 15 00:49:19 2021
Response via : Initial Calibration

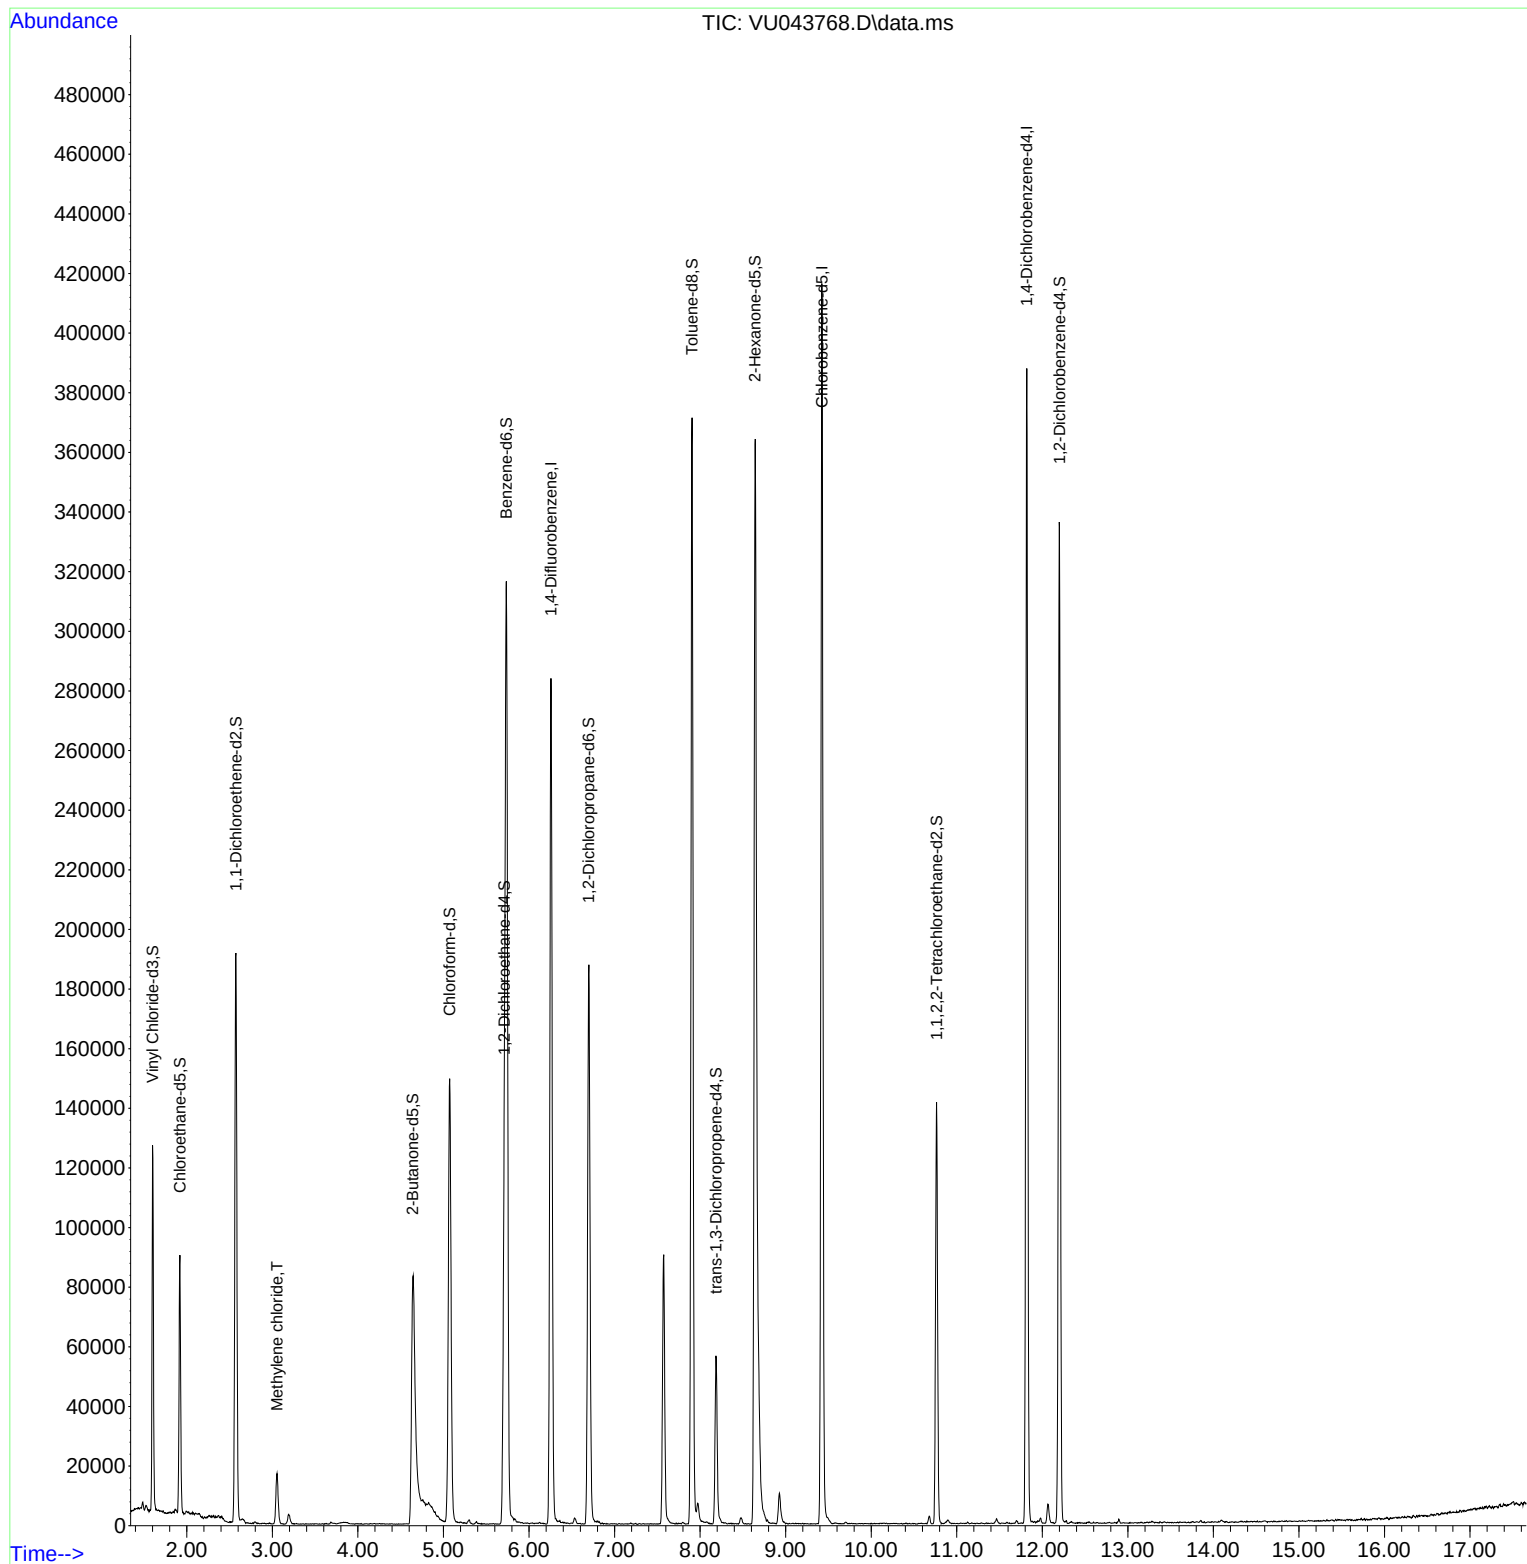

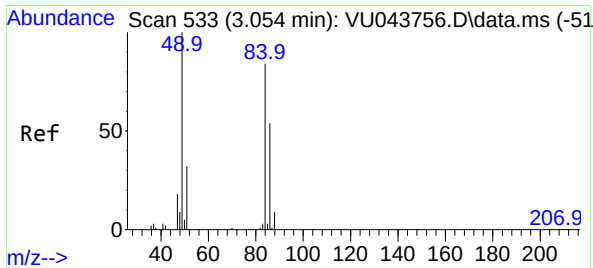

#16
Methylene chloride
Concen: 0.37 ug/L
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU043768.D
Acq: 14 May 2021 20:39

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

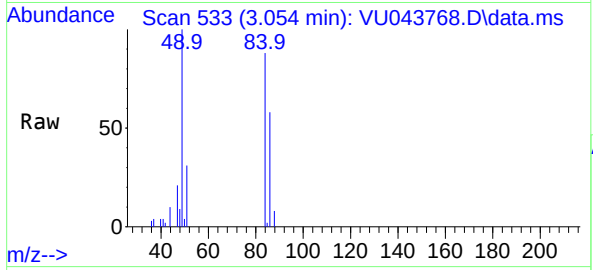

Tgt Ion:	84	Resp:	8271
Ion	Ratio	Lower	Upper
84	100		
86	65.7	44.7	82.9
49	113.2	83.1	154.3

