

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
 Data File : VU043770.D
 Acq On : 14 May 2021 21:27
 Operator : SY/MD
 Sample : M2418-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG1Y9

Quant Time: May 15 01:20:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 15 00:49:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	222939	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	227084	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	109410	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	84790	5.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.20%
7) Chloroethane-d5	1.919	69	57636	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.40%
11) 1,1-Dichloroethene-d2	2.571	65	34501	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	101.20%
20) 2-Butanone-d5	4.639	46	197308	63.13	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.26%
24) Chloroform-d	5.073	84	137695	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
26) 1,2-Dichloroethane-d4	5.710	65	72642	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.00%
32) Benzene-d6	5.735	84	291883	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.700	67	93473	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.906	98	246430	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
43) trans-1,3-Dichloroprop...	8.185	79	32271	4.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.60%
46) 2-Hexanone-d5	8.642	63	154881	50.40	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.80%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	73078	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
66) 1,2-Dichlorobenzene-d4	12.201	152	94562	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%
Target Compounds						
13) Acetone	2.645	43	5478	2.76	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
Data File : VU043770.D
Acq On : 14 May 2021 21:27
Operator : SY/MD
Sample : M2418-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Y9

Quant Time: May 15 01:20:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 15 00:49:19 2021
Response via : Initial Calibration

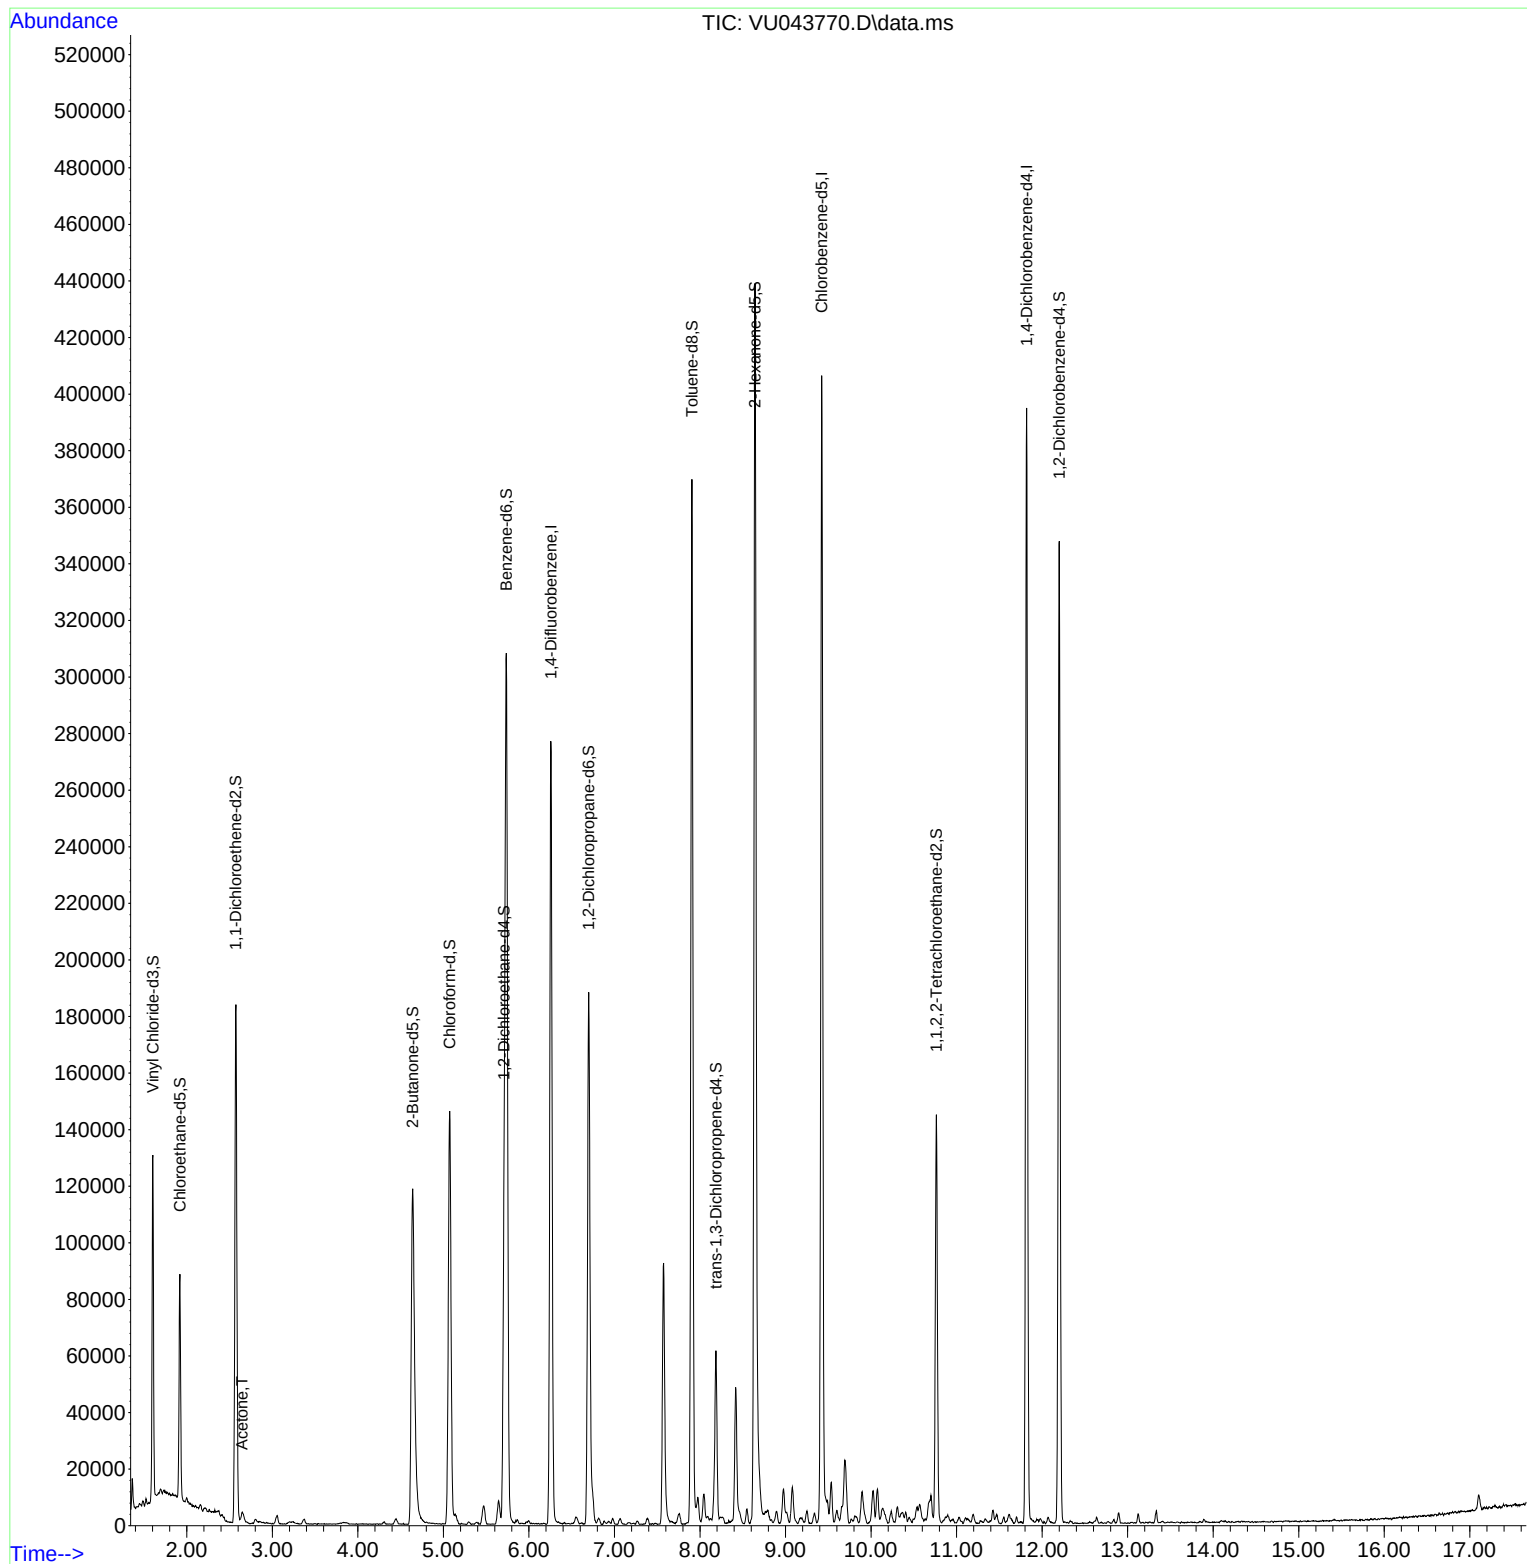

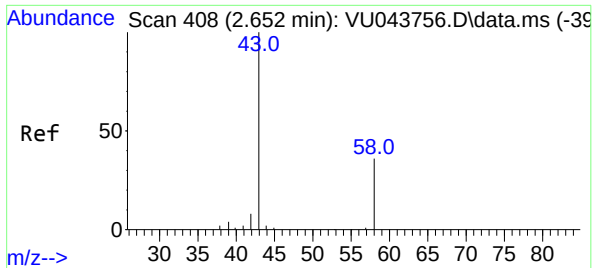

#13
 Acetone
 Concen: 2.76 ug/L
 RT: 2.645 min Scan# 406
 Delta R.T. -0.007 min
 Lab File: VU043770.D
 Acq: 14 May 2021 21:27

Instrument :
 MSVOA_U
 ClientSampleId :
 BG1Y9

Tgt Ion: 43	Resp: 5478
Ion Ratio	Lower Upper
43	100
58	30.3 0.0 71.6

