

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
 Data File : VU043768.D
 Acq On : 14 May 2021 20:39
 Operator : SY/MD
 Sample : M2376-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rBV	122376	136176	16.56%	2.023%
2	1.919	171	180	190	rBV	86383	109547	13.33%	1.627%
3	2.575	371	384	399	rBV	190830	313050	38.08%	4.650%
4	3.054	517	533	548	rBV	16972	31811	3.87%	0.472%
5	4.645	1011	1028	1057	rBV	83321	273249	33.24%	4.058%
6	5.073	1144	1161	1184	rVB	148703	326762	39.75%	4.853%
7	5.735	1342	1367	1394	rBV2	316197	804756	97.89%	11.952%
8	6.256	1512	1529	1545	rBV	283678	534793	65.05%	7.943%
9	6.700	1652	1667	1689	rBV	187558	368238	44.79%	5.469%
10	7.575	1926	1939	1966	rBV	90233	162905	19.82%	2.420%
11	7.906	2028	2042	2057	rBV	371041	638435	77.66%	9.482%
12	7.970	2058	2062	2076	rVB2	6195	10808	1.31%	0.161%
13	8.186	2116	2129	2152	rBV	56394	99545	12.11%	1.478%
14	8.645	2258	2272	2313	rBV	363883	822091	100.00%	12.210%
15	8.928	2349	2360	2375	rBV2	10318	20577	2.50%	0.306%
16	9.423	2500	2514	2534	rBV	416046	677328	82.39%	10.060%
17	10.764	2919	2931	2948	rVB	141418	228712	27.82%	3.397%
18	11.819	3242	3259	3275	rBV	387372	611948	74.44%	9.089%
19	12.066	3325	3336	3348	rBV3	6476	11348	1.38%	0.169%
20	12.198	3359	3377	3396	rBV	335931	550877	67.01%	8.182%




Sum of corrected areas: 6732956

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
Data File : VU043768.D
Acq On : 14 May 2021 20:39
Operator : SY/MD
Sample : M2376-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

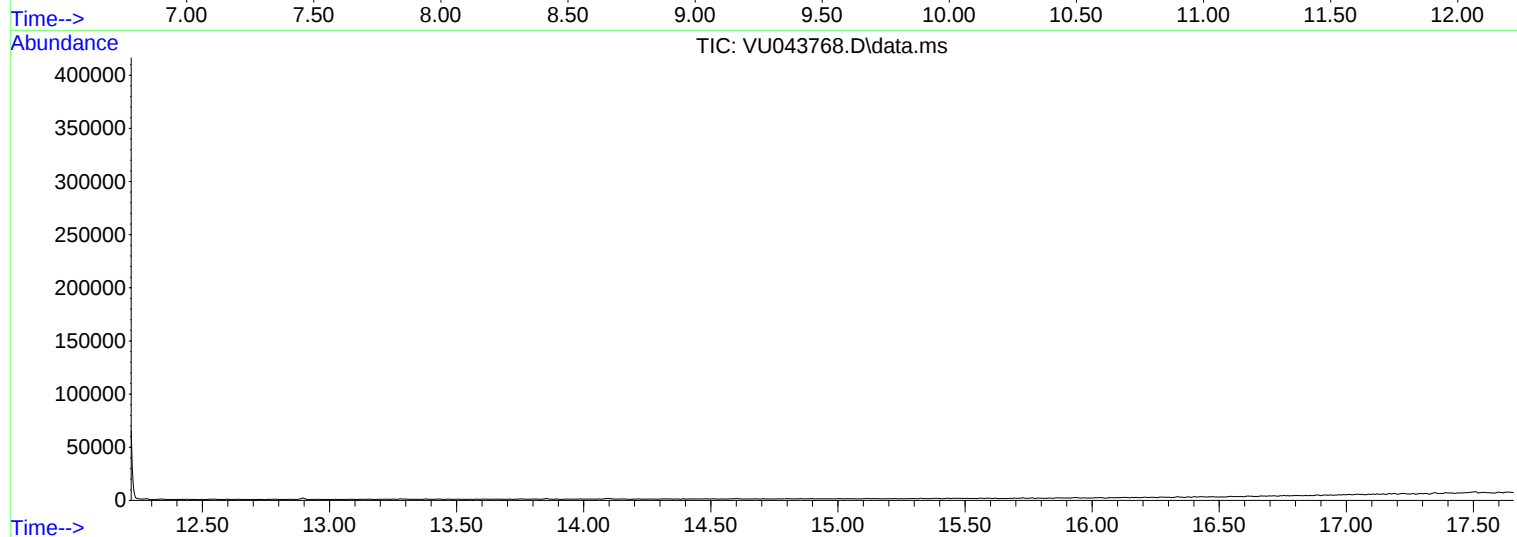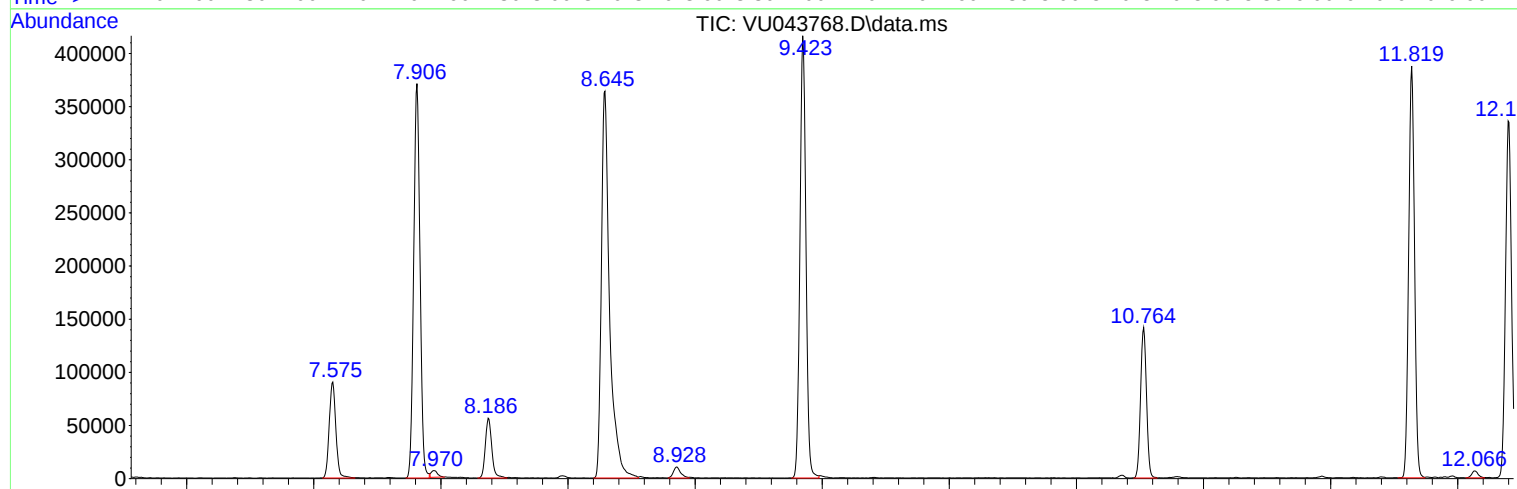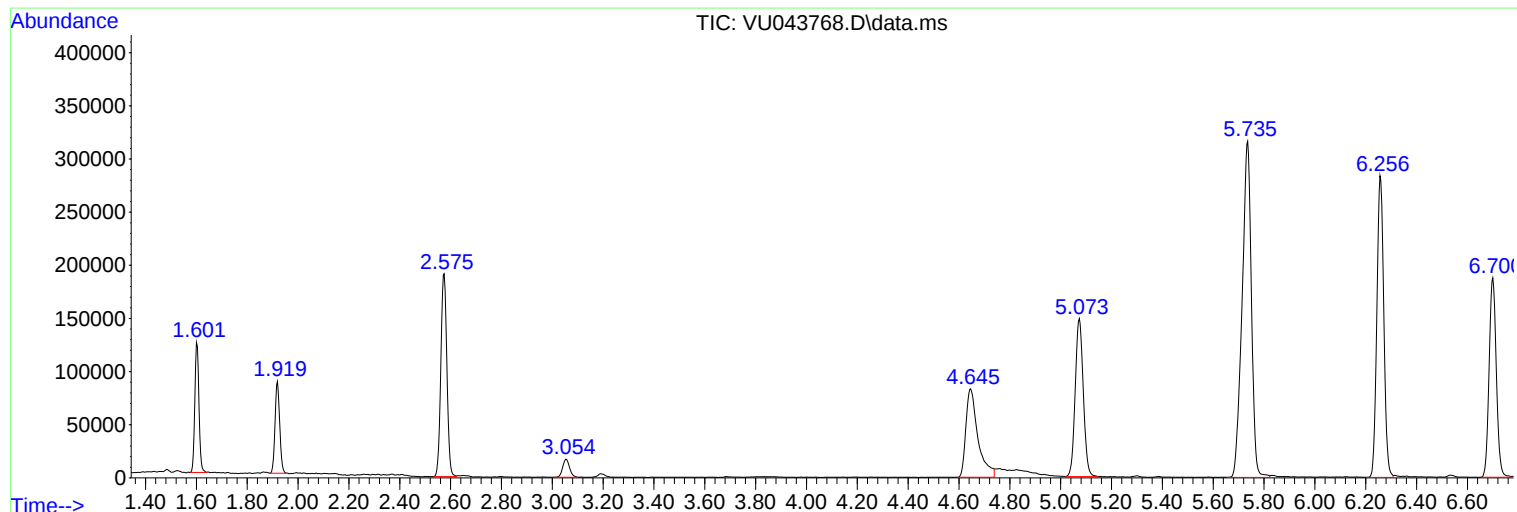

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
Data File : VU043768.D
Acq On : 14 May 2021 20:39
Operator : SY/MD
Sample : M2376-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
Data File : VU043768.D
Acq On : 14 May 2021 20:39
Operator : SY/MD
Sample : M2376-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
