


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051521\
Data File : VU043753.D
Acq On : 14 May 2021 14:05
Operator : SY/MD
Sample : BFB44
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB144

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat May 15 00:49:19 2021

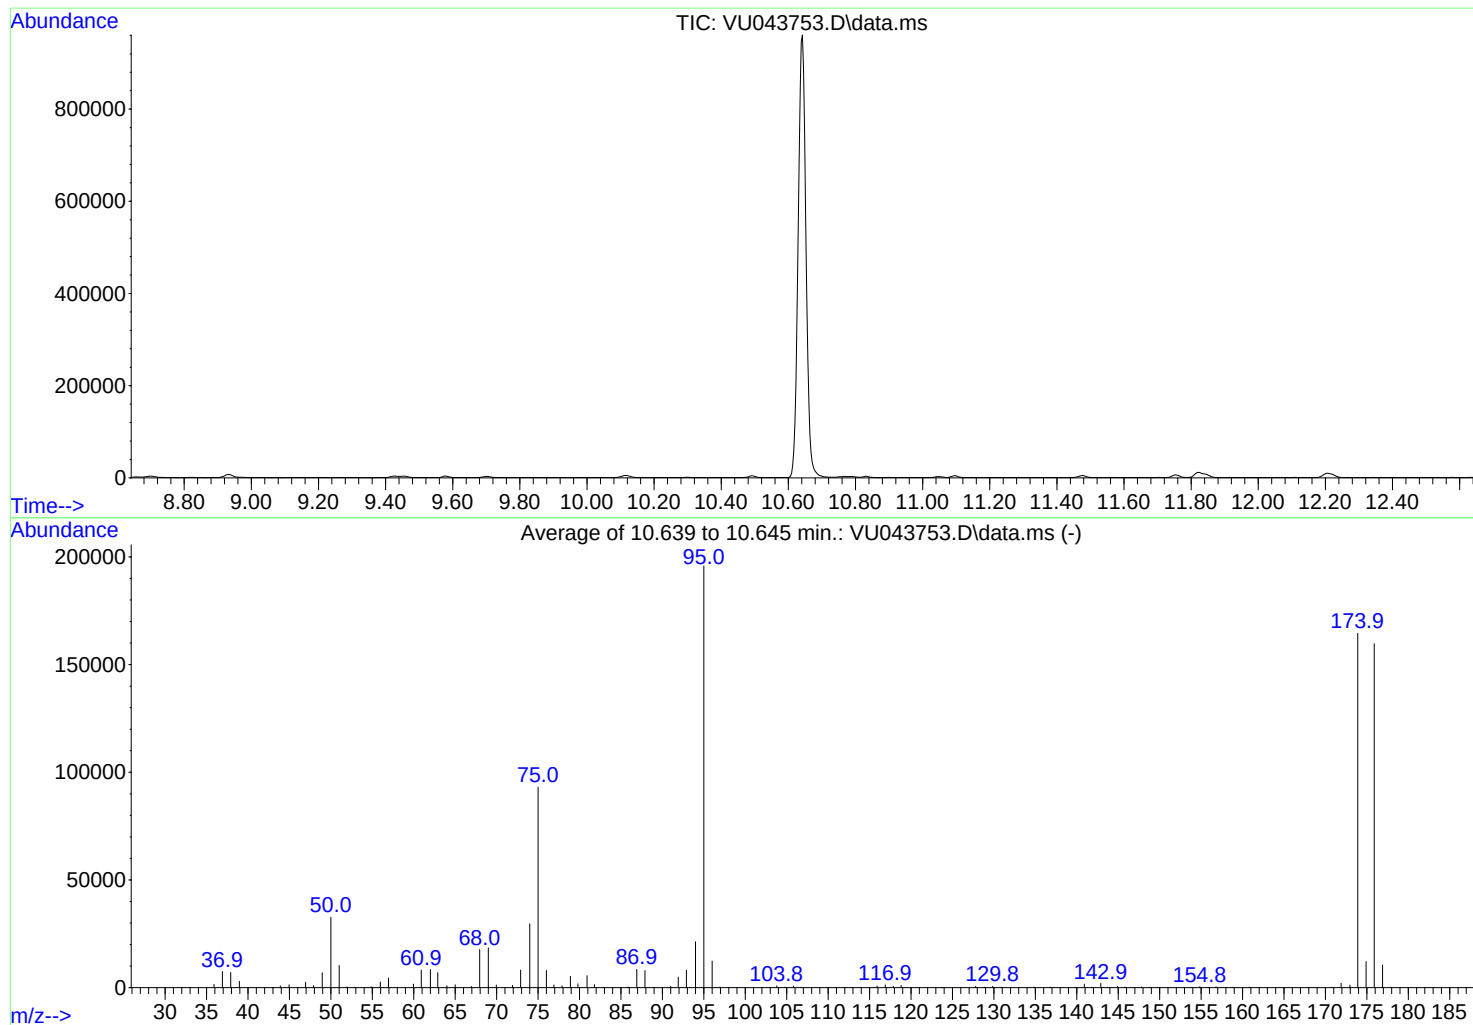

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	32715	PASS
75	95	30	80	47.5	93099	PASS
95	95	100	100	100.0	195861	PASS
96	95	5	9	6.3	12374	PASS
173	174	0.00	2	0.7	1168	PASS
174	95	50	120	84.0	164523	PASS
175	174	5	9	7.4	12137	PASS
176	174	95	101	97.1	159765	PASS
177	176	5	9	6.6	10467	PASS

m/z	Abundance
35.90	1503.0
36.90	7109.0
37.90	6514.0
38.90	2968.0
39.90	366.0
42.90	106.0
43.90	1320.0
44.90	1347.0
46.90	2409.0
47.90	966.0
48.90	6528.0
50.00	30832.0
51.00	9525.0
51.90	384.0
52.80	113.0
54.90	435.0
56.00	2539.0
57.00	4307.0
58.00	225.0
60.00	1552.0
60.90	7648.0
62.00	8136.0
62.90	6439.0
64.00	897.0
65.00	1151.0
66.00	140.0
67.00	492.0
67.90	16624.0
69.00	17648.0
69.90	1137.0
71.90	952.0
72.90	7715.0
74.00	28432.0
75.00	87928.0
76.00	7492.0
76.90	1239.0
77.90	824.0
78.90	5107.0
79.80	1653.0
80.90	5340.0
81.80	1263.0
82.90	166.0
85.80	303.0
86.90	8061.0
87.90	7339.0
91.00	518.0
91.90	4686.0
92.90	7798.0
94.00	20208.0
95.00	185024.0
96.00	11446.0
96.90	224.0
103.80	816.0
104.80	282.0
105.80	773.0
106.80	135.0
112.90	119.0
114.90	123.0
115.90	695.0
116.90	1242.0
117.90	649.0
118.80	985.0
127.80	554.0
128.90	229.0
129.90	659.0
130.90	215.0
134.90	249.0
136.80	258.0
139.90	131.0
140.90	1474.0
141.80	233.0
142.90	1849.0
143.80	149.0
144.90	555.0
145.90	245.0
147.80	407.0
148.80	116.0
149.80	163.0
152.90	163.0
153.80	114.0
154.90	411.0
155.90	107.0
156.80	417.0
158.80	143.0
160.80	228.0
170.70	180.0
171.90	1916.0
173.90	159168.0
174.90	11343.0
175.90	154816.0
176.90	9937.0
177.90	200.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
39.90	160.0
43.90	505.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	1474.0
36.90	7721.0
37.90	7489.0
39.00	2844.0
39.90	281.0
44.00	1337.0
45.00	1314.0
46.00	202.0
47.00	2554.0
47.90	955.0
48.90	7061.0
50.00	33592.0
51.00	10708.0
52.00	378.0
52.80	132.0
54.80	457.0
55.90	2582.0
56.90	4588.0
58.10	228.0
59.90	1745.0
60.90	8506.0
62.00	8449.0
62.90	7292.0
64.00	948.0
65.00	1497.0
66.00	207.0
66.90	487.0
68.00	18248.0
69.00	18600.0
70.00	1383.0
71.90	1086.0
72.90	8297.0
74.00	30064.0
75.00	95480.0
76.00	8157.0
76.90	1212.0
77.90	825.0
78.90	5393.0
79.80	1823.0
80.90	5594.0
81.80	1479.0
82.90	162.0
86.00	279.0
86.90	8611.0
87.90	8286.0
91.00	636.0
91.90	5055.0
92.90	7978.0
94.00	21704.0
95.00	200448.0
96.00	12992.0
97.00	323.0
103.80	755.0
104.80	268.0
105.80	734.0
106.80	167.0
110.90	105.0
112.80	135.0
115.90	763.0
116.90	1188.0
117.80	540.0
118.80	1023.0
123.70	103.0
127.80	619.0
128.80	265.0
129.80	568.0
130.80	245.0
134.80	274.0
136.80	288.0
139.70	115.0
140.90	1680.0
141.80	210.0
142.90	2113.0
143.70	158.0
144.90	674.0
145.70	323.0
146.80	143.0
147.80	412.0
148.90	150.0
149.70	139.0
153.00	133.0
153.80	148.0
154.80	443.0
156.80	419.0
158.80	170.0
160.80	158.0
170.70	311.0
171.90	2001.0
172.90	1734.0
173.90	165056.0
174.90	12501.0
175.90	159616.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

176.9010626.0

177.90201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

m/z	Abundance
35.90	1542.0
36.90	7697.0
37.90	7200.0
39.00	3011.0
39.90	318.0
44.00	1359.0
45.00	1404.0
46.90	2716.0
47.90	996.0
49.00	7116.0
50.00	33720.0
51.00	10580.0
51.90	396.0
52.80	135.0
54.80	478.0
55.90	2687.0
57.00	4605.0
58.10	243.0
59.90	1730.0
60.90	8376.0
62.00	8633.0
62.90	7229.0
64.00	930.0
65.00	1396.0
66.10	188.0
67.00	534.0
68.00	18160.0
69.00	18992.0
70.00	1306.0
71.90	1072.0
72.90	8419.0
74.00	30520.0
75.00	95888.0
76.00	8193.0
76.90	1258.0
77.90	832.0
78.90	5453.0
79.80	1862.0
80.90	5743.0
81.80	1430.0
82.90	183.0
85.80	272.0
86.90	8783.0
87.90	8266.0
91.00	619.0
91.90	5046.0
92.90	8206.0
94.00	22032.0
95.00	202112.0
96.00	12683.0
97.00	267.0
103.80	829.0
104.80	266.0
105.80	781.0
106.70	151.0
110.80	106.0
112.80	129.0
114.90	118.0
115.90	743.0
116.90	1279.0
117.90	600.0
118.80	1059.0
127.80	614.0
128.80	258.0
129.80	610.0
130.90	231.0
134.90	283.0
136.80	285.0
139.80	120.0
140.90	1683.0
141.80	244.0
142.90	2059.0
143.70	160.0
144.90	628.0
145.80	282.0
146.80	115.0
147.80	424.0
148.90	146.0
149.80	151.0
152.90	167.0
153.80	135.0
154.90	437.0
155.80	104.0
156.80	455.0
158.80	158.0
160.80	203.0
170.70	244.0
171.90	2030.0
173.00	1770.0
173.90	169344.0
174.90	12568.0
175.90	164864.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144

176.90	10839.0
177.90	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB144