


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051524\
Data File : VU058895.D
Acq On : 15 May 2024 10:30
Operator : MD/SY
Sample : BFB155
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB155

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu May 16 01:51:35 2024

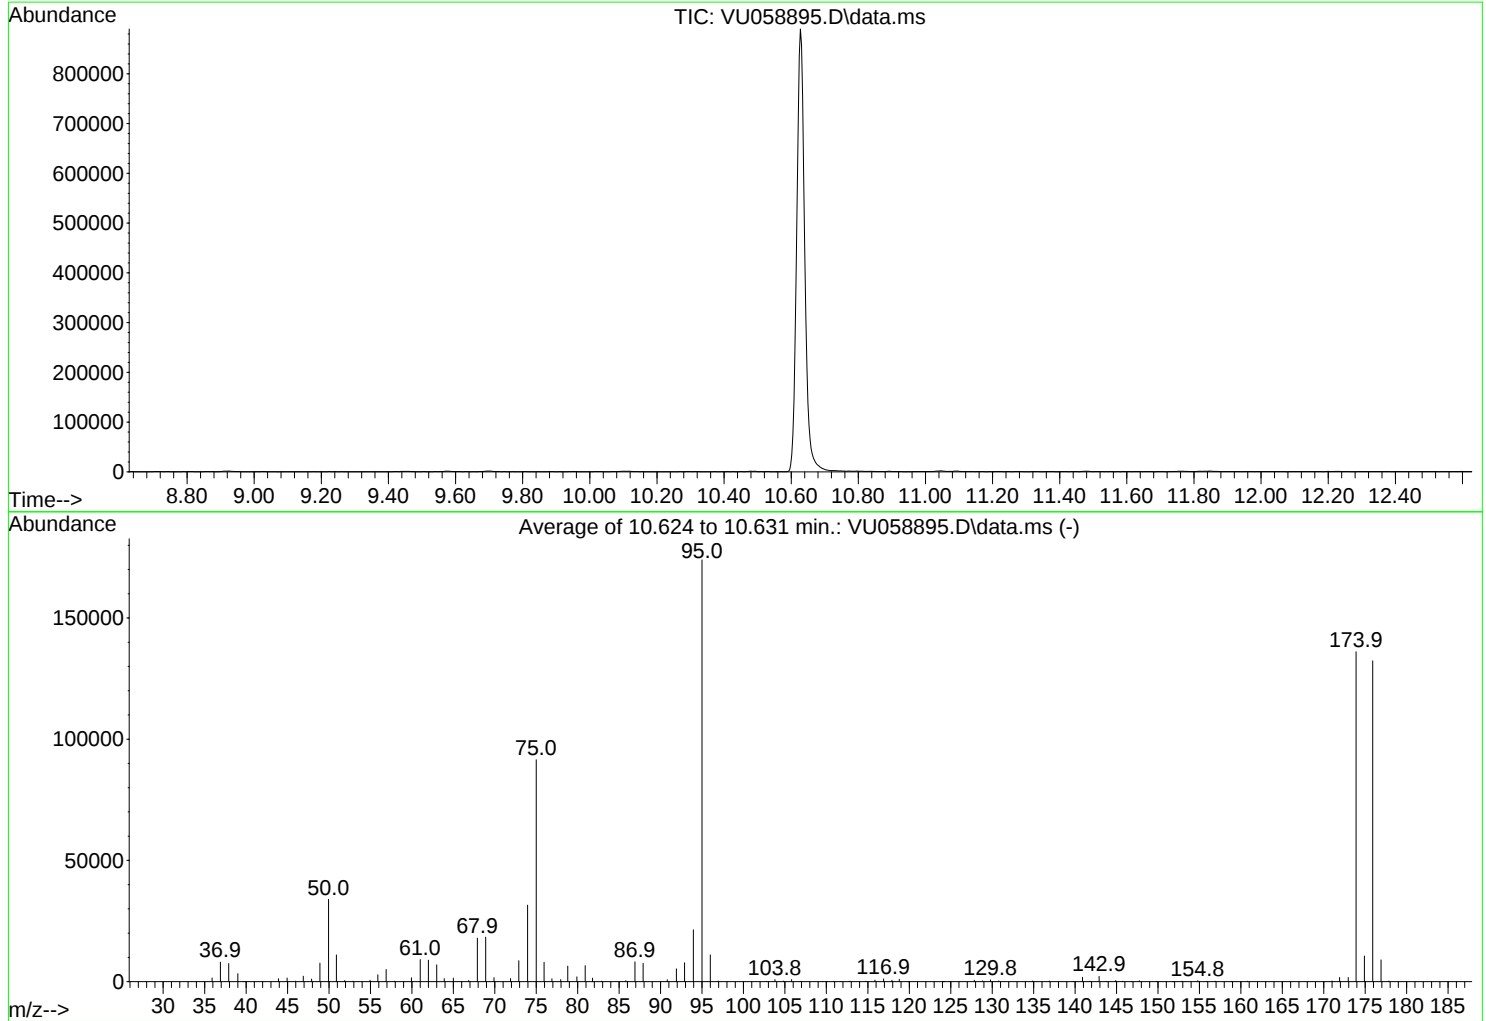

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	33907	PASS
75	95	30	80	52.6	91515	PASS
95	95	100	100	100.0	173995	PASS
96	95	5	9	6.3	11021	PASS
173	174	0.00	2	1.3	1703	PASS
174	95	50	120	78.2	136125	PASS
175	174	5	9	7.8	10585	PASS
176	174	95	101	97.2	132333	PASS
177	176	5	9	6.8	8978	PASS

m/z	Abundance
39.80	123.0
43.90	293.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

m/z	Abundance
35.90	1510.0
36.90	8028.0
37.90	7670.0
39.00	3397.0
39.70	287.0
43.90	1442.0
44.90	1469.0
45.90	179.0
46.90	2070.0
47.90	1055.0
48.90	7728.0
50.00	33584.0
50.90	10844.0
51.90	489.0
53.00	188.0
54.90	554.0
55.90	2788.0
56.90	4921.0
57.90	224.0
59.90	1576.0
61.00	8933.0
62.00	9022.0
63.00	6923.0
63.90	1251.0
65.00	1428.0
65.90	142.0
66.80	477.0
67.90	17864.0
68.90	18384.0
69.90	1547.0
71.90	1291.0
72.90	8272.0
74.00	31144.0
75.00	90072.0
75.90	8174.0
76.90	1243.0
77.90	776.0
78.80	6251.0
79.90	1908.0
80.90	6491.0
81.80	1367.0
82.90	191.0
85.80	403.0
86.90	8098.0
87.90	7567.0
90.80	852.0
91.90	5091.0
92.90	7654.0
94.00	21064.0
95.00	169792.0
96.00	10843.0
97.00	293.0
102.80	102.0
103.80	842.0
104.80	259.0
105.80	837.0
106.80	142.0
109.50	112.0
111.00	160.0
111.70	128.0
112.90	166.0
114.80	191.0
115.90	608.0
116.90	1084.0
117.90	525.0
118.80	898.0
119.90	110.0
124.10	100.0
127.90	627.0
128.90	299.0
129.80	722.0
130.80	345.0
134.80	206.0
136.90	276.0
139.80	167.0
140.90	1722.0
141.80	200.0
142.90	2140.0
143.80	139.0
144.90	444.0
145.70	258.0
146.80	122.0
147.70	368.0
149.80	132.0
152.90	176.0
154.80	417.0
156.90	187.0
158.80	158.0
160.80	204.0
171.00	197.0
171.90	1710.0
172.90	1620.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

173.90	128440.0
174.90	10460.0
175.90	124744.0
176.90	8676.0
177.90	290.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

m/z	Abundance
35.90	1557.0
36.90	8272.0
37.90	7686.0
39.00	3460.0
39.70	259.0
43.90	1475.0
45.00	1599.0
45.90	191.0
46.90	2357.0
47.90	1071.0
48.90	7982.0
49.90	35048.0
50.90	11319.0
51.90	494.0
52.90	171.0
55.00	611.0
55.90	2904.0
56.90	5195.0
57.90	183.0
60.00	1641.0
61.00	9486.0
62.00	9111.0
63.00	7169.0
63.90	1278.0
65.00	1501.0
65.90	131.0
66.90	501.0
67.90	18568.0
68.90	18888.0
69.90	1705.0
71.90	1275.0
72.90	8974.0
74.00	32376.0
75.00	94600.0
76.00	8296.0
76.90	1248.0
78.00	853.0
78.80	6657.0
79.90	2047.0
80.90	6880.0
81.80	1523.0
82.90	168.0
85.80	404.0
86.90	8471.0
87.90	7894.0
90.80	792.0
91.90	5502.0
92.90	8007.0
93.90	22016.0
95.00	179840.0
96.00	11408.0
96.90	302.0
102.80	126.0
103.80	889.0
104.80	252.0
105.80	915.0
106.80	172.0
109.60	126.0
110.90	171.0
111.70	141.0
112.90	213.0
114.80	224.0
115.80	678.0
116.90	1113.0
117.90	642.0
118.80	994.0
124.90	106.0
127.90	602.0
128.80	346.0
129.80	808.0
130.80	361.0
134.90	252.0
136.90	283.0
139.80	148.0
140.90	1785.0
141.80	228.0
142.90	2302.0
143.70	162.0
144.90	507.0
145.80	228.0
146.80	168.0
147.70	452.0
149.90	137.0
152.90	191.0
154.80	434.0
155.80	108.0
156.90	236.0
158.80	164.0
160.80	226.0
171.00	255.0
171.90	1759.0
173.00	1735.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

173.90	140288.0
174.90	11002.0
175.90	137024.0
176.90	9328.0
177.80	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

m/z	Abundance
35.90	1481.0
36.90	7925.0
37.90	7025.0
39.00	3131.0
39.90	213.0
43.90	1509.0
45.00	1499.0
46.00	190.0
46.90	2358.0
47.90	996.0
48.90	7344.0
50.00	33088.0
50.90	10885.0
51.90	426.0
52.80	153.0
54.90	600.0
55.90	2852.0
56.90	5002.0
58.00	128.0
60.00	1589.0
61.00	8954.0
62.00	8411.0
63.00	6721.0
63.90	1151.0
65.00	1481.0
66.00	123.0
66.90	445.0
67.90	17488.0
68.90	17768.0
69.90	1634.0
71.90	1181.0
72.90	8721.0
73.90	31152.0
75.00	89872.0
76.00	7450.0
76.90	1164.0
77.90	875.0
78.80	6395.0
79.90	1925.0
80.90	6538.0
81.80	1562.0
82.90	174.0
85.80	366.0
86.90	7935.0
87.90	7377.0
90.80	664.0
91.90	5218.0
92.90	7635.0
93.90	21016.0
95.00	172352.0
96.00	10811.0
96.90	289.0
102.80	130.0
103.80	915.0
104.80	230.0
105.80	883.0
106.90	136.0
110.00	103.0
110.80	156.0
111.80	145.0
112.80	220.0
114.70	208.0
115.90	718.0
116.90	1149.0
117.90	702.0
118.80	1016.0
124.90	105.0
127.80	575.0
128.80	373.0
129.80	725.0
130.80	306.0
134.90	301.0
136.90	250.0
139.80	136.0
140.90	1774.0
141.80	208.0
142.90	2194.0
143.70	155.0
144.90	549.0
145.80	231.0
146.80	192.0
147.80	439.0
149.90	185.0
151.80	107.0
152.90	147.0
154.80	434.0
155.90	127.0
156.90	262.0
158.90	144.0
160.80	229.0
171.00	287.0
171.90	1644.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155

173.00	1753.0
173.90	139648.0
174.90	10293.0
175.90	135232.0
176.90	8931.0
177.90	269.0

Instrument :
MSVOA_U
ClientSampleId :
BFB155