

Data File : VU032092.D
Acq On : 17 May 2019 09:54
Operator : JC/SP
Sample : K2739-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB885

Quant Time: May 18 01:54:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 18 01:51:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	378069	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	399021	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	160039	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	134318	4.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.20%
7) Chloroethane-d5	1.67	69	118979	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.27	63	188440	3.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.20%
20) 2-Butanone-d5	4.19	46	253140	40.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.98%
24) Chloroform-d	4.64	84	236472	4.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.40%
26) 1,2-Dichloroethane-d4	5.31	65	125287	4.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.80%
32) Benzene-d6	5.33	84	489799	4.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.40%
36) 1,2-Dichloropropane-d6	6.32	67	143489	4.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.60%
41) Toluene-d8	7.56	98	418884	3.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.20%
43) trans-1,3-Dichloropropene-	7.85	79	48723	3.80	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.00%
46) 2-Hexanone-d5	8.31	63	216529	37.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.88%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	121819	4.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.80%
64) 1,2-Dichlorobenzene-d4	11.86	152	156334	4.61	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.20%

Target Compounds

					Qvalue
3) Chloromethane	1.33	50	3458	0.190 ug/L	84
8) Chloroethane	1.68	64	1079	0.091 ug/L #	56
12) 1,1-Dichloroethene	2.27	96	2120	0.140 ug/L #	1
13) Acetone	2.32	43	15252	7.431 ug/L	95
14) Carbon disulfide	2.48	76	5155	0.106 ug/L #	88
17) Methyl tert-butyl Ether	3.00	73	5638	0.158 ug/L #	87
21) 2-Butanone	4.30	43	2926	0.993 ug/L	78
22) cis-1,2-Dichloroethene	4.22	96	9855	0.616 ug/L	94
35) Methylcyclohexane	6.33	83	34280	1.432 ug/L #	20
37) 1,2-Dichloropropane	6.32	63	15350	1.025 ug/L #	88
39) cis-1,3-Dichloropropene	7.22	75	2926	0.141 ug/L #	53
42) Toluene	7.64	91	10842	0.169 ug/L	95
44) trans-1,3-Dichloropropene	7.85	75	1838	0.114 ug/L	99
47) Tetrachloroethene	8.22	164	2976	0.240 ug/L	82
48) 2-Hexanone	8.37	43	8318	1.544 ug/L #	45
49) Dibromochloromethane	8.23	129	2667	0.209 ug/L #	10
59) 1,2,3-Trichloropropane	11.48	75	16260	1.709 ug/L	98

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU051619\
Quantitation Report (Not Reviewed)

Data File : VU032092.D
Acq On : 17 May 2019 09:54
Operator : JC/SP
Sample : K2739-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB885

Quant Time: May 18 01:54:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 18 01:51:41 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU032092.D
Acq On : 17 May 2019 09:54
Operator : JC/SP
Sample : K2739-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB885

Quant Time: May 18 01:54:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 18 01:51:41 2019
Response via : Initial Calibration

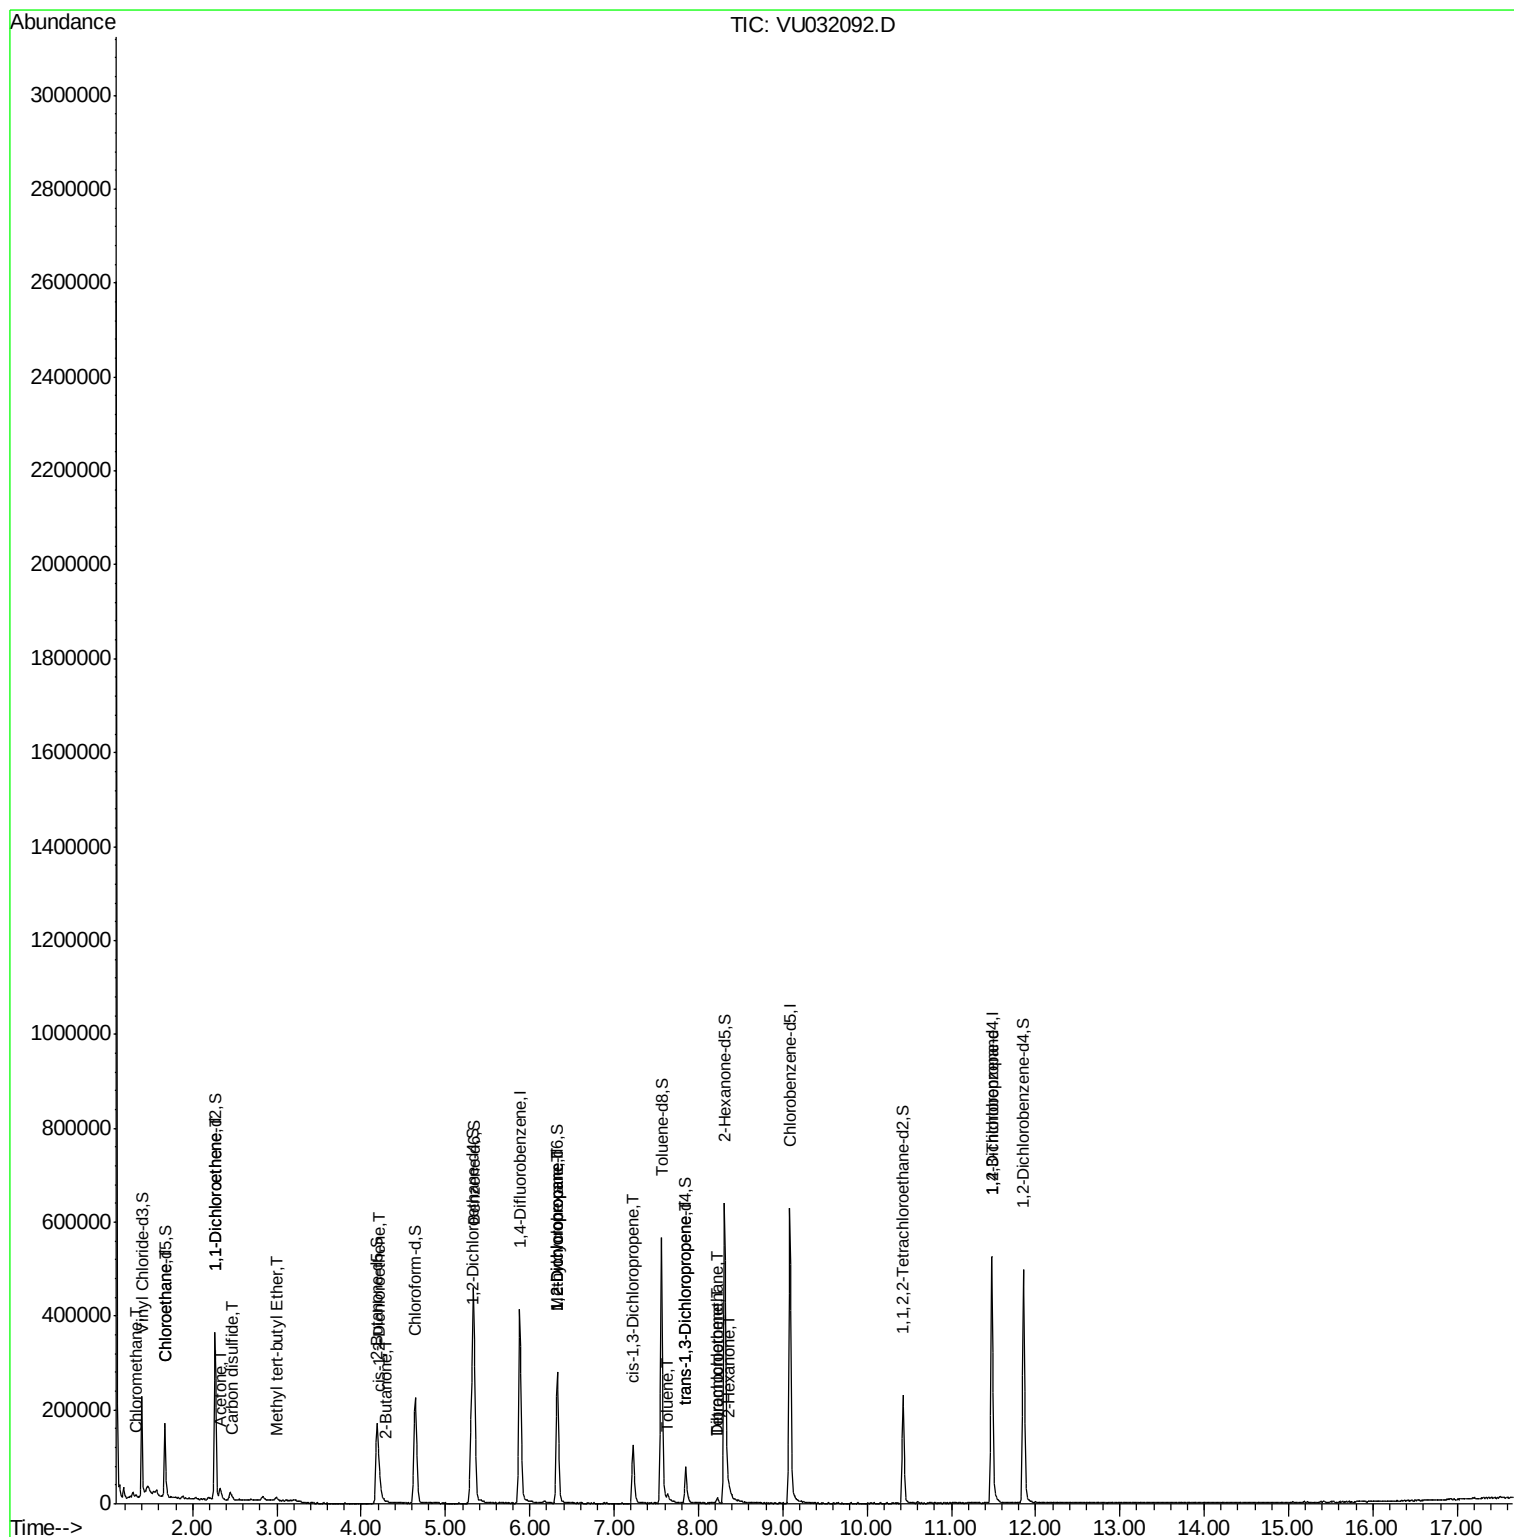

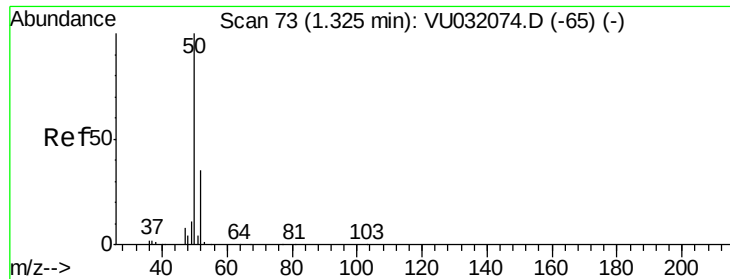

#3

Chloromethane

Concen: 0.190 ug/L

RT: 1.33 min Scan# 74

Delta R.T. 0.00 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54

Instrument :

MSVOA_U

ClientSampleId :


DB885

Tgt Ion: 50 Resp: 3458

Ion Ratio Lower Upper




50 100

52 23.8 23.2 43.0

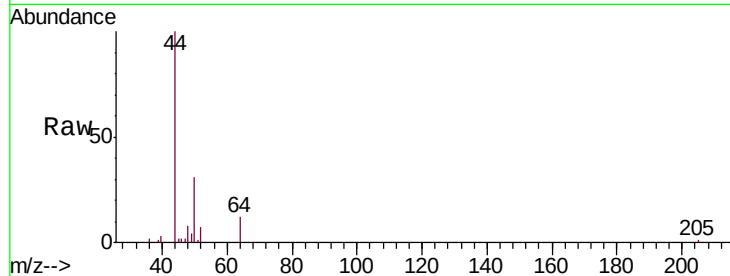

Abundance Ion 50.05 (49.75 to 50.75): VU032074.D (-65) (-)

Ion 52.05 (51.75 to 52.75): VU032092.D (-1) (-)

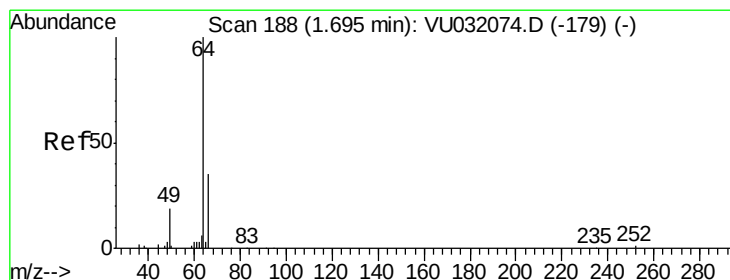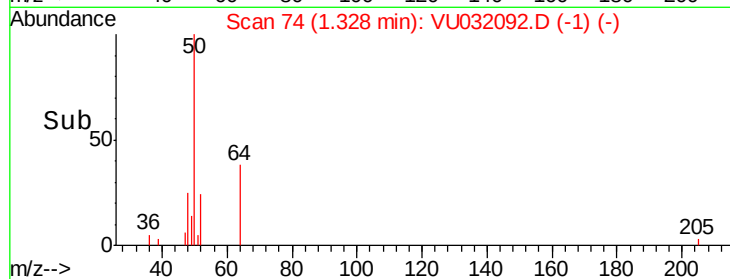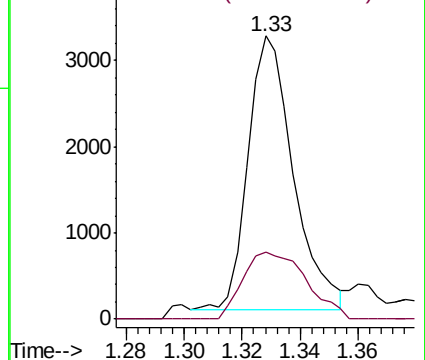

#8

Chloroethane

Concen: 0.091 ug/L

RT: 1.68 min Scan# 182

Delta R.T. -0.02 min

Lab File: VU032092.D


Acq: 17 May 2019 09:54

Tgt Ion: 64 Resp: 1079

Ion Ratio Lower Upper



64 100


66 7.1 22.0 41.0#

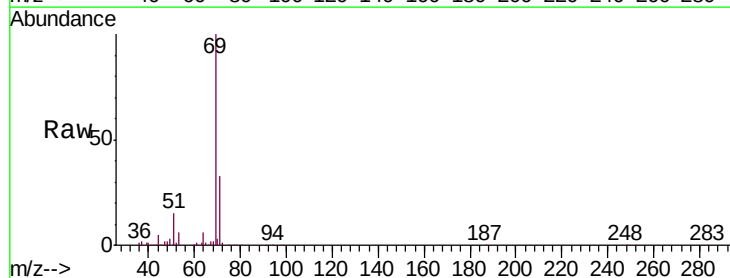

Abundance Ion 64.10 (63.80 to 64.80): VU032074.D (-179) (-)

Ion 66.05 (65.75 to 66.75): VU032092.D (-95) (-)

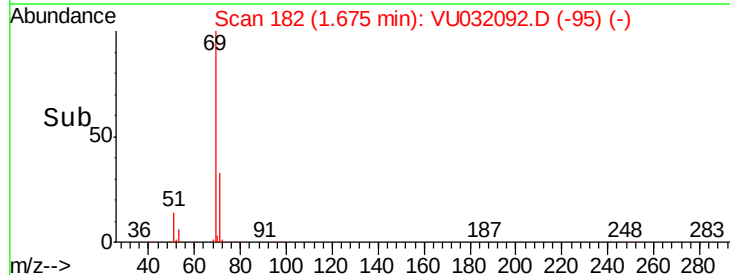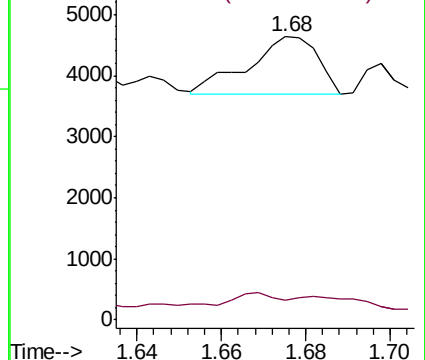

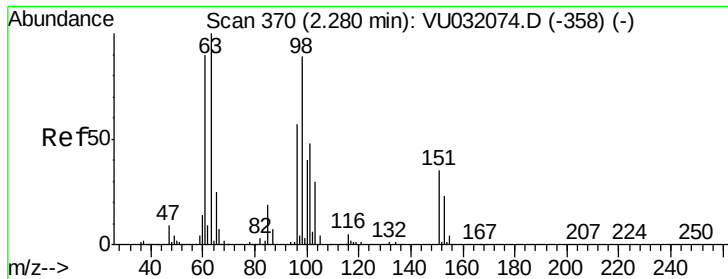

#12

1,1-Dichloroethene

Concen: 0.140 ug/L

RT: 2.27 min Scan# 368

Delta R.T. -0.01 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54

Instrument :

MSVOA_U

ClientSampleId :

DB885





Tgt Ion: 96 Resp: 2120

Ion Ratio Lower Upper

96 100

61 917.4 111.7 207.5#

63 8099.8 152.2 282.6#

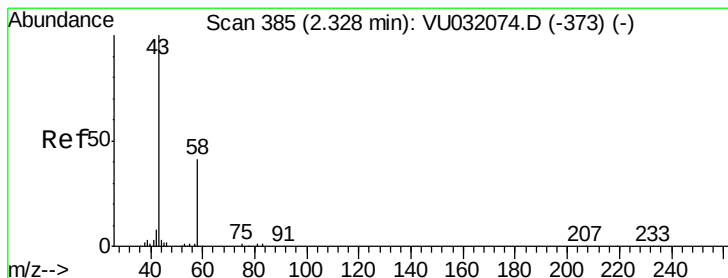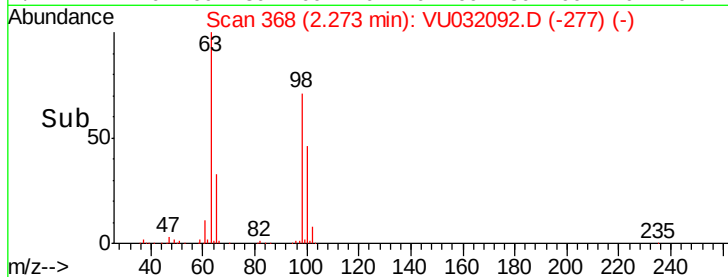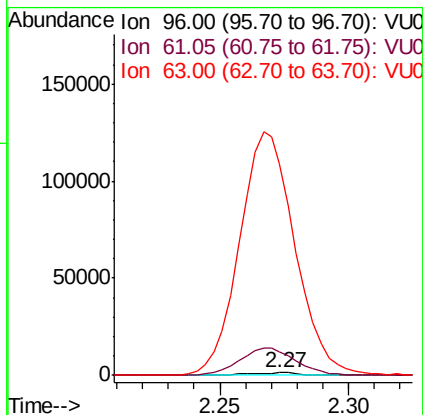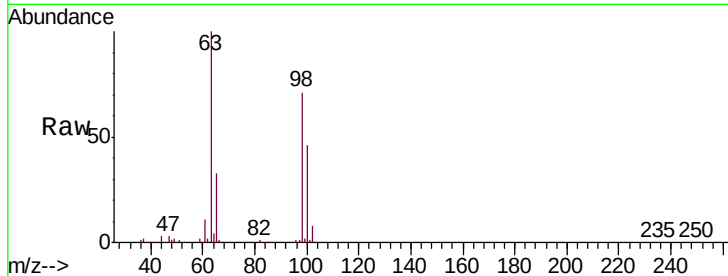

#13

Acetone

Concen: 7.431 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.01 min

Lab File: VU032092.D




Acq: 17 May 2019 09:54


Tgt Ion: 43 Resp: 15252

Ion Ratio Lower Upper

43 100

58 36.2 0.0 78.8

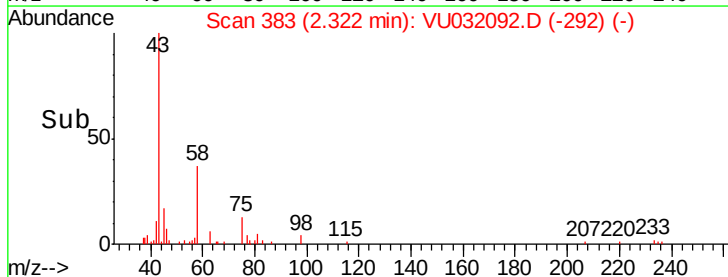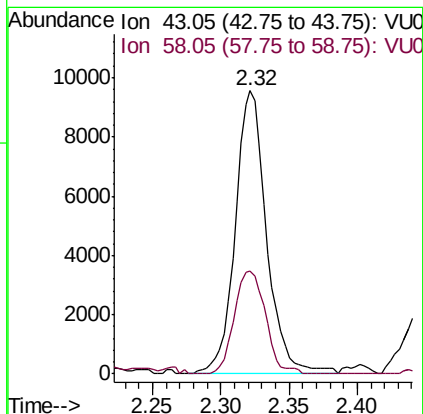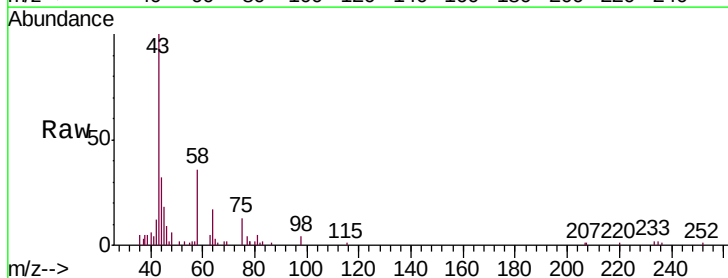

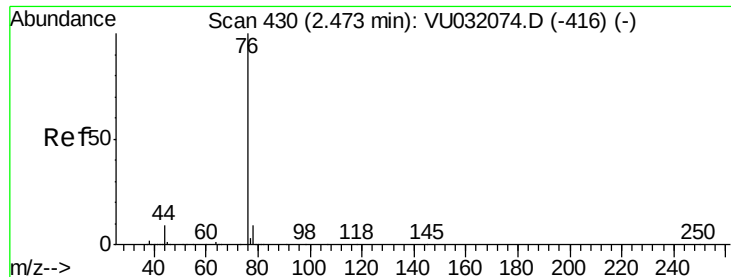

#14

Carbon disulfide

Concen: 0.106 ug/L

RT: 2.48 min Scan# 431

Delta R.T. 0.00 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54

Instrument :

MSVOA_U

ClientSampleId :





DB885

Tgt Ion: 76 Resp: 5155

Ion Ratio Lower Upper

76 100

78 13.9 7.8 11.6#

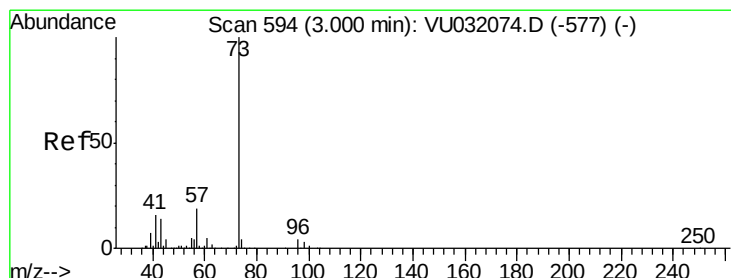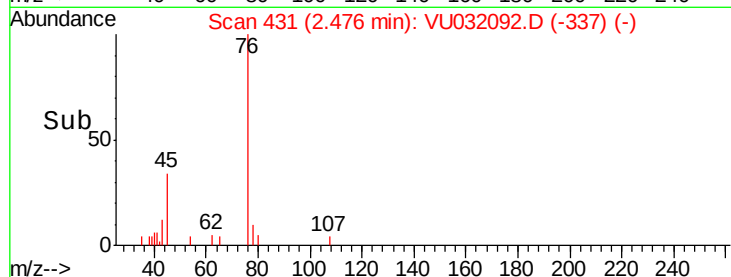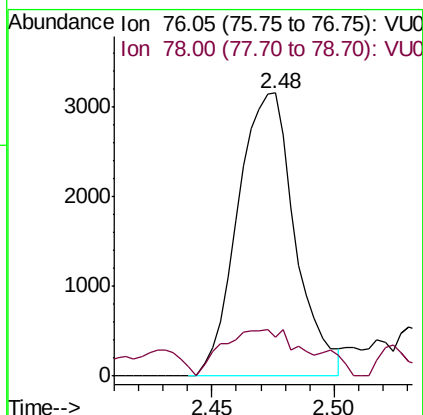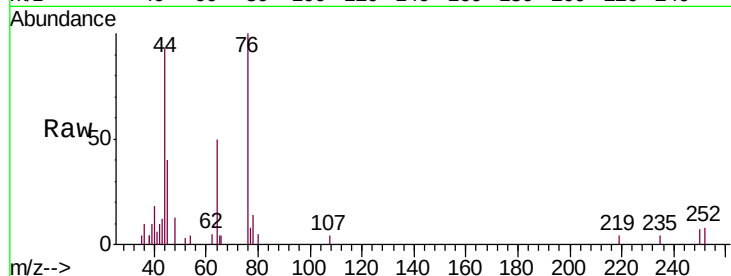

#17

Methyl tert-butyl Ether

Concen: 0.158 ug/L

RT: 3.00 min Scan# 595

Delta R.T. 0.00 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54




Tgt Ion: 73 Resp: 5638


Ion Ratio Lower Upper

73 100

43 20.9 13.0 19.6#

57 15.3 17.9 26.9#

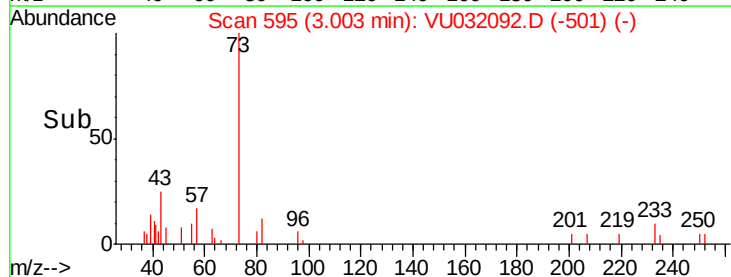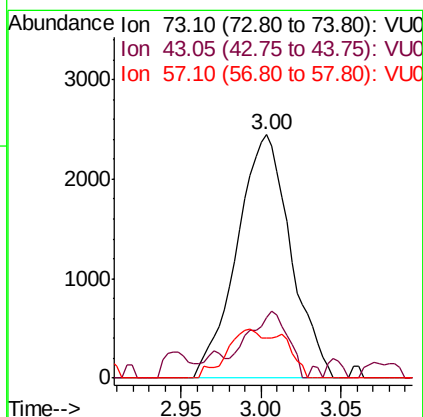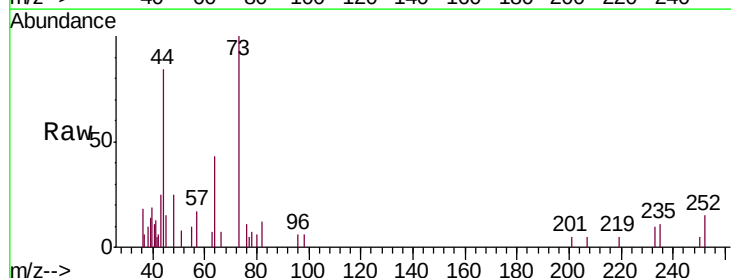

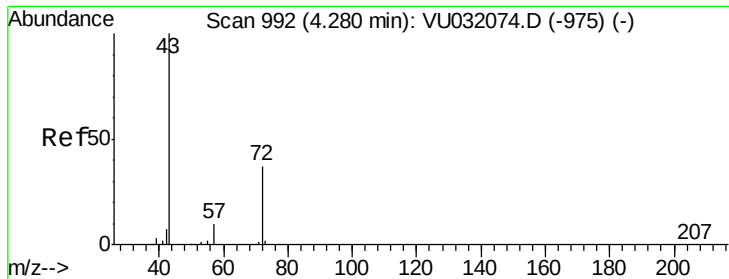

#21

2-Butanone

Concen: 0.993 ug/L

RT: 4.30 min Scan# 999

Delta R.T. 0.02 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54

Instrument :

MSVOA_U

ClientSampleId :





DB885

Tgt Ion: 43 Resp: 2926

Ion Ratio Lower Upper

43 100

72 20.9 16.8 50.3

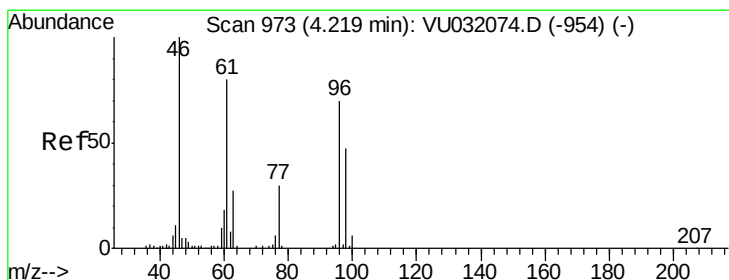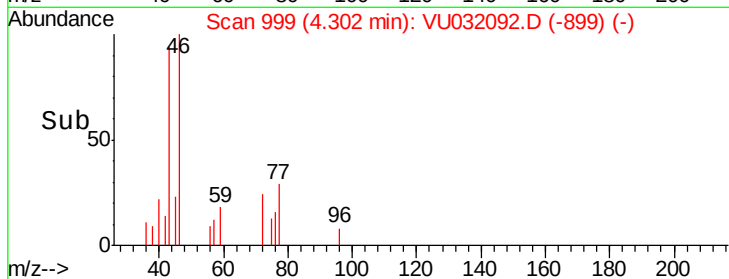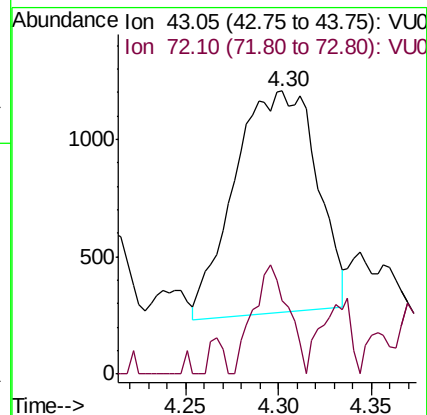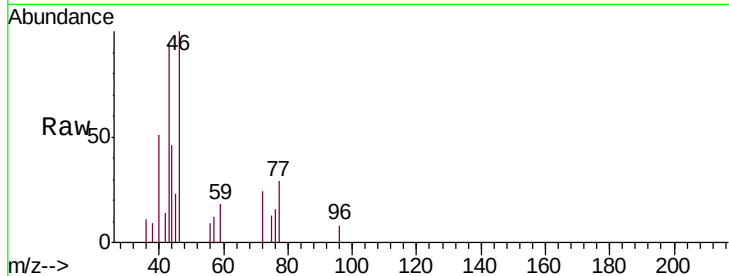

#22

cis-1,2-Dichloroethene

Concen: 0.616 ug/L

RT: 4.22 min Scan# 973

Delta R.T. 0.00 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54




Tgt Ion: 96 Resp: 9855


Ion Ratio Lower Upper

96 100

61 116.4 85.8 159.4

68 0.0 0.0 0.0


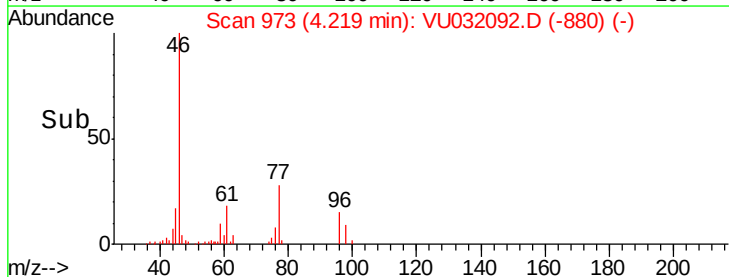
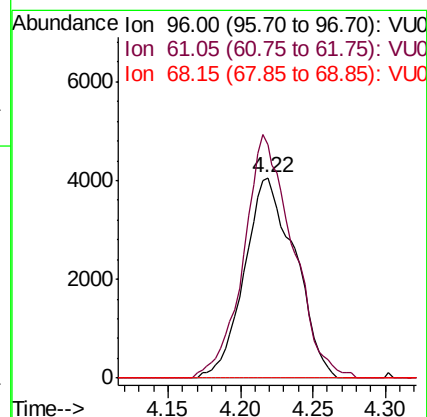
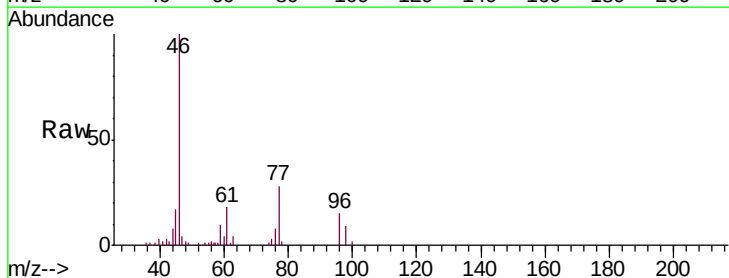


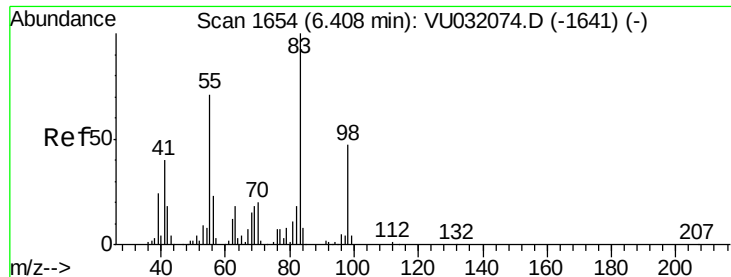

#35
Methylcyclohexane
Concen: 1.432 ug/L
RT: 6.33 min Scan# 1629
Delta R.T. -0.08 min
Lab File: VU032092.D
Acq: 17 May 2019 09:54




Instrument :
MSVOA_U
ClientSampleId :
DB885


Tgt Ion: 83 Resp: 34280
Ion Ratio Lower Upper
83 100
55 0.1 59.7 89.5#
98 2.0 36.8 55.2#

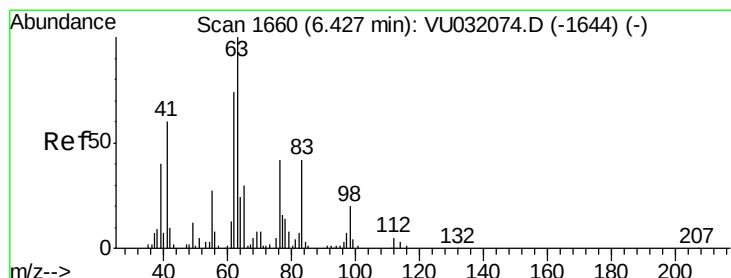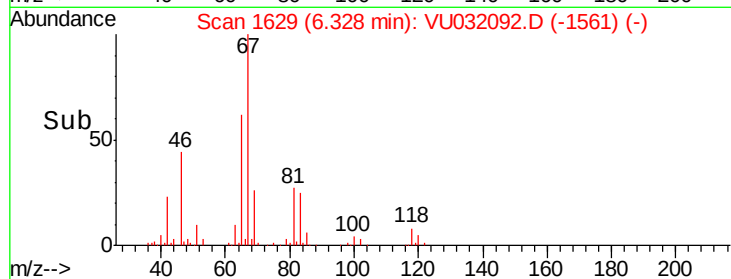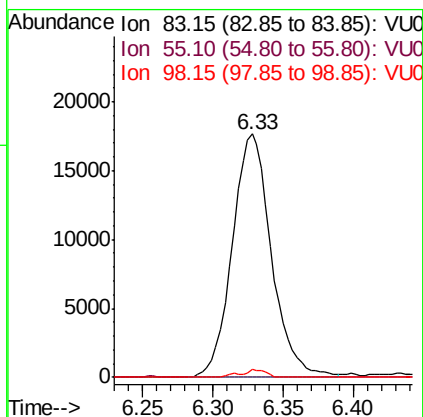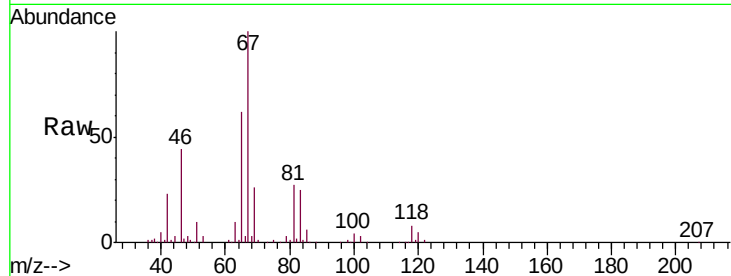

#37
1,2-Dichloropropane
Concen: 1.025 ug/L
RT: 6.32 min Scan# 1628
Delta R.T. -0.10 min
Lab File: VU032092.D
Acq: 17 May 2019 09:54

Tgt Ion: 63 Resp: 15350
Ion Ratio Lower Upper
63 100
112 0.8 3.8 5.6#

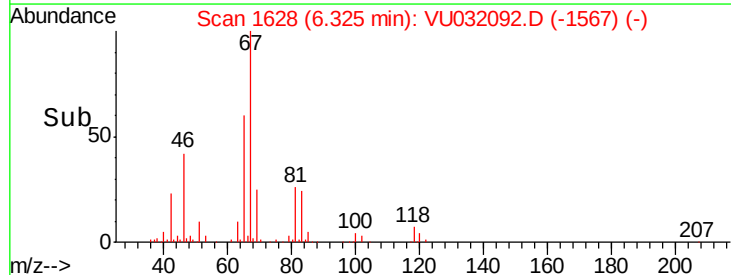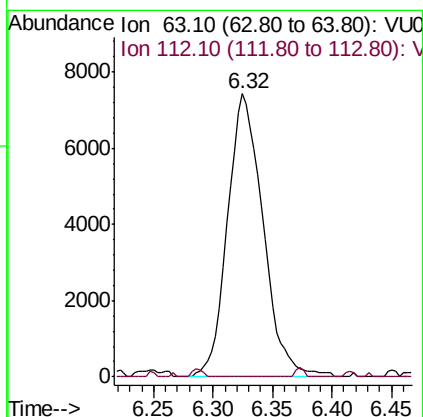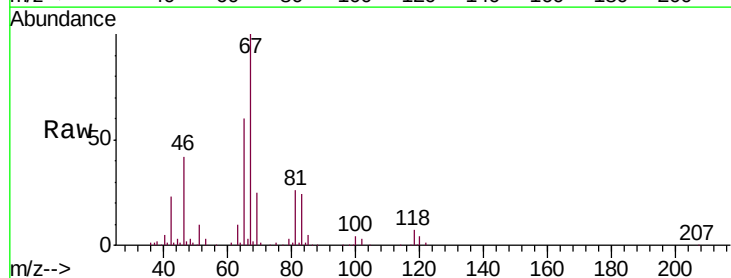

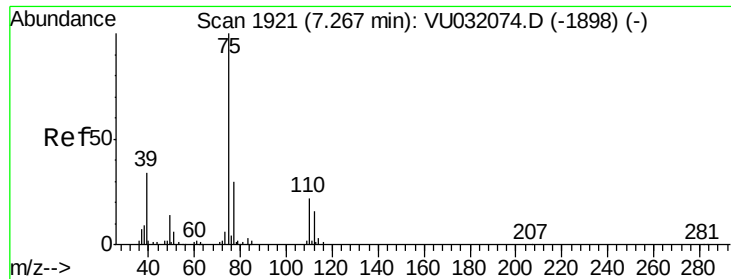

#39

cis-1,3-Dichloropropene

Concen: 0.141 ug/L

RT: 7.22 min Scan# 1908

Delta R.T. -0.04 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54

Instrument :

MSVOA_U

ClientSampleId :





DB885

Tgt Ion: 75 Resp: 2926

Ion Ratio Lower Upper

75 100

77 56.7 21.7 40.3#

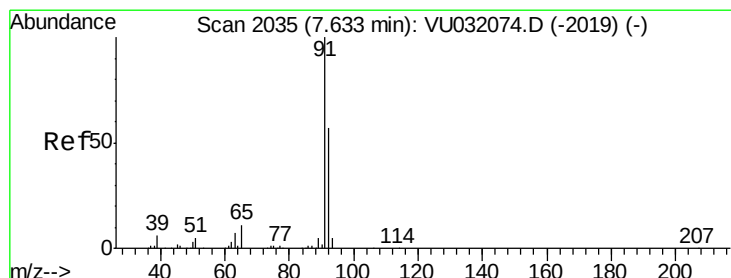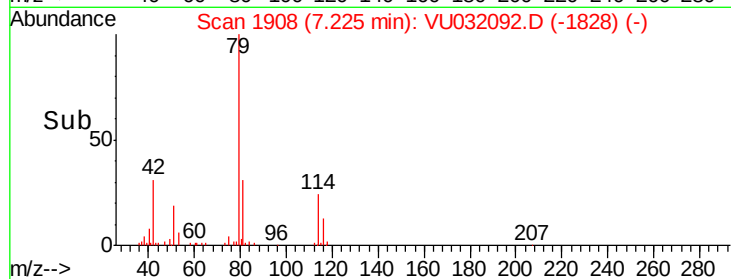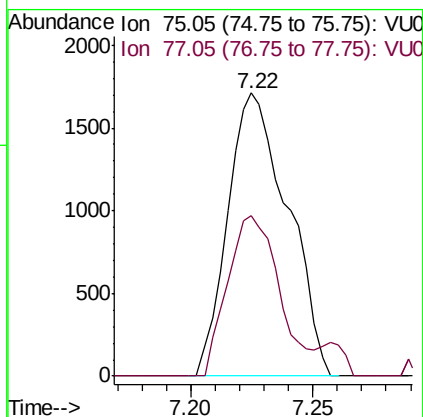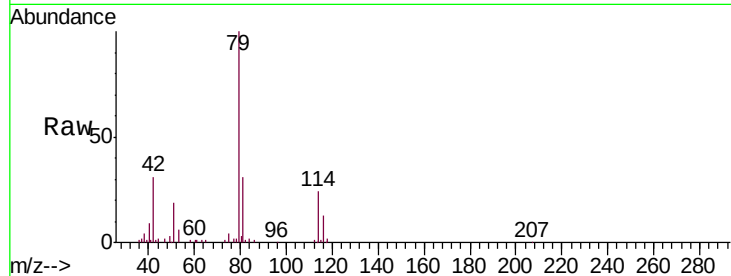

#42

Toluene

Concen: 0.169 ug/L

RT: 7.64 min Scan# 2036

Delta R.T. 0.00 min

Lab File: VU032092.D




Acq: 17 May 2019 09:54


Tgt Ion: 91 Resp: 10842

Ion Ratio Lower Upper

91 100

92 61.0 40.2 74.6

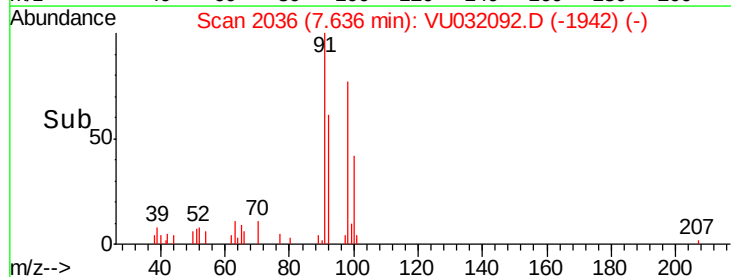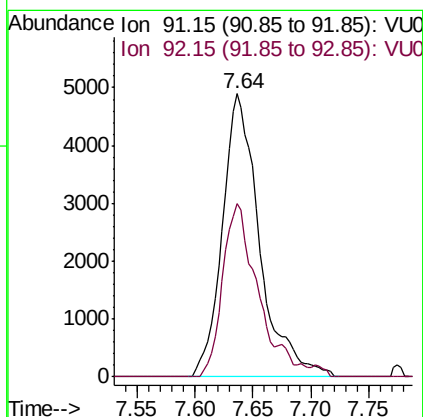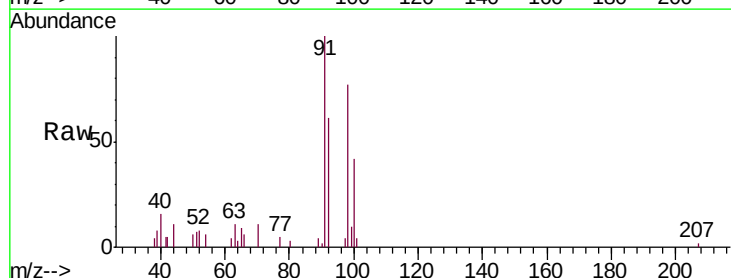

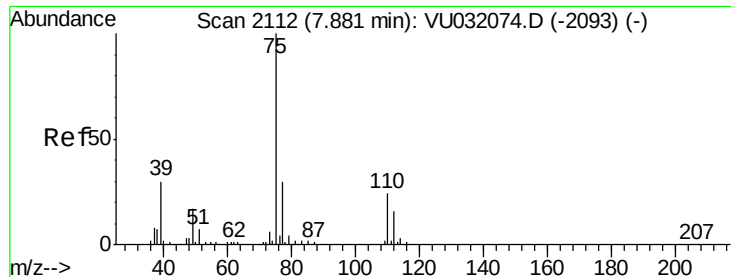

#44

trans-1,3-Dichloropropene

Concen: 0.114 ug/L

RT: 7.85 min Scan# 2103

Delta R.T. -0.03 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54

Instrument :

MSVOA_U

ClientSampleId :


DB885

Tgt Ion: 75 Resp: 1838

Ion Ratio Lower Upper

75 100

77 30.7 21.0 39.0

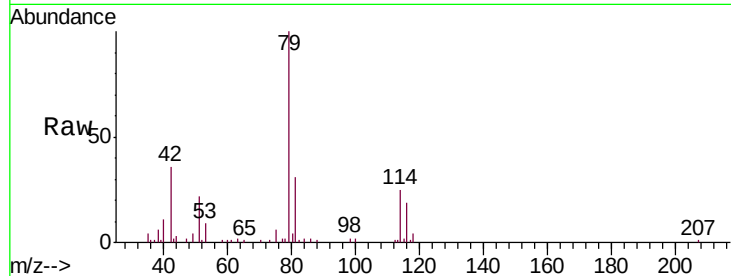

Abundance Ion 75.05 (74.75 to 75.75): VU032074.D (-2093) (-)

Ion 77.05 (76.75 to 77.75): VU032074.D (-2093) (-)

7.85

1500



1000

500

0

7.80 7.85 7.90

Time-->

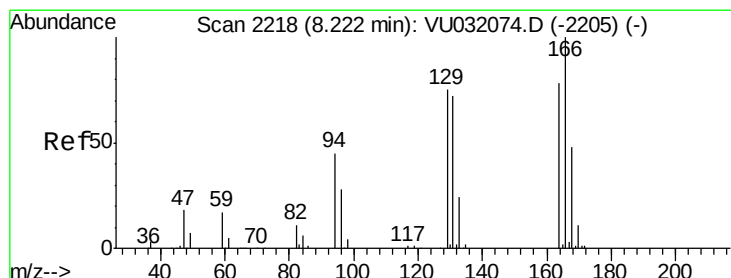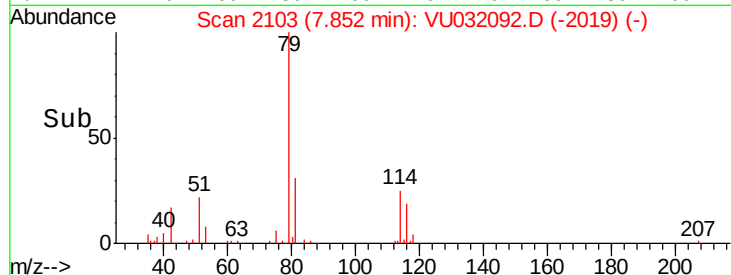

#47

Tetrachloroethene

Concen: 0.240 ug/L

RT: 8.22 min Scan# 2219

Delta R.T. 0.00 min

Lab File: VU032092.D

Acq: 17 May 2019 09:54

Tgt Ion: 164 Resp: 2976


Ion Ratio Lower Upper

164 100

129 77.7 70.3 130.5

131 86.4 64.5 119.9

166 104.3 92.3 171.5

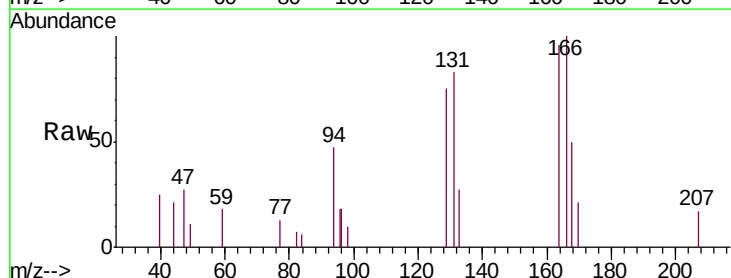

Abundance Ion 163.90 (163.60 to 164.60): VU032074.D (-2205) (-)

Ion 128.95 (128.65 to 129.65): VU032074.D (-2205) (-)

Ion 130.95 (130.65 to 131.65): VU032074.D (-2205) (-)

Ion 165.90 (165.60 to 166.60): VU032074.D (-2205) (-)

3000

2500

2000

1500


1000


500

0

8.20 8.25

Time-->




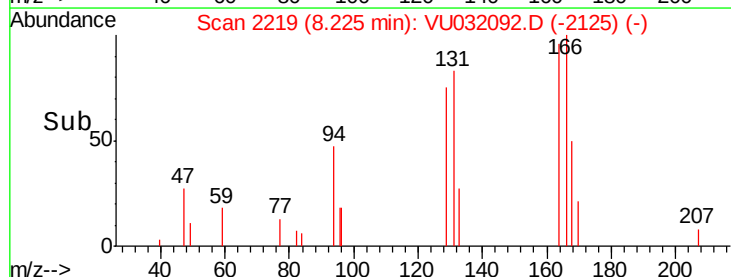


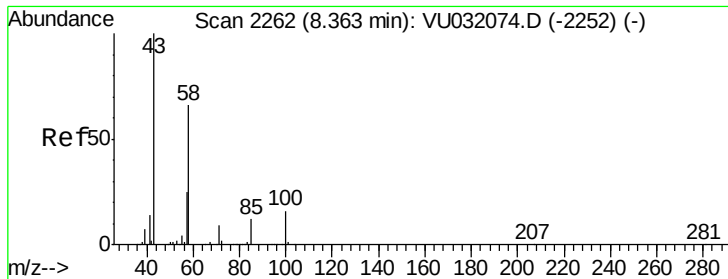

#48
2-Hexanone
Concen: 1.544 ug/L
RT: 8.37 min Scan# 2263
Delta R.T. 0.00 min
Lab File: VU032092.D
Acq: 17 May 2019 09:54




Instrument :
MSVOA_U
ClientSampleId :
DB885


Tgt Ion: 43 Resp: 8318
Ion Ratio Lower Upper
43 100
58 0.0 51.6 77.4#
57 18.2 18.4 27.6#
100 10.5 12.2 18.4#

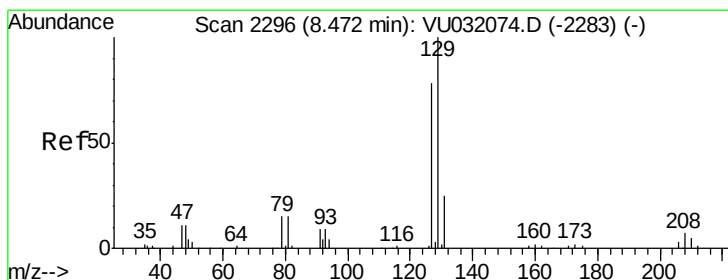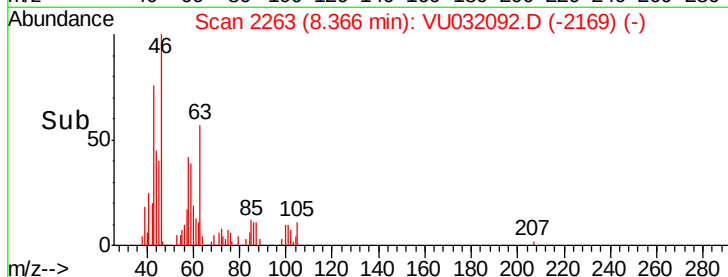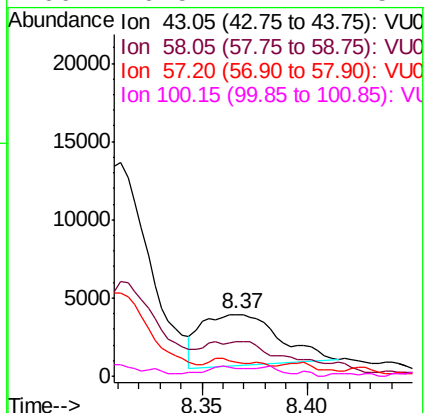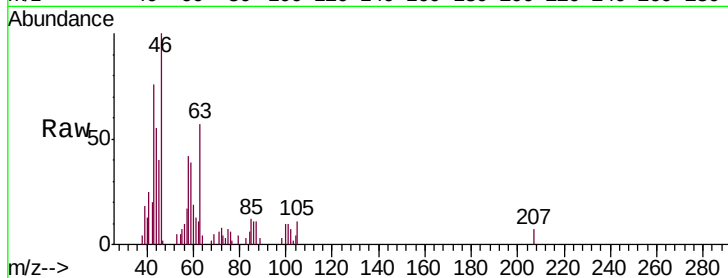

#49
Dibromochloromethane
Concen: 0.209 ug/L
RT: 8.23 min Scan# 2220
Delta R.T. -0.24 min
Lab File: VU032092.D
Acq: 17 May 2019 09:54

Tgt Ion: 129 Resp: 2667
Ion Ratio Lower Upper
129 100
127 0.0 55.2 102.6#

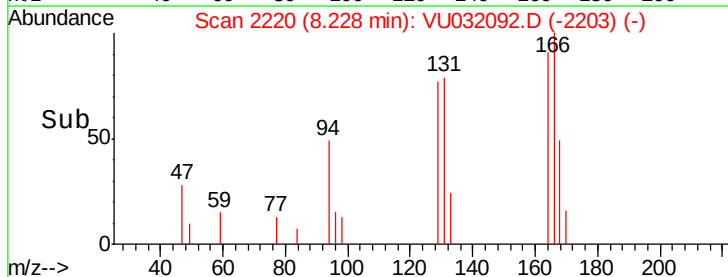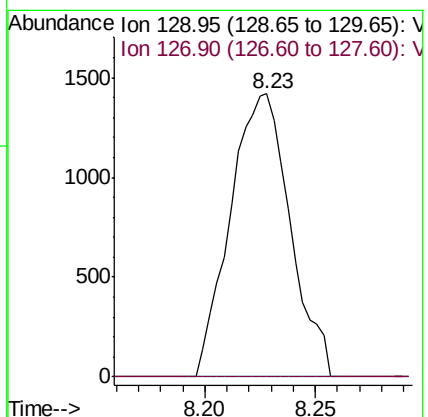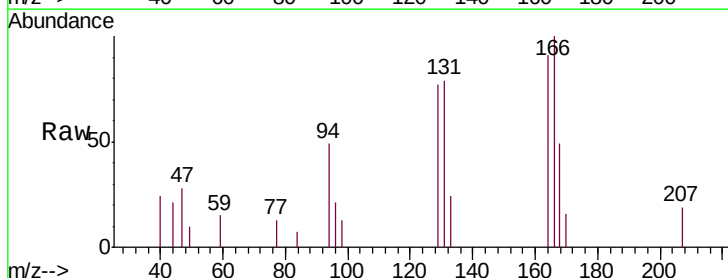

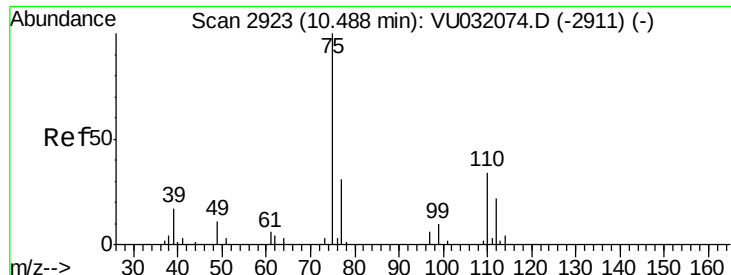

#59
 1,2,3-Trichloropropane
 Concen: 1.709 ug/L
 RT: 11.48 min Scan# 3231
 Delta R.T. 0.99 min
 Lab File: VU032092.D
 Acq: 17 May 2019 09:54

Instrument :
 MSVOA_U
 ClientSampleId :
 DB885

Tgt Ion: 75 Resp: 16260
 Ion Ratio Lower Upper
 75 100
 77 33.7 26.2 39.2

