

Data File : VU032097.D
Acq On : 17 May 2019 11:59
Operator : JC/SP
Sample : K2859-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9W47

Quant Time: May 18 01:55:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 18 01:51:41 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	369564	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	380862	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	144986	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	136318	4.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.60%
7) Chloroethane-d5	1.67	69	117878	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.27	63	195327	3.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.80%
20) 2-Butanone-d5	4.19	46	255288	41.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.54%
24) Chloroform-d	4.64	84	247178	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
26) 1,2-Dichloroethane-d4	5.30	65	121185	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
32) Benzene-d6	5.33	84	500368	4.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.20%
36) 1,2-Dichloropropane-d6	6.32	67	146606	4.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.40%
41) Toluene-d8	7.56	98	433342	4.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.60%
43) trans-1,3-Dichloropropene-	7.85	79	44711	3.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.20%
46) 2-Hexanone-d5	8.31	63	210193	38.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.14%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	120097	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	152405	4.96	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.20%

Target Compounds


					Qvalue
3) Chloromethane	1.33	50	4549	0.256	ug/L 93
13) Acetone	2.32	43	66230	33.009	ug/L 98
15) Methyl Acetate	2.45	43	3477	0.604	ug/L # 43
16) Methylene chloride	2.69	84	21956	1.239	ug/L 93
21) 2-Butanone	4.29	43	4926	1.710	ug/L 72
25) Chloroform	4.67	83	149662	5.554	ug/L 99
27) 1,2-Dichloroethane	5.33	62	2356	0.151	ug/L # 73
35) Methylcyclohexane	6.32	83	35839	1.569	ug/L # 21
37) 1,2-Dichloropropane	6.32	63	15680	1.097	ug/L # 89
38) Bromodichloromethane	6.76	83	42972	2.350	ug/L 96
42) Toluene	7.64	91	11319	0.185	ug/L 91
48) 2-Hexanone	8.38	43	5303	1.031	ug/L # 87
59) 1,2,3-Trichloropropane	11.48	75	15417	1.698	ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU032097.D
Acq On : 17 May 2019 11:59
Operator : JC/SP
Sample : K2859-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9W47

Quant Time: May 18 01:55:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 18 01:51:41 2019
Response via : Initial Calibration

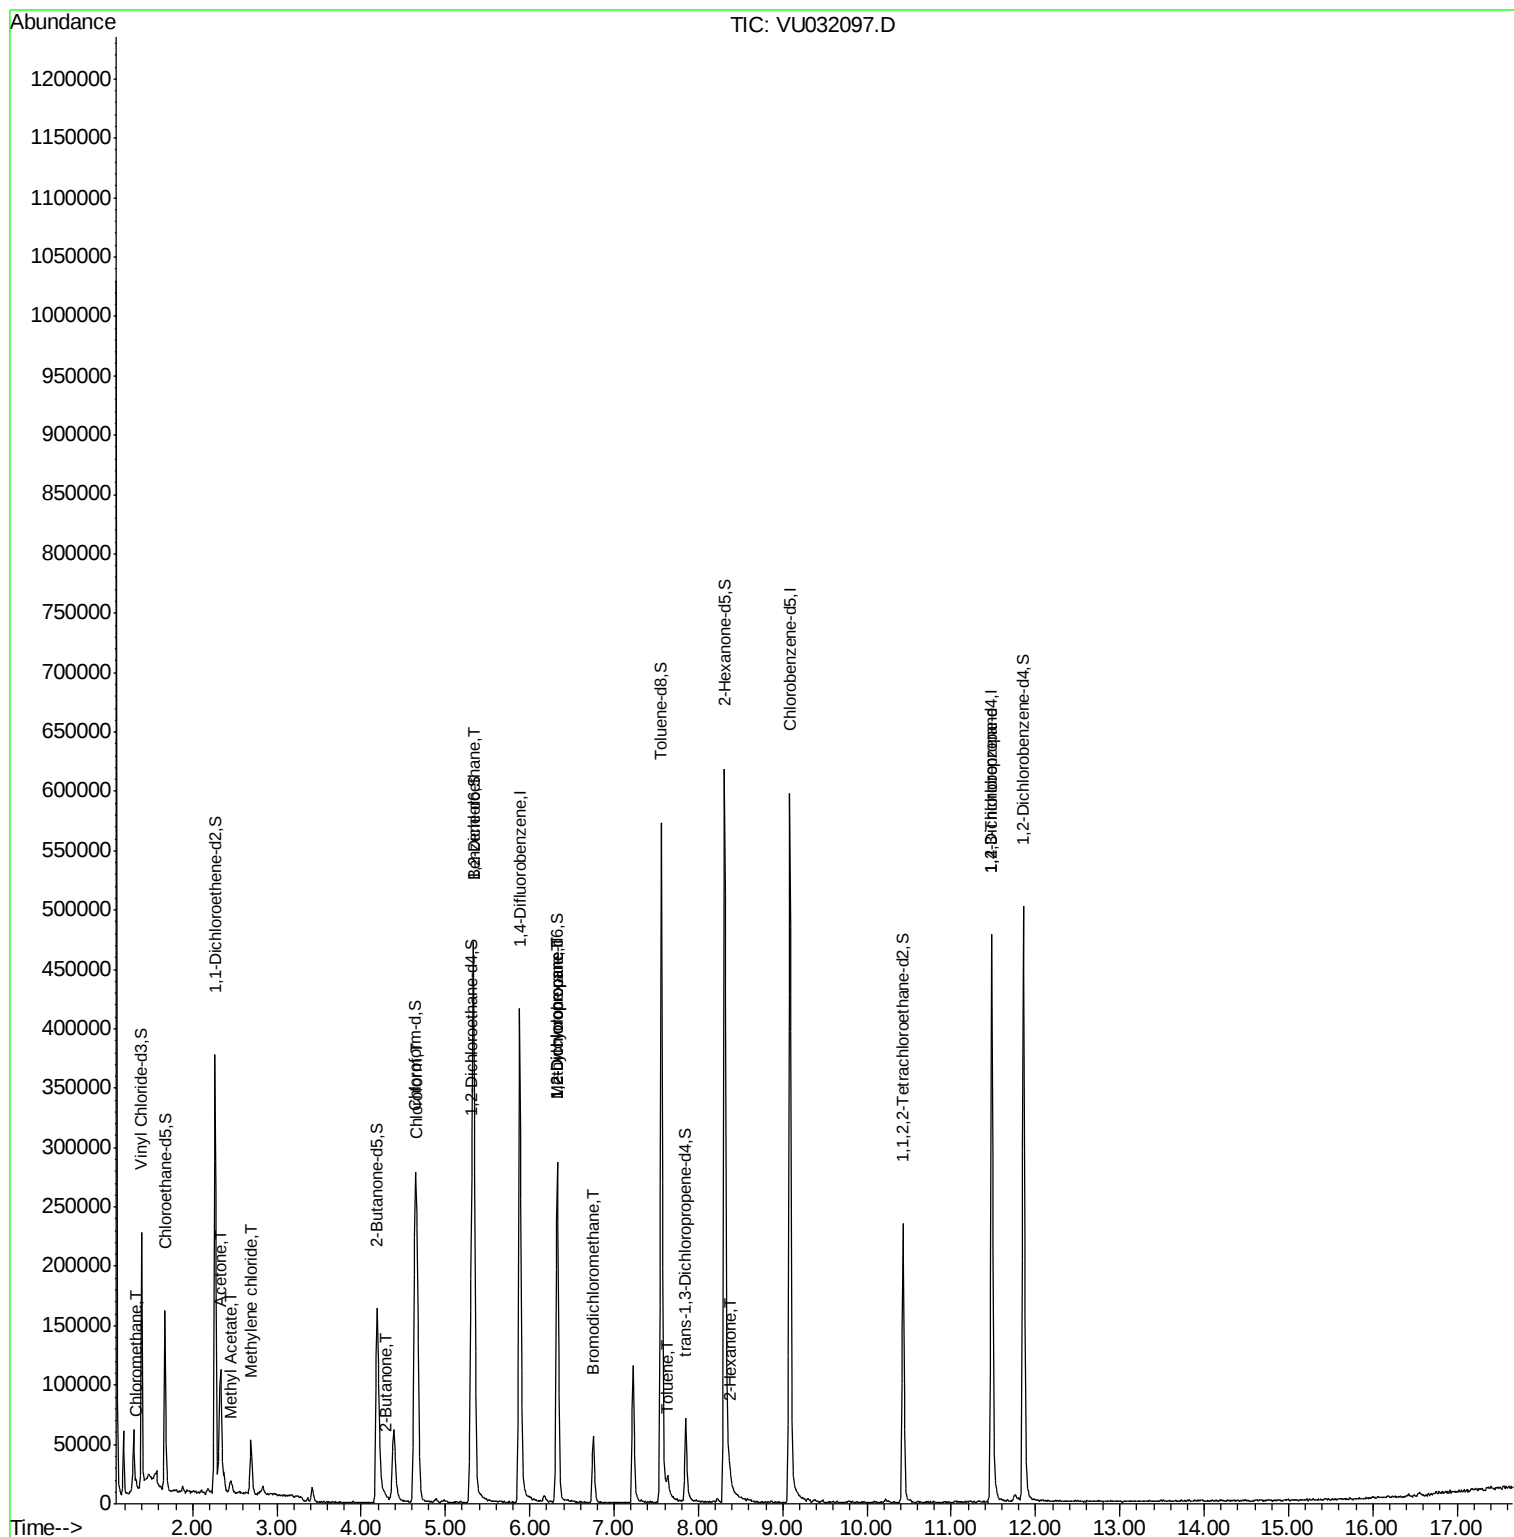



#3

Chloromethane

Concen: 0.256 ug/L

RT: 1.33 min Scan# 74

Delta R.T. 0.00 min

Lab File: VU032097.D

Acq: 17 May 2019 11:59

Instrument :

MSVOA_U

ClientSampled :





F9W47

Tgt Ion: 50 Resp: 4549

Ion Ratio Lower Upper

50 100

52 36.9 23.2 43.0

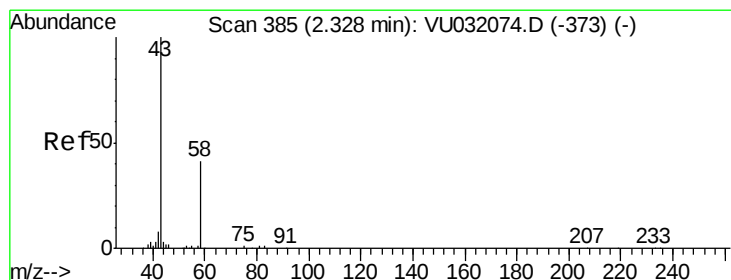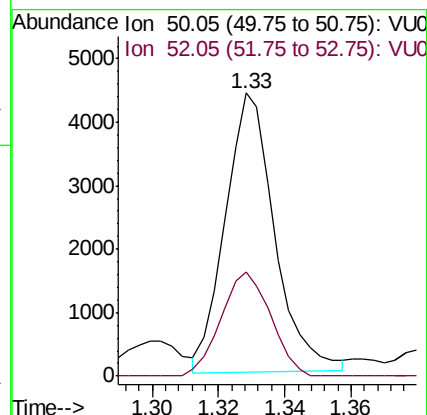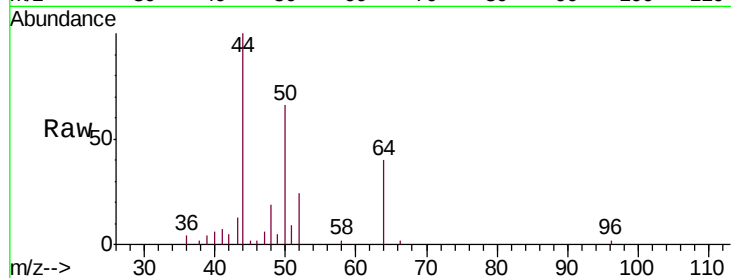

#13

Acetone

Concen: 33.009 ug/L

RT: 2.32 min Scan# 383

Delta R.T. -0.01 min

Lab File: VU032097.D




Acq: 17 May 2019 11:59


Tgt Ion: 43 Resp: 66230

Ion Ratio Lower Upper

43 100

58 38.1 0.0 78.8

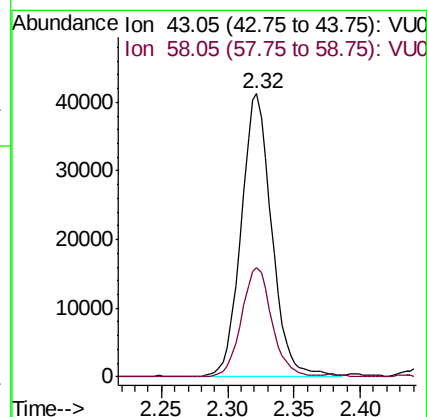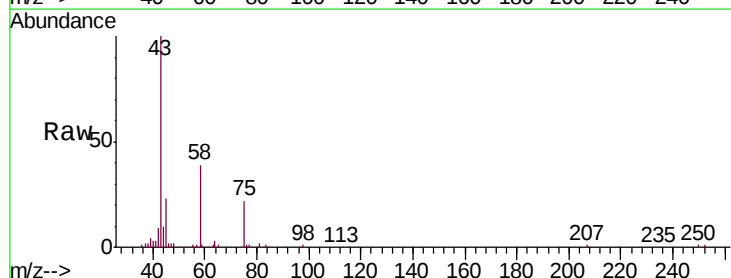

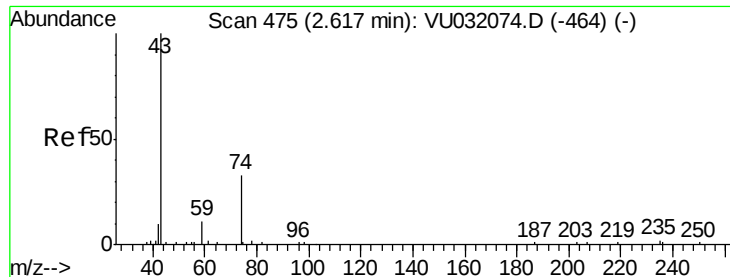

#15

Methyl Acetate

Concen: 0.604 ug/L

RT: 2.45 min Scan# 423

Delta R.T. -0.17 min

Lab File: VU032097.D

Acq: 17 May 2019 11:59

Instrument :

MSVOA_U

ClientSampleId :


F9W47

Tgt Ion: 43 Resp: 3477

Ion Ratio Lower Upper




43 100

74 0.6 26.4 39.6#

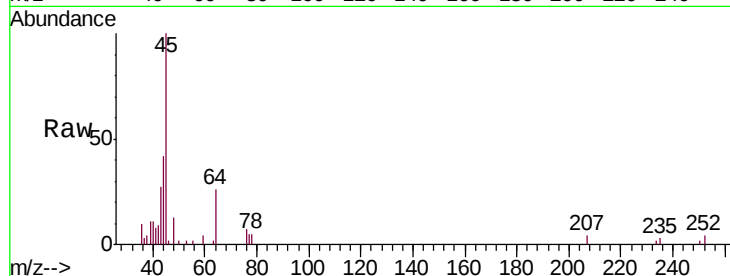

Abundance Ion 43.05 (42.75 to 43.75): VU032097.D (-464) (-)

Ion 74.05 (73.75 to 74.75): VU032097.D (-464) (-)

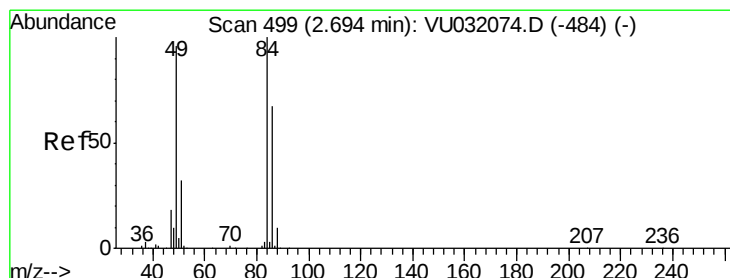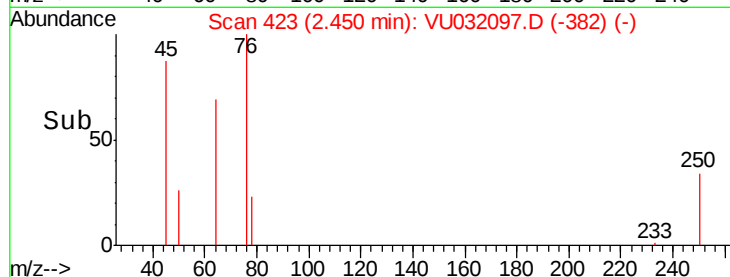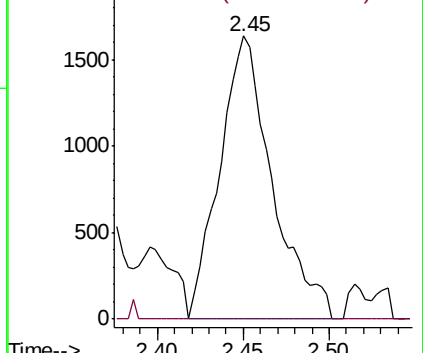

#16

Methylene chloride

Concen: 1.239 ug/L

RT: 2.69 min Scan# 499

Delta R.T. 0.00 min

Lab File: VU032097.D

Acq: 17 May 2019 11:59


Tgt Ion: 84 Resp: 21956

Ion Ratio Lower Upper

84 100

86 65.3 43.1 80.1



49 89.1 67.7 125.7

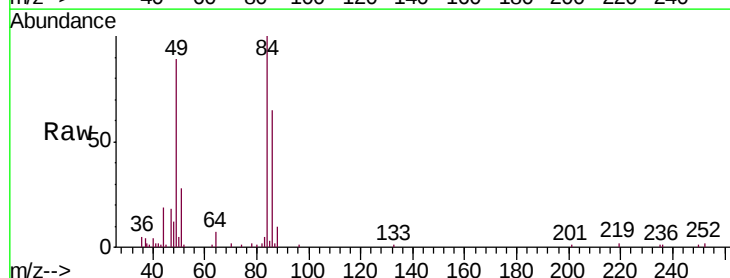


Abundance Ion 84.05 (83.75 to 84.75): VU032097.D (-484) (-)

Ion 86.00 (85.70 to 86.70): VU032097.D (-484) (-)

Ion 49.10 (48.80 to 49.80): VU032097.D (-484) (-)

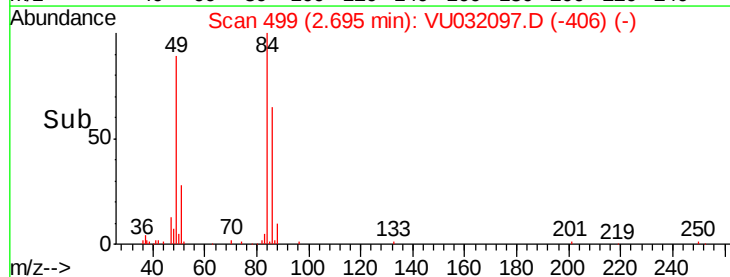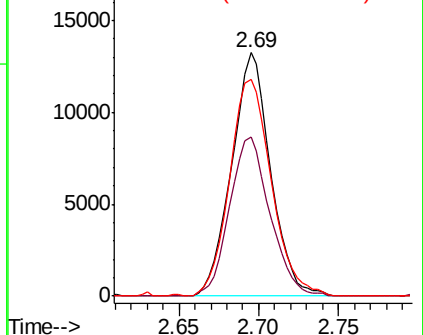

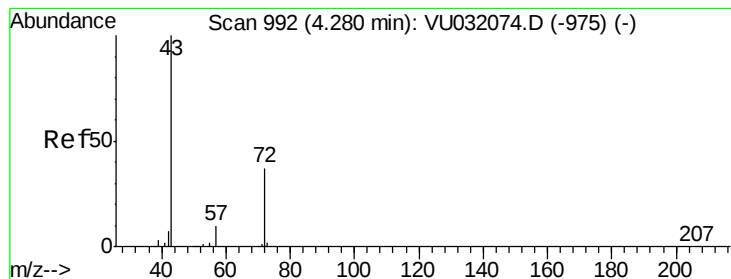

#21

2-Butanone

Concen: 1.710 ug/L

RT: 4.29 min Scan# 996

Delta R.T. 0.01 min

Lab File: VU032097.D

Acq: 17 May 2019 11:59

Instrument :

MSVOA_U

ClientSampleId :


F9W47

Tgt Ion: 43 Resp: 4926

Ion Ratio Lower Upper




43 100

72 17.4 16.8 50.3

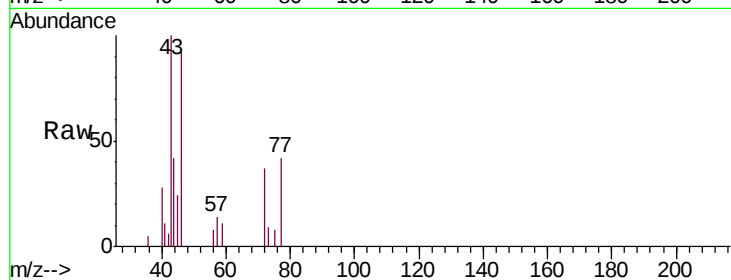

Abundance Ion 43.05 (42.75 to 43.75): VU032097.D (-996) (-)

Ion 72.10 (71.80 to 72.80): VU032097.D (-996) (-)

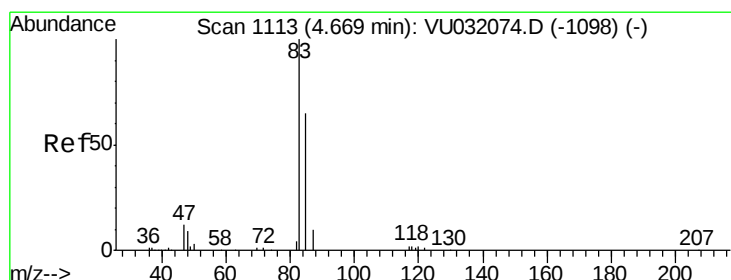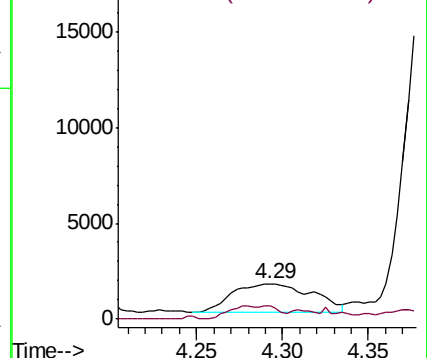

#25

Chloroform

Concen: 5.554 ug/L

RT: 4.67 min Scan# 1112

Delta R.T. -0.00 min

Lab File: VU032097.D


Acq: 17 May 2019 11:59

Tgt Ion: 83 Resp: 149662

Ion Ratio Lower Upper



83 100


85 65.1 44.9 83.3

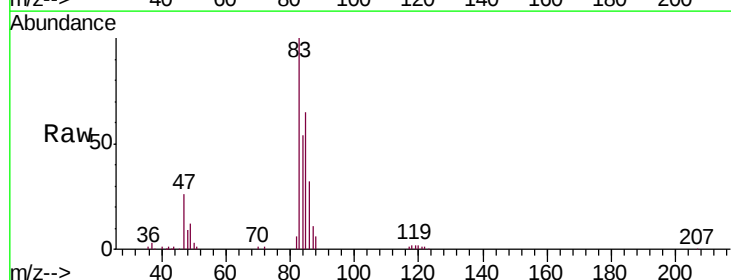

Abundance Ion 83.05 (82.75 to 83.75): VU032097.D (-1112) (-)

Ion 85.00 (84.70 to 85.70): VU032097.D (-1112) (-)




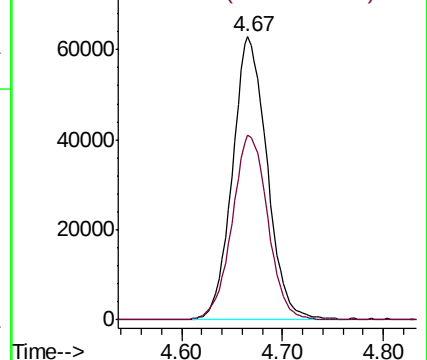




#27
 1,2-Dichloroethane
 Concen: 0.151 ug/L
 RT: 5.33 min Scan# 1319
 Delta R.T. -0.07 min
 Lab File: VU032097.D
 Acq: 17 May 2019 11:59




Instrument :
 MSVOA_U
 ClientSampled :
 F9W47


Tgt Ion: 62 Resp: 2356
 Ion Ratio Lower Upper
 62 100
 98 0.0 8.0 12.0#

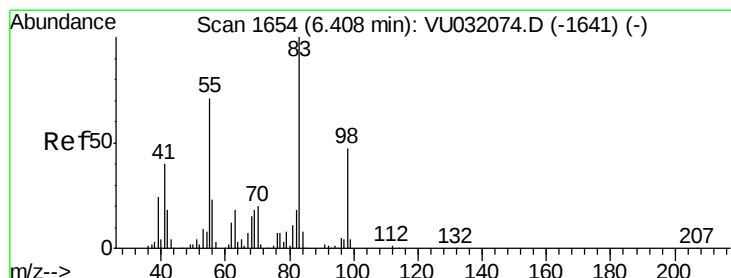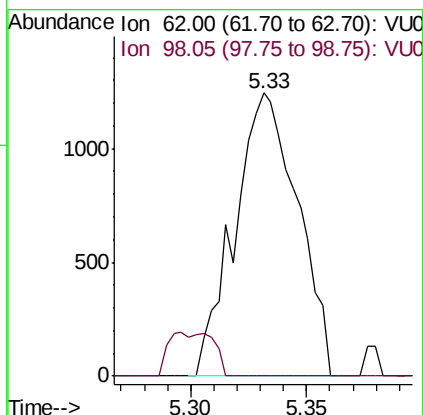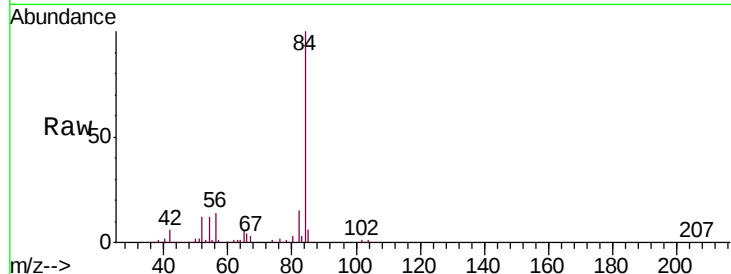

#35
 Methylcyclohexane
 Concen: 1.569 ug/L
 RT: 6.32 min Scan# 1628
 Delta R.T. -0.08 min
 Lab File: VU032097.D
 Acq: 17 May 2019 11:59

Tgt Ion: 83 Resp: 35839
 Ion Ratio Lower Upper
 83 100
 55 0.4 59.7 89.5#
 98 2.0 36.8 55.2#



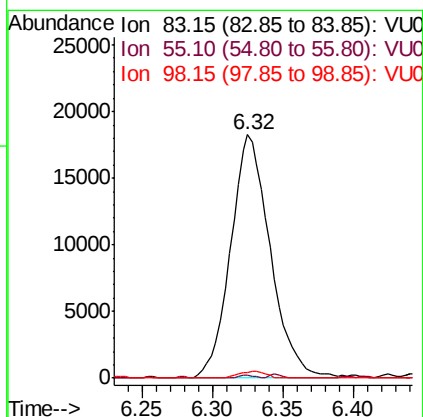
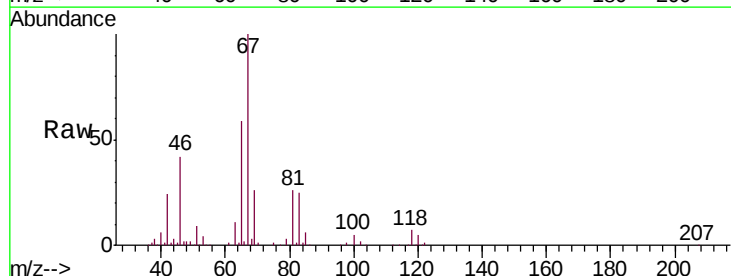


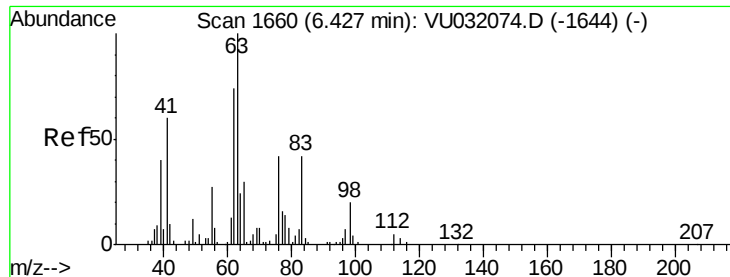

#37
 1,2-Dichloropropane
 Concen: 1.097 ug/L
 RT: 6.32 min Scan# 1628
 Delta R.T. -0.10 min
 Lab File: VU032097.D
 Acq: 17 May 2019 11:59




Instrument :
 MSVOA_U
 ClientSampleId :
 F9W47


Tgt Ion: 63 Resp: 15680
 Ion Ratio Lower Upper
 63 100
 112 0.9 3.8 5.6#

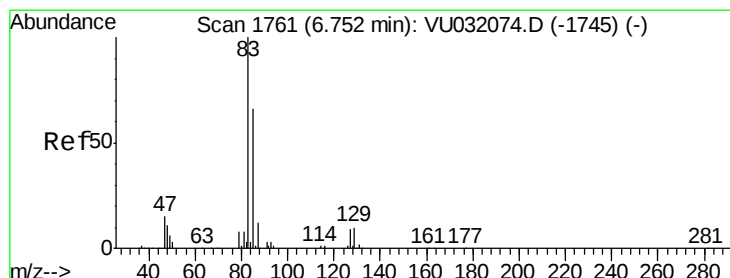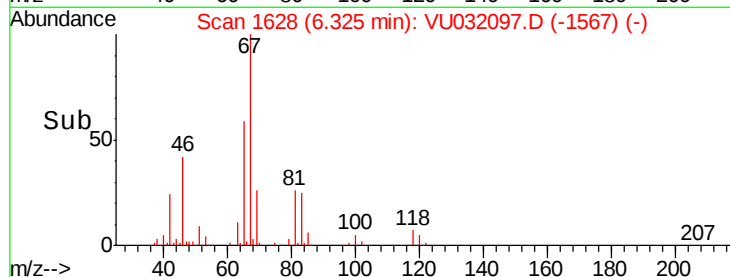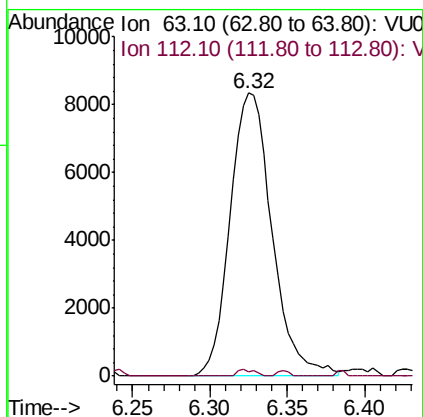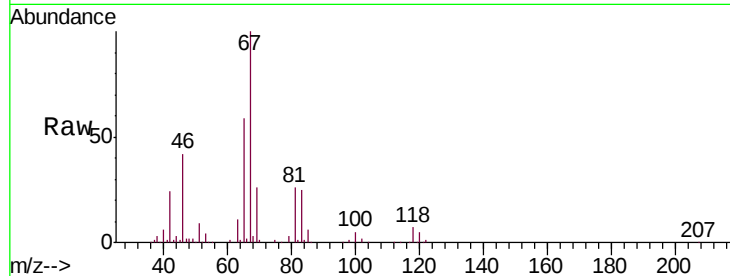

#38
 Bromodichloromethane
 Concen: 2.350 ug/L
 RT: 6.76 min Scan# 1762
 Delta R.T. 0.00 min
 Lab File: VU032097.D
 Acq: 17 May 2019 11:59

Tgt Ion: 83 Resp: 42972
 Ion Ratio Lower Upper
 83 100
 85 61.5 45.5 84.5
 127 9.3 6.3 9.5

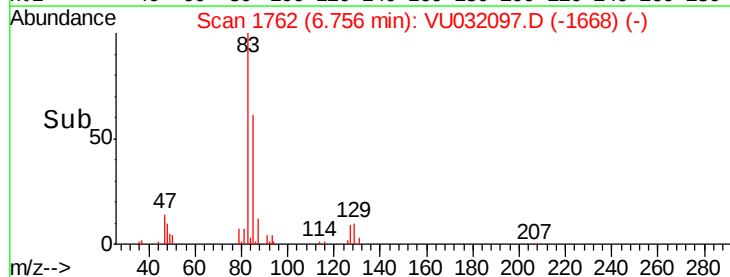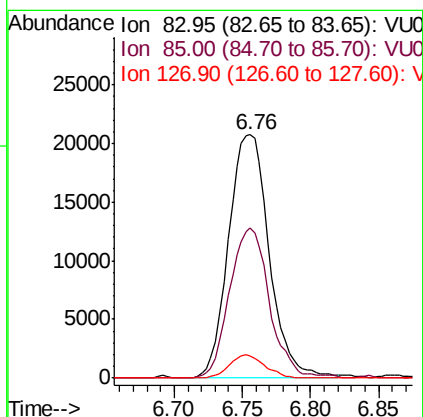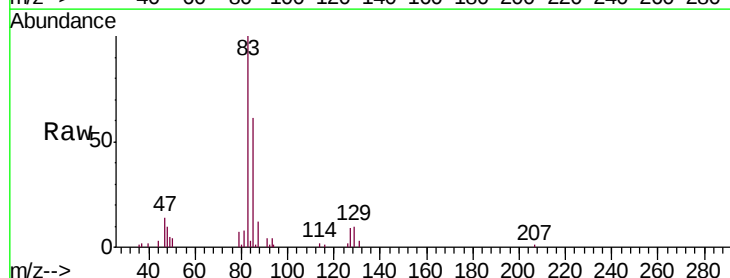



#42

Toluene

Concen: 0.185 ug/L

RT: 7.64 min Scan# 2036

Delta R.T. 0.00 min

Lab File: VU032097.D

Acq: 17 May 2019 11:59

Instrument :

MSVOA_U

ClientSampleId :





F9W47

Tgt Ion: 91 Resp: 11319

Ion Ratio Lower Upper

91 100

92 50.4 40.2 74.6

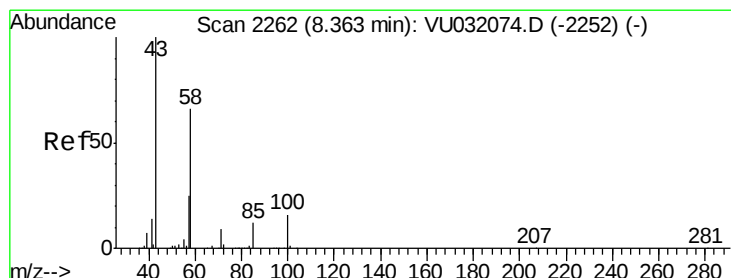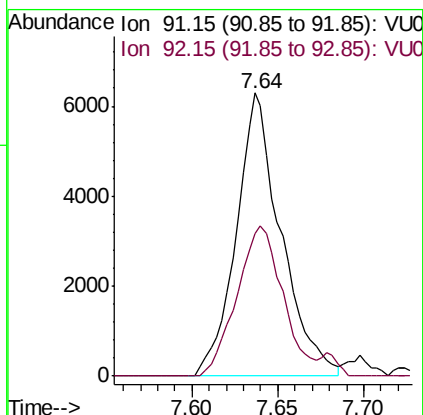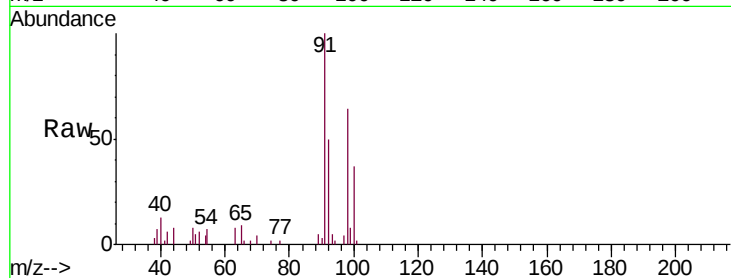

#48

2-Hexanone

Concen: 1.031 ug/L

RT: 8.38 min Scan# 2267

Delta R.T. 0.02 min

Lab File: VU032097.D

Acq: 17 May 2019 11:59

Tgt Ion: 43 Resp: 5303




Ion Ratio Lower Upper


43 100

58 77.2 51.6 77.4

57 16.4 18.4 27.6#

100 16.0 12.2 18.4

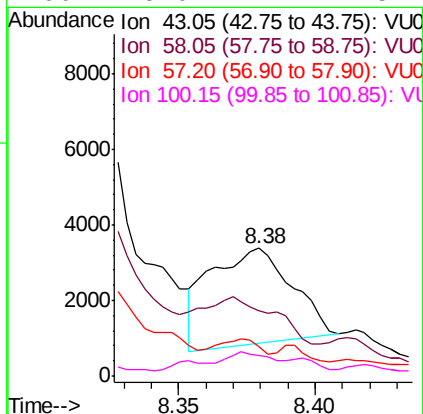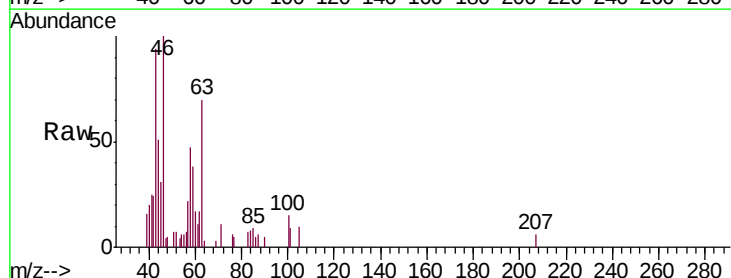

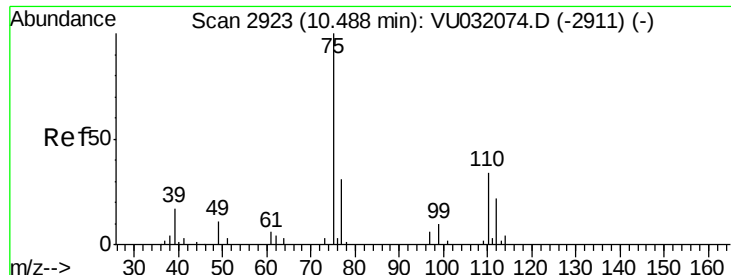

#59

1,2,3-Trichloropropane

Concen: 1.698 ug/L

RT: 11.48 min Scan# 3232

Delta R.T. 0.99 min

Lab File: VU032097.D

Acq: 17 May 2019 11:59

Instrument :

MSVOA_U

ClientSampleId :


F9W47

Tgt Ion: 75 Resp: 15417

Ion Ratio Lower Upper

75 100

77 36.7 26.2 39.2

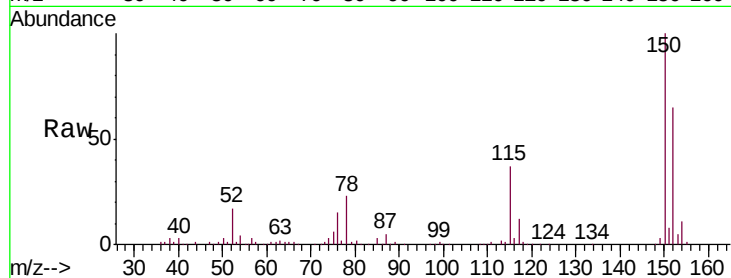

Abundance Ion 75.00 (74.70 to 75.70): VU0

Ion 77.00 (76.70 to 77.70): VU0

