

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051619\
 Data File : VU032076.D
 Acq On : 17 May 2019 03:18
 Operator : JC/SP
 Sample : K2859-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9W51

Quant Time: May 17 12:29:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 17 08:41:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	382892	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	397875	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	150016	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	143959	4.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.20%
7) Chloroethane-d5	1.68	69	123757	4.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.80%
11) 1,1-Dichloroethene-d2	2.27	63	203263	3.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.00%
20) 2-Butanone-d5	4.21	46	285763	45.13	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.26%
24) Chloroform-d	4.64	84	258278	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.31	65	133786	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
32) Benzene-d6	5.33	84	531901	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
36) 1,2-Dichloropropane-d6	6.33	67	156462	4.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.20%
41) Toluene-d8	7.56	98	442855	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	7.85	79	49628	3.89	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.80%
46) 2-Hexanone-d5	8.31	63	241842	41.93	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.86%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	128549	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	161035	5.07	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.40%


Target Compounds				Ovalue
13) Acetone	2.34	43	4796	2.307 ug/L 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051619\
Data File : VU032076.D
Acq On : 17 May 2019 03:18
Operator : JC/SP
Sample : K2859-12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9W51

Quant Time: May 17 12:29:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 17 08:41:24 2019
Response via : Initial Calibration

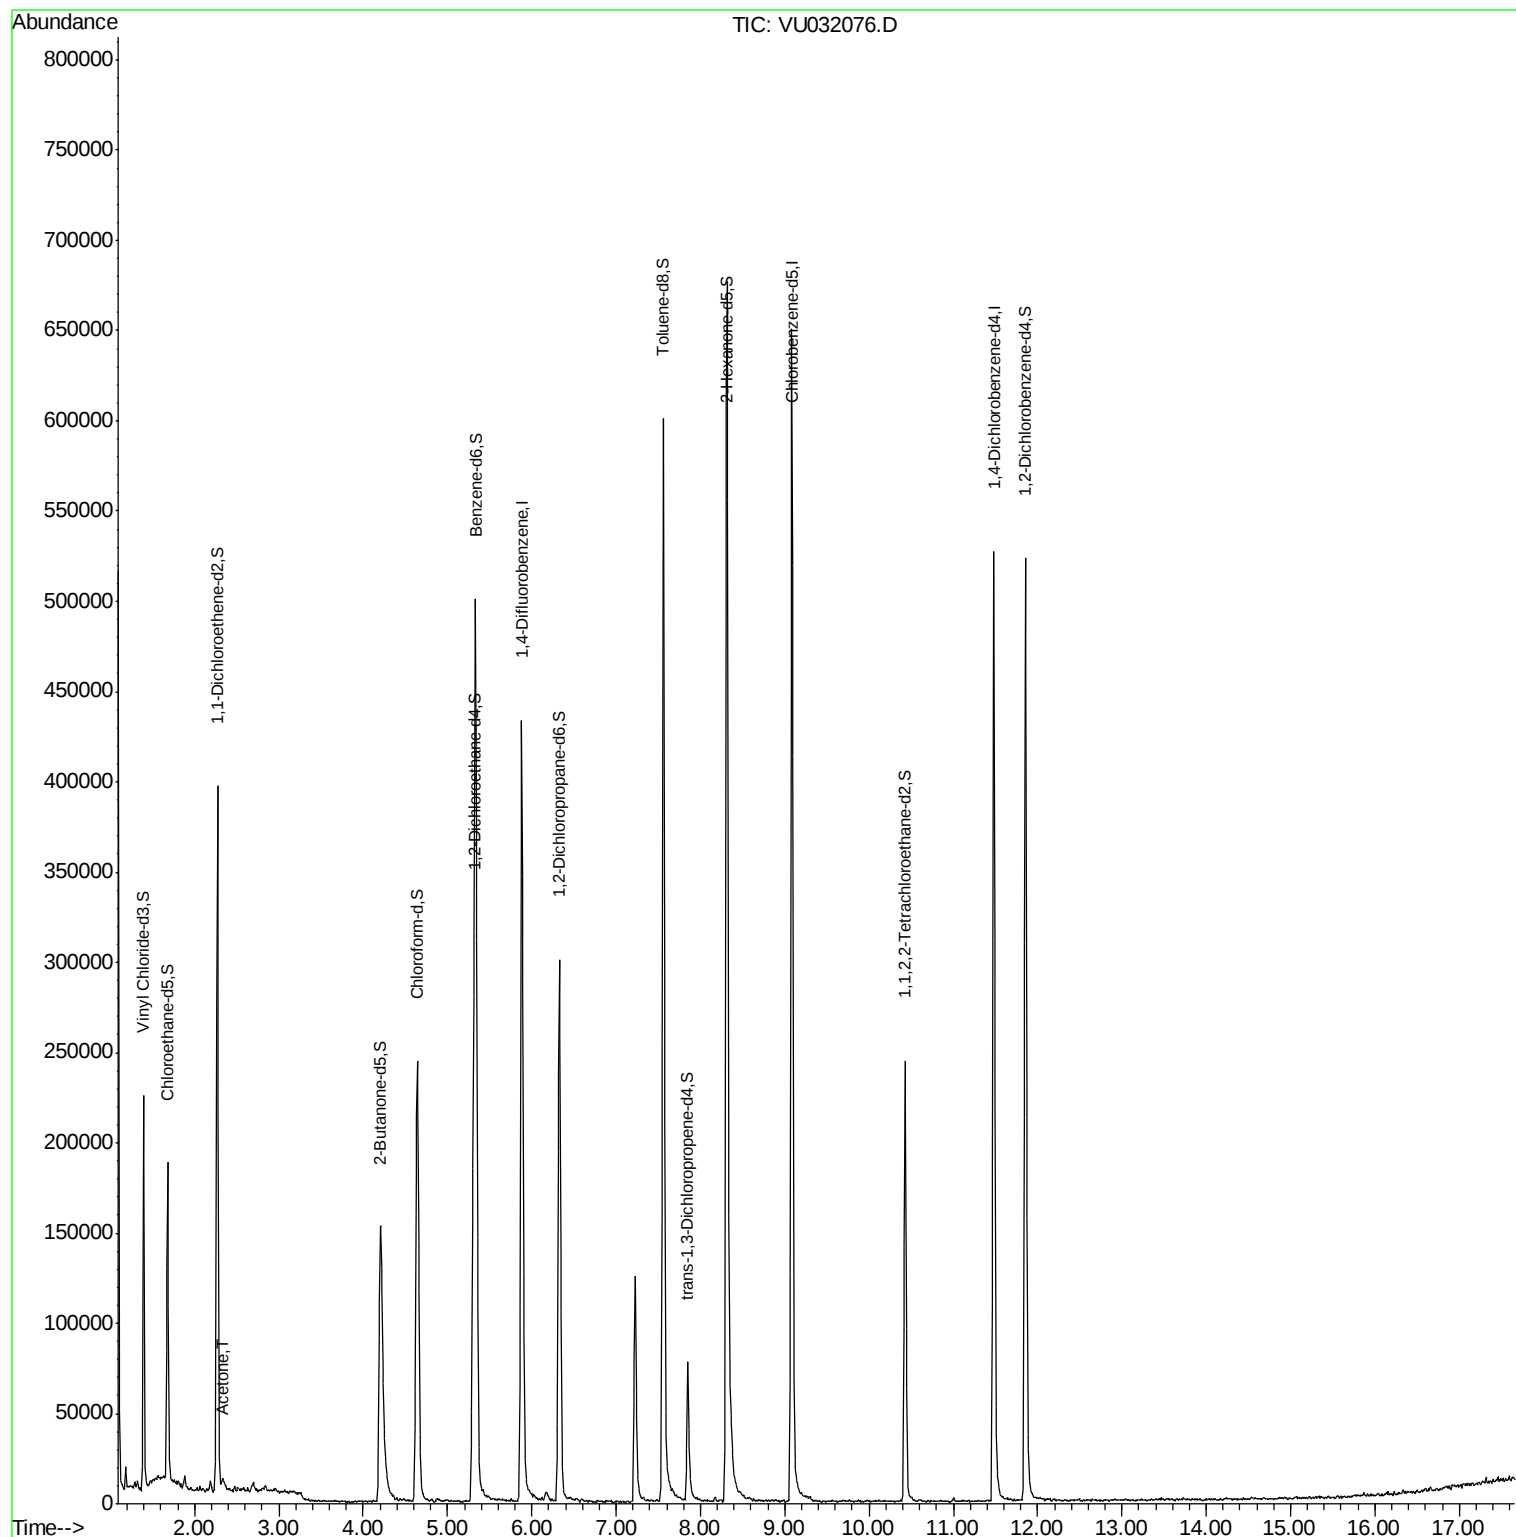

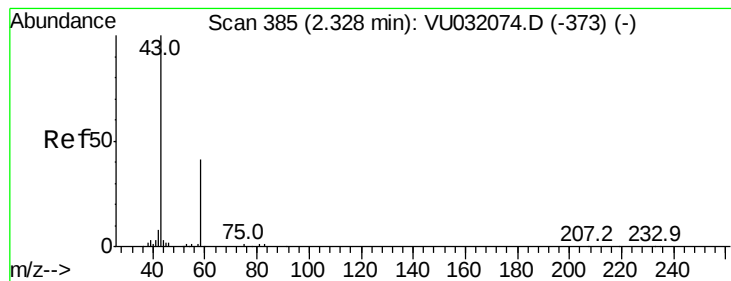

#13
 Acetone
 Concen: 2.307 ug/L
 RT: 2.34 min Scan# 389
 Delta R.T. 0.01 min
 Lab File: VU032076.D
 Acq: 17 May 2019 03:18

Instrument :
 MSVOA_U
 ClientSampleId :
 F9W51

Tot Ion: 43 Resp: 4796
 Ion Ratio Lower Upper
 43 100
 58 30.1 0.0 78.8

