


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051619\
Data File : VU032041.D
Acq On : 16 May 2019 10:56
Operator : JC/SP
Sample : BFB08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB08

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon May 20 04:57:10 2019

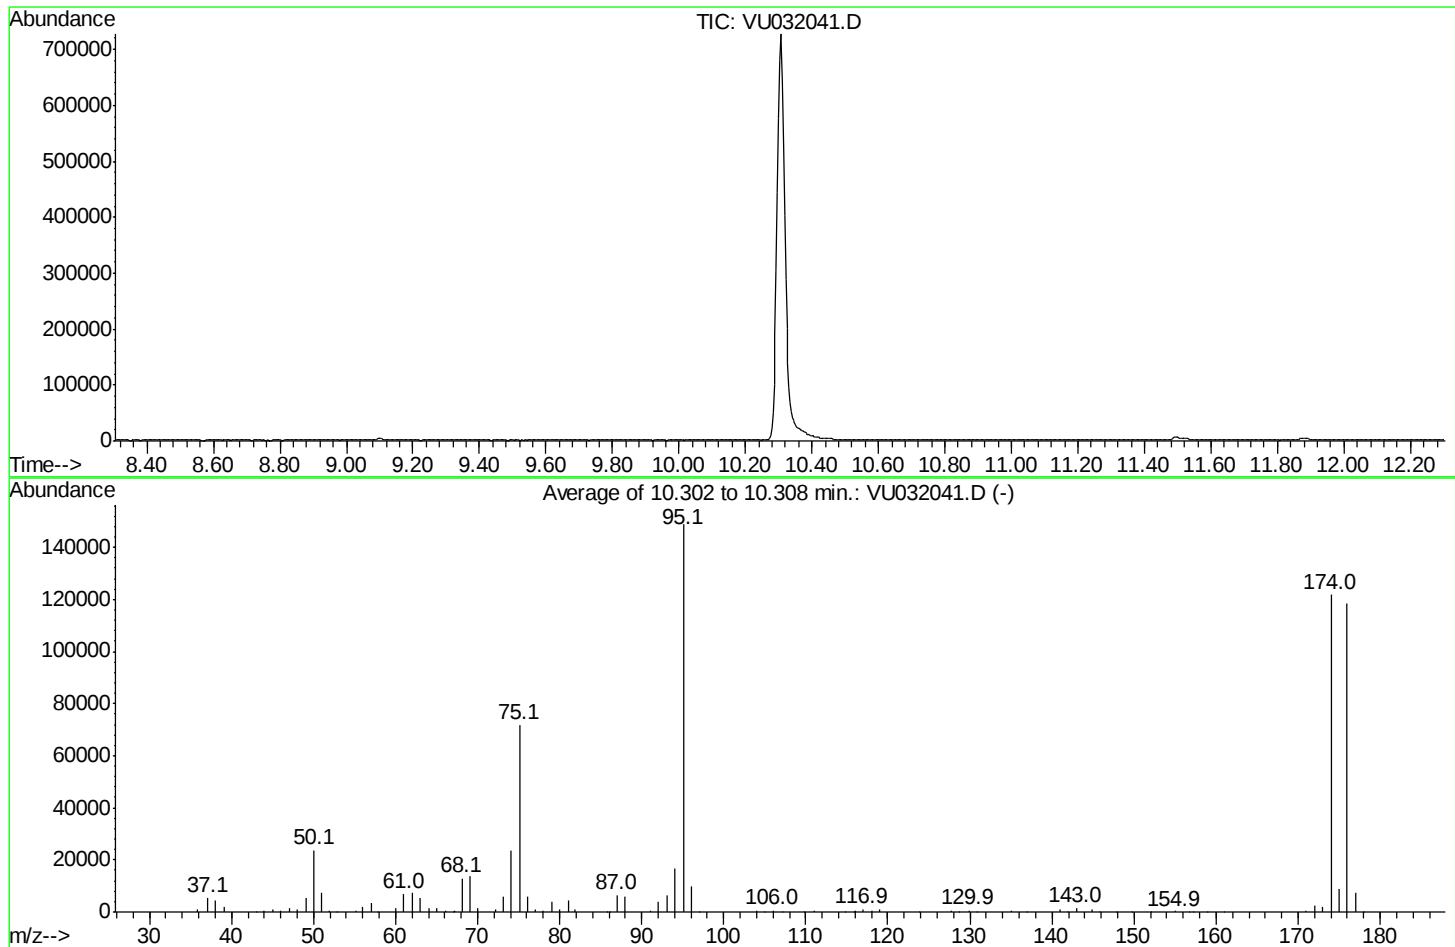

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	23826	PASS
75	95	30	80	48.3	71861	PASS
95	95	100	100	100.0	148821	PASS
96	95	5	9	6.5	9688	PASS
173	174	0.00	2	1.7	2049	PASS
174	95	50	120	81.9	121810	PASS
175	174	5	9	7.4	9049	PASS
176	174	95	101	97.1	118314	PASS
177	176	5	9	6.1	7184	PASS

m/z	Abundance
35.90	905.0
37.10	5347.0
38.00	4668.0
39.00	1872.0
40.00	638.0
43.00	252.0
44.00	1368.0
45.10	937.0
45.90	289.0
47.10	1307.0
48.00	747.0
49.10	4966.0
50.10	22664.0
51.00	7367.0
52.10	337.0
52.90	112.0
55.10	280.0
56.00	1558.0
57.00	3404.0
57.80	255.0
60.00	1268.0
61.00	6912.0
62.00	7134.0
63.10	5253.0
64.00	1431.0
65.00	1511.0
66.10	230.0
67.00	436.0
68.10	12352.0
69.10	13213.0
70.00	1371.0
72.10	1050.0
73.10	5398.0
74.10	22208.0
75.10	69992.0
76.10	5974.0
76.90	1005.0
78.00	550.0
79.00	3959.0
80.00	1091.0
81.00	4462.0
81.90	1141.0
86.00	379.0
87.00	6361.0
88.00	5436.0
91.10	465.0
92.10	3888.0
93.10	6290.0
94.10	16285.0
95.10	145024.0
96.10	9489.0
97.10	286.0
104.00	628.0
104.90	165.0
106.00	746.0
107.10	113.0
111.00	251.0
115.00	101.0
115.80	478.0
116.80	1009.0
118.00	490.0
119.10	912.0
123.80	115.0
127.80	319.0
128.70	168.0
129.90	580.0
130.90	162.0
135.10	187.0
136.90	189.0
140.90	964.0
141.90	131.0
143.00	1678.0
144.90	1054.0
145.90	301.0
147.90	209.0
149.70	122.0
152.00	106.0
154.90	347.0
156.70	200.0
157.20	163.0
159.00	184.0
171.00	419.0
172.00	2445.0
173.00	2067.0
174.00	113464.0
175.00	8559.0
176.00	111512.0
177.00	7143.0
177.90	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
35.90	1002.0
37.10	5847.0
38.00	4540.0
39.10	2083.0
40.00	542.0
43.00	180.0
44.00	1320.0
45.00	993.0
45.90	379.0
47.10	1370.0
48.00	851.0
49.10	5507.0
50.10	24664.0
51.00	7918.0
51.90	283.0
52.90	165.0
55.10	385.0
56.00	2015.0
57.00	3477.0
57.80	155.0
60.00	1453.0
61.00	7205.0
62.00	7778.0
63.00	5256.0
64.00	1320.0
65.00	1399.0
66.00	254.0
67.20	464.0
68.10	12945.0
69.10	14155.0
70.00	1479.0
72.10	950.0
73.00	5985.0
74.10	24216.0
75.10	73912.0
76.10	5894.0
77.00	907.0
77.90	681.0
79.00	4215.0
79.90	1164.0
81.00	4673.0
81.90	1186.0
86.10	303.0
87.00	6752.0
88.00	5835.0
91.10	545.0
92.10	4124.0
93.10	6783.0
94.10	17032.0
95.10	153472.0
96.10	9971.0
97.00	253.0
104.00	588.0
104.90	224.0
106.00	796.0
111.00	293.0
114.80	132.0
116.00	543.0
116.90	1216.0
118.10	571.0
119.00	917.0
127.80	417.0
128.70	174.0
129.90	609.0
130.90	157.0
135.10	288.0
136.90	268.0
141.00	1093.0
141.90	167.0
143.00	1591.0
144.90	1018.0
145.80	240.0
147.90	253.0
149.70	142.0
154.90	344.0
156.80	221.0
158.90	246.0
160.90	150.0
170.90	393.0
172.00	2801.0
173.00	2153.0
174.00	125064.0
175.10	9232.0
176.00	121776.0
177.00	7316.0
178.00	175.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

m/z	Abundance
35.90	984.0
37.10	5786.0
38.00	4060.0
39.10	2101.0
40.00	382.0
44.00	1295.0
45.00	883.0
45.90	366.0
47.00	1287.0
48.00	798.0
49.10	5578.0
50.10	24152.0
51.00	7322.0
51.90	265.0
52.90	186.0
55.10	420.0
56.00	2270.0
57.00	3387.0
57.80	113.0
60.10	1438.0
61.00	6806.0
62.00	7476.0
63.10	5151.0
64.00	1154.0
65.00	1376.0
66.00	331.0
67.20	501.0
68.10	13046.0
69.10	13892.0
70.00	1427.0
72.20	699.0
73.00	6316.0
74.10	24136.0
75.10	71680.0
76.00	5398.0
77.00	782.0
77.90	825.0
79.00	4077.0
79.90	1344.0
81.00	4425.0
81.90	1148.0
85.80	119.0
87.00	6800.0
88.00	5904.0
91.10	640.0
92.00	4030.0
93.10	6477.0
94.10	16736.0
95.10	147968.0
96.10	9604.0
97.00	237.0
104.00	499.0
104.90	219.0
106.00	717.0
109.80	125.0
111.00	265.0
114.80	175.0
116.00	575.0
117.00	1255.0
118.00	510.0
118.90	857.0
127.80	445.0
128.70	164.0
129.90	591.0
130.90	144.0
135.10	320.0
136.90	322.0
141.00	1118.0
141.90	177.0
143.00	1521.0
144.90	861.0
145.80	192.0
147.90	318.0
149.80	101.0
155.00	300.0
156.90	213.0
158.80	277.0
160.90	180.0
170.90	385.0
172.00	2791.0
173.00	1927.0
174.00	126904.0
175.10	9358.0
176.00	121656.0
177.00	7094.0
178.00	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08

Scan 2852 (10.260 min): VU032041.D
BFB08

m/z	Abundance
39.90	763.0
43.90	801.0

Instrument :
MSVOA_U
ClientSampleId :
BFB08