

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
 Data File : VU048585.D
 Acq On : 16 May 2022 17:13
 Operator : SY/MD
 Sample : N2848-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX1

Quant Time: May 17 07:01:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 17 06:52:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	233040	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	232020	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	129746	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	66424	46.537	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	93.080%
7) Chloroethane-d5	1.912	69	51269	47.944	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.880%
11) 1,1-Dichloroethene-d2	2.568	63	116949	36.229	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.460%
21) 2-Butanone-d5	4.620	46	128675	94.732	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.730%
24) Chloroform-d	5.067	84	173224	48.026	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.060%
26) 1,2-Dichloroethane-d4	5.703	65	128300	50.420	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.840%
32) Benzene-d6	5.729	84	312208	48.350	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.700%
36) 1,2-Dichloropropane-d6	6.694	67	91261	48.142	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.280%
41) Toluene-d8	7.899	98	292756	48.200	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.400%
43) trans-1,3-Dichloroprop...	8.182	79	55513	45.795	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.600%
47) 2-Hexanone-d5	8.632	63	93044	89.499	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.500%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	145591	46.414	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.820%
66) 1,2-Dichlorobenzene-d4	12.195	152	130137	49.064	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.120%
Target Compounds						
					Qvalue	
13) Acetone	2.629	43	9122	8.266	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
Data File : VU048585.D
Acq On : 16 May 2022 17:13
Operator : SY/MD
Sample : N2848-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX1

Quant Time: May 17 07:01:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 17 06:52:50 2022
Response via : Initial Calibration

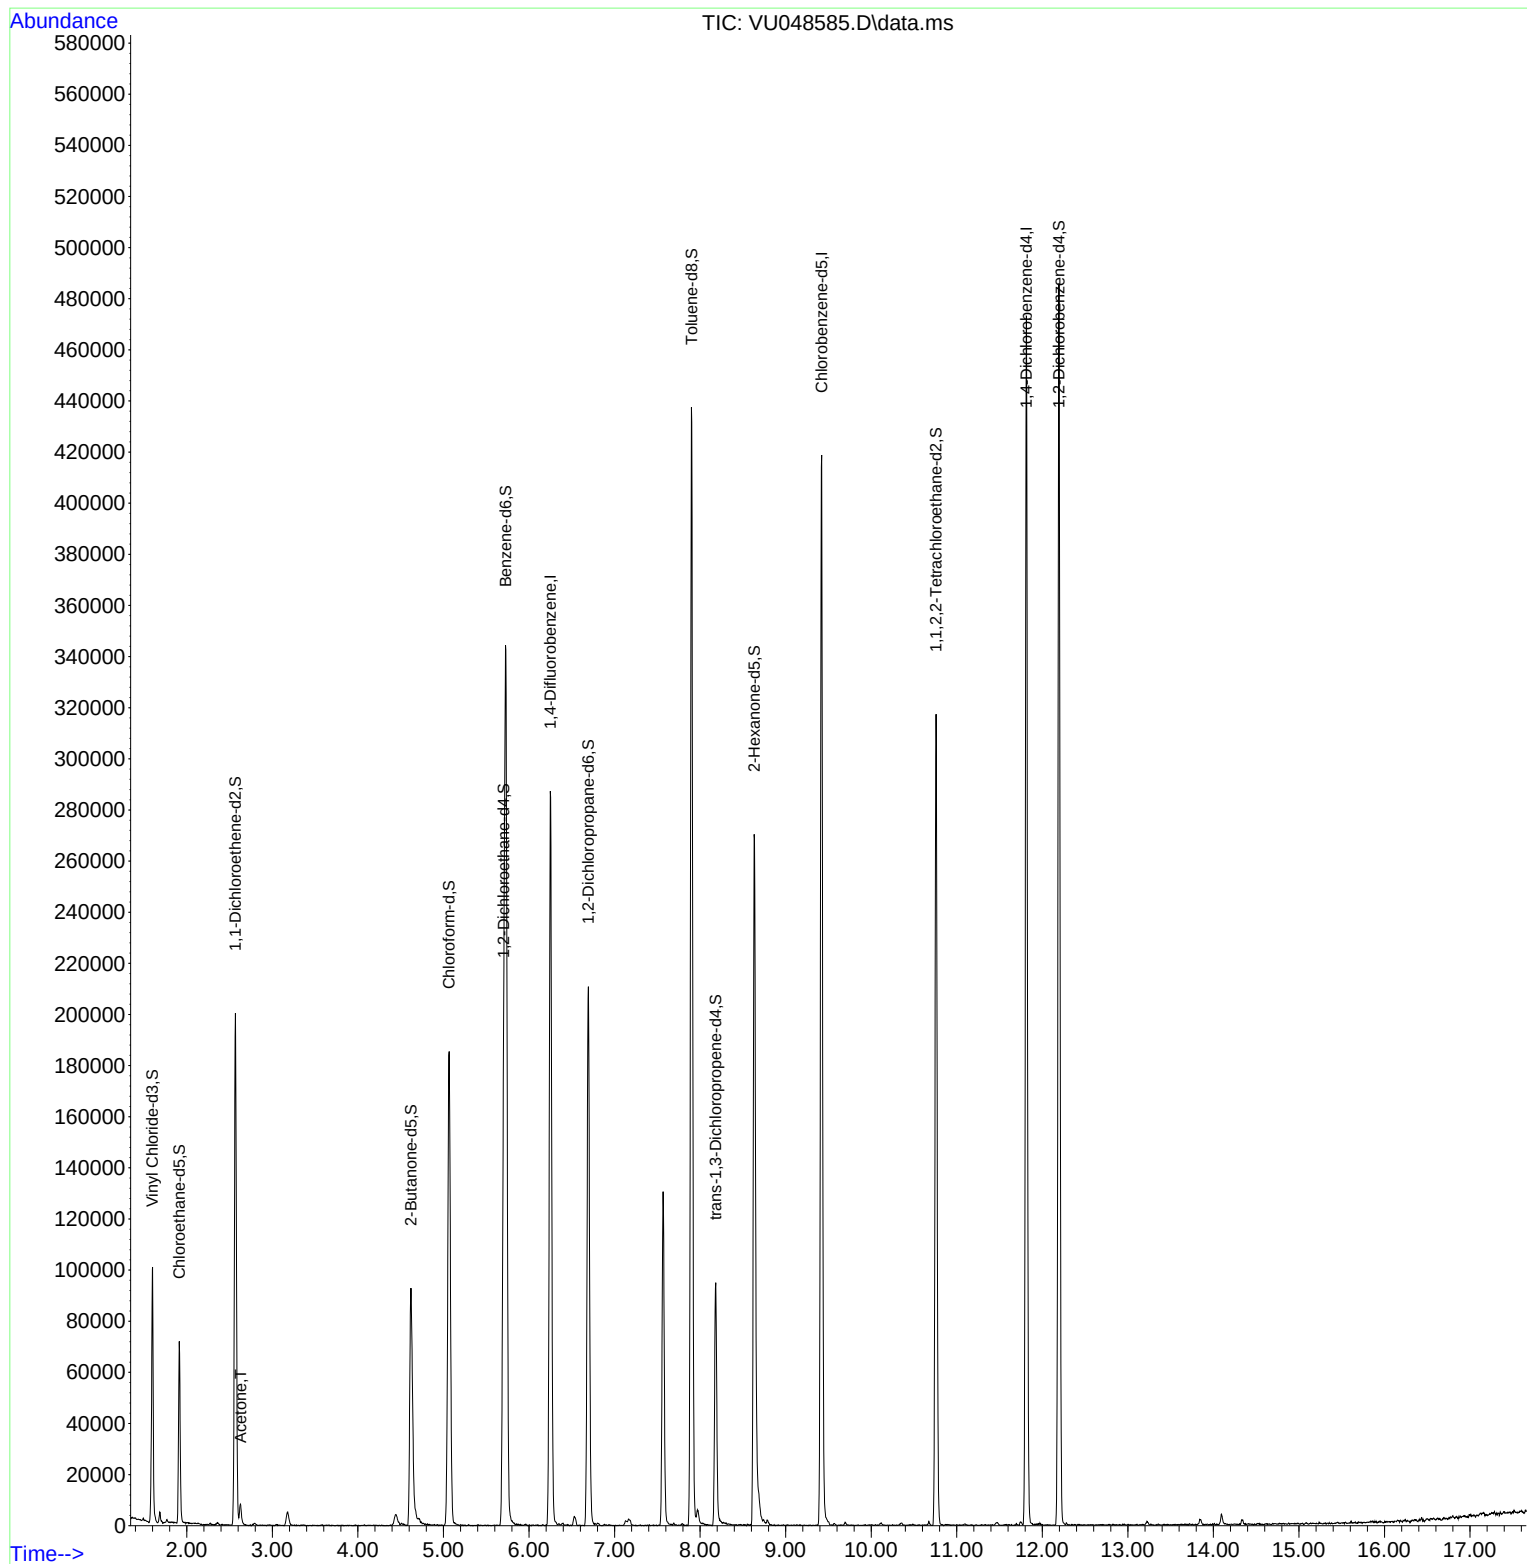

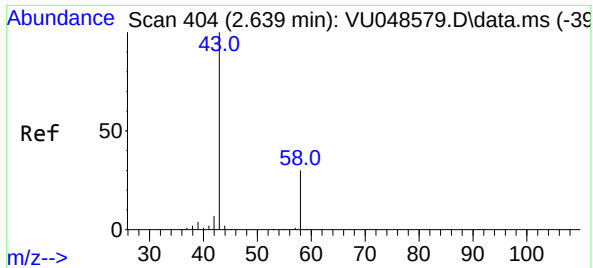

#13
 Acetone
 Concen: 8.266 ug/L
 RT: 2.629 min Scan# 40
 Delta R.T. -0.010 min
 Lab File: VU048585.D
 Acq: 16 May 2022 17:13

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX1

Tgt Ion: 43 Resp: 9122
 Ion Ratio Lower Upper
 43 100
 58 27.0 0.0 59.8

