

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
 Data File : VU048594.D
 Acq On : 16 May 2022 20:44
 Operator : SY/MD
 Sample : N2849-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX2

Quant Time: May 17 07:02:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 17 06:52:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	225961	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	228020	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	127134	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	59515	43.002	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.000%
7) Chloroethane-d5	1.912	69	47417	45.731	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.460%
11) 1,1-Dichloroethene-d2	2.568	63	107159	34.236	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.480%
21) 2-Butanone-d5	4.616	46	129722	98.495	ug/L	-0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.490%
24) Chloroform-d	5.063	84	164064	46.911	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.820%
26) 1,2-Dichloroethane-d4	5.703	65	118817	48.156	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.320%
32) Benzene-d6	5.729	84	293319	46.221	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.440%
36) 1,2-Dichloropropane-d6	6.690	67	85114	45.687	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.380%
41) Toluene-d8	7.899	98	267983	44.895	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.800%
43) trans-1,3-Dichloroprop...	8.179	79	51217	42.993	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.980%
47) 2-Hexanone-d5	8.632	63	91244	89.307	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.310%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	138806	45.027	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.060%
66) 1,2-Dichlorobenzene-d4	12.195	152	122151	47.000	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.000%
Target Compounds						
13) Acetone	2.626	43	3192	2.983	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
Data File : VU048594.D
Acq On : 16 May 2022 20:44
Operator : SY/MD
Sample : N2849-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX2

Quant Time: May 17 07:02:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 17 06:52:50 2022
Response via : Initial Calibration

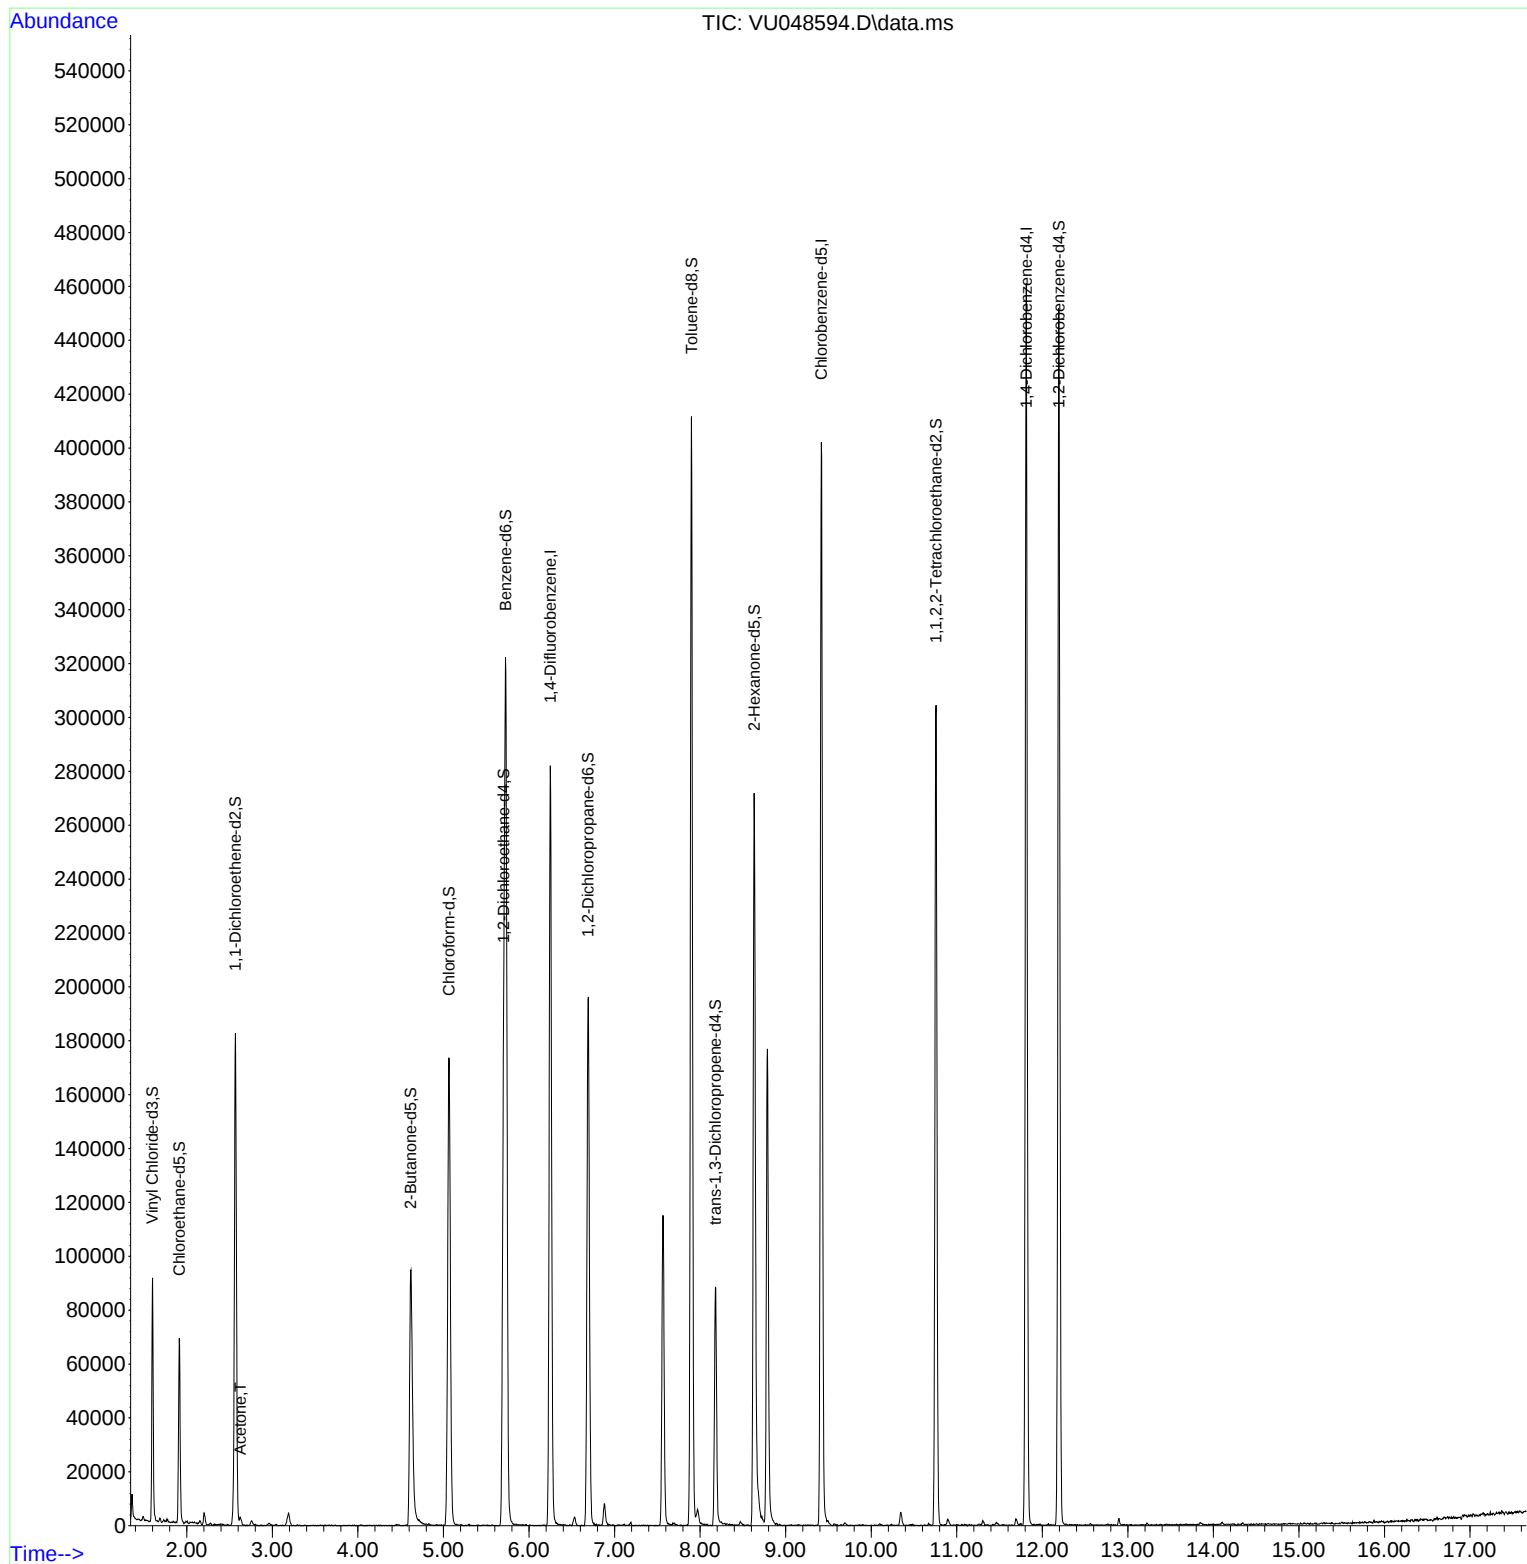

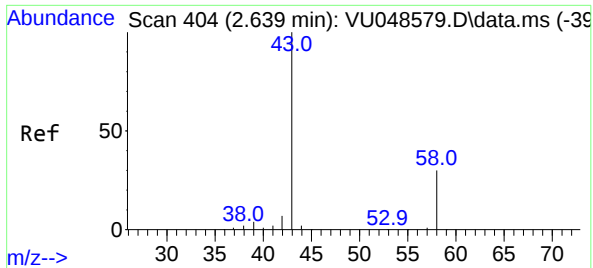

#13
Acetone
Concen: 2.983 ug/L
RT: 2.626 min Scan# 40
Delta R.T. -0.013 min
Lab File: VU048594.D
Acq: 16 May 2022 20:44

Instrument :
MSVOA_U
ClientSampleId :
EXXX2

Tgt Ion: 43 Resp: 3192
Ion Ratio Lower Upper
43 100
58 32.1 0.0 59.8

