

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
 Data File : VU048584.D
 Acq On : 16 May 2022 16:24
 Operator : SY/MD
 Sample : N2790-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	92884	101676	11.04%	1.351%
2	1.912	170	178	193	rBV	68963	90640	9.85%	1.205%
3	2.392	325	327	332	rBV2	355	315	0.03%	0.004%
4	2.568	370	382	399	rBV	190415	308585	33.52%	4.101%
5	2.691	417	420	423	rBV2	382	242	0.03%	0.003%
6	2.790	446	451	461	rVB3	1309	2076	0.23%	0.028%
7	2.961	499	504	509	rBB2	308	377	0.04%	0.005%
8	2.993	510	514	516	rBV	205	196	0.02%	0.003%
9	3.002	516	517	521	rVV	303	197	0.02%	0.003%
10	3.047	523	531	541	rVV3	2764	5196	0.56%	0.069%
11	3.099	543	547	550	rBB	218	187	0.02%	0.002%
12	3.189	561	575	596	rBV	8540	20379	2.21%	0.271%
13	3.324	614	617	621	rBV2	274	278	0.03%	0.004%
14	3.408	641	643	645	rVB	302	146	0.02%	0.002%
15	3.430	648	650	653	rBV	302	185	0.02%	0.002%
16	3.472	660	663	668	rVB2	209	145	0.02%	0.002%
17	3.530	677	681	682	rBV	312	239	0.03%	0.003%
18	3.652	716	719	721	rBV	287	181	0.02%	0.002%
19	3.758	748	752	754	rBV	250	208	0.02%	0.003%
20	3.916	799	801	804	rBV	195	152	0.02%	0.002%
21	4.015	829	832	835	rBV	304	248	0.03%	0.003%
22	4.334	928	931	933	rBV2	250	156	0.02%	0.002%
23	4.414	954	956	959	rVB	253	151	0.02%	0.002%
24	4.462	968	971	978	rBB	357	398	0.04%	0.005%
25	4.620	1008	1020	1043	rBV	100639	243519	26.45%	3.236%
26	4.964	1125	1127	1130	rVB	284	167	0.02%	0.002%
27	4.980	1130	1132	1135	rBV	232	146	0.02%	0.002%
28	5.067	1139	1159	1184	rBV	175405	387410	42.08%	5.148%
29	5.166	1184	1190	1194	rBV2	374	443	0.05%	0.006%
30	5.215	1201	1205	1207	rBV	266	231	0.03%	0.003%
31	5.427	1267	1271	1272	rBV	323	245	0.03%	0.003%
32	5.501	1290	1294	1297	rBB	323	230	0.02%	0.003%
33	5.565	1312	1314	1318	rBV	156	156	0.02%	0.002%
34	5.616	1327	1330	1333	rBB	282	180	0.02%	0.002%
35	5.726	1343	1364	1391	rBV2	328344	920648	100.00%	12.234%
36	5.903	1418	1419	1422	rVB	369	177	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
 Data File : VU048584.D
 Acq On : 16 May 2022 16:24
 Operator : SY/MD
 Sample : N2790-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	5.932	1425	1428	1432	rVV2	436	348	0.04%	0.005%
38	5.970	1435	1440	1443	rBB2	372	301	0.03%	0.004%
39	5.986	1443	1445	1448	rBB	383	175	0.02%	0.002%
40	6.006	1448	1451	1453	rBV2	321	199	0.02%	0.003%
41	6.076	1468	1473	1475	rBV3	261	208	0.02%	0.003%
42	6.150	1490	1496	1497	rBB	321	219	0.02%	0.003%
43	6.250	1512	1527	1552	rBV	295625	557755	60.58%	7.412%
44	6.533	1606	1615	1624	rBV8	3558	6708	0.73%	0.089%
45	6.604	1635	1637	1642	rBV	328	295	0.03%	0.004%
46	6.694	1651	1665	1684	rVV2	204083	402800	43.75%	5.353%
47	6.796	1694	1697	1700	rBV3	446	341	0.04%	0.005%
48	6.816	1700	1703	1707	rVB	793	569	0.06%	0.008%
49	6.896	1725	1728	1729	rBV	306	183	0.02%	0.002%
50	6.986	1754	1756	1759	rBV	196	142	0.02%	0.002%
51	7.096	1788	1790	1794	rVB	299	220	0.02%	0.003%
52	7.179	1808	1816	1817	rBV2	988	919	0.10%	0.012%
53	7.243	1832	1836	1837	rBV2	273	196	0.02%	0.003%
54	7.272	1840	1845	1850	rBB	261	278	0.03%	0.004%
55	7.308	1851	1856	1859	rBB2	308	253	0.03%	0.003%
56	7.378	1875	1878	1880	rBV2	241	169	0.02%	0.002%
57	7.420	1886	1891	1895	rBV	277	409	0.04%	0.005%
58	7.568	1924	1937	1957	rBV	125861	220875	23.99%	2.935%
59	7.674	1968	1970	1971	rBV	417	148	0.02%	0.002%
60	7.764	1992	1998	2001	rBV	317	363	0.04%	0.005%
61	7.796	2001	2008	2014	rVV4	1254	1524	0.17%	0.020%
62	7.899	2026	2040	2057	rBV	425307	737016	80.05%	9.794%
63	8.102	2100	2103	2105	rBB	263	156	0.02%	0.002%
64	8.182	2114	2128	2146	rBV	89492	160399	17.42%	2.132%
65	8.542	2235	2240	2241	rBV	175	177	0.02%	0.002%
66	8.562	2241	2246	2251	rVB2	524	535	0.06%	0.007%
67	8.587	2251	2254	2256	rBV	182	154	0.02%	0.002%
68	8.632	2256	2268	2300	rBV	288246	527183	57.26%	7.006%
69	8.864	2337	2340	2343	rVB2	314	255	0.03%	0.003%
70	8.883	2344	2346	2349	rBV	345	291	0.03%	0.004%
71	8.919	2349	2357	2358	rBV	971	943	0.10%	0.013%
72	9.211	2445	2448	2450	rBV	270	142	0.02%	0.002%
73	9.250	2456	2460	2465	rVB	343	338	0.04%	0.004%
74	9.420	2499	2513	2536	rBV	421472	711197	77.25%	9.451%
75	9.639	2577	2581	2584	rBV3	327	263	0.03%	0.003%
76	9.690	2592	2597	2598	rBV	932	604	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
 Data File : VU048584.D
 Acq On : 16 May 2022 16:24
 Operator : SY/MD
 Sample : N2790-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.012	2696	2697	2701	rVB2	305	154	0.02%	0.002%
78	10.099	2720	2724	2726	rBV2	630	497	0.05%	0.007%
79	10.385	2811	2813	2817	rVB	377	172	0.02%	0.002%
80	10.484	2839	2844	2845	rBV	561	440	0.05%	0.006%
81	10.549	2861	2864	2868	rBV2	313	236	0.03%	0.003%
82	10.674	2896	2903	2909	rVB2	1186	1430	0.16%	0.019%
83	10.758	2916	2929	2946	rBV	314148	512403	55.66%	6.809%
84	10.825	2946	2950	2955	rVB3	548	492	0.05%	0.007%
85	11.092	3027	3033	3039	rBV4	694	966	0.10%	0.013%
86	11.443	3139	3142	3143	rBV2	650	339	0.04%	0.005%
87	11.613	3192	3195	3197	rVB	261	143	0.02%	0.002%
88	11.697	3217	3221	3228	rVB2	430	454	0.05%	0.006%
89	11.748	3231	3237	3244	rVV4	2063	2522	0.27%	0.034%
90	11.812	3244	3257	3277	rVV	493542	793767	86.22%	10.548%
91	12.195	3363	3376	3393	rBV	473038	771889	83.84%	10.258%
92	12.507	3467	3473	3476	rBV2	424	406	0.04%	0.005%
93	12.880	3586	3589	3591	rBV	242	169	0.02%	0.002%
94	13.221	3692	3695	3698	rBV4	1539	1258	0.14%	0.017%
95	13.279	3711	3713	3716	rVB2	324	171	0.02%	0.002%
96	13.642	3822	3826	3831	rBV	411	364	0.04%	0.005%
97	13.674	3831	3836	3840	rVV2	393	383	0.04%	0.005%
98	13.844	3882	3889	3902	rVB4	3636	5362	0.58%	0.071%
99	13.967	3924	3927	3930	rBV2	407	306	0.03%	0.004%
100	14.092	3960	3966	3978	rVB	5708	9407	1.02%	0.125%




Sum of corrected areas: 7525085

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
Data File : VU048584.D
Acq On : 16 May 2022 16:24
Operator : SY/MD
Sample : N2790-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

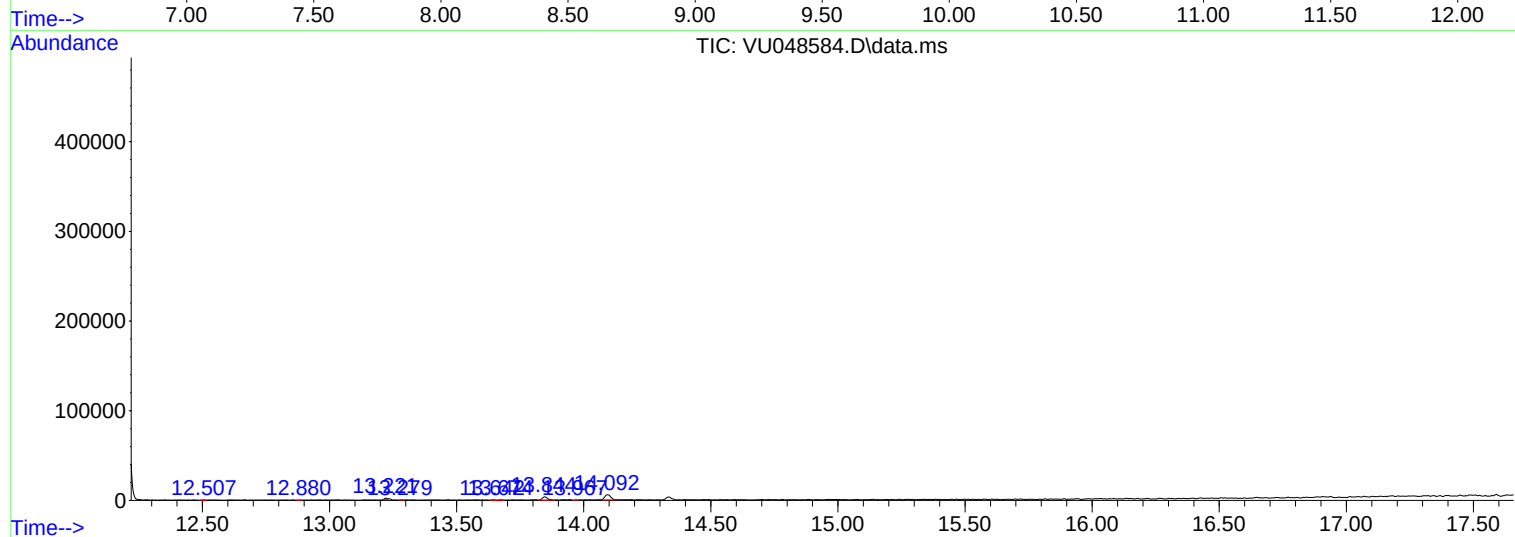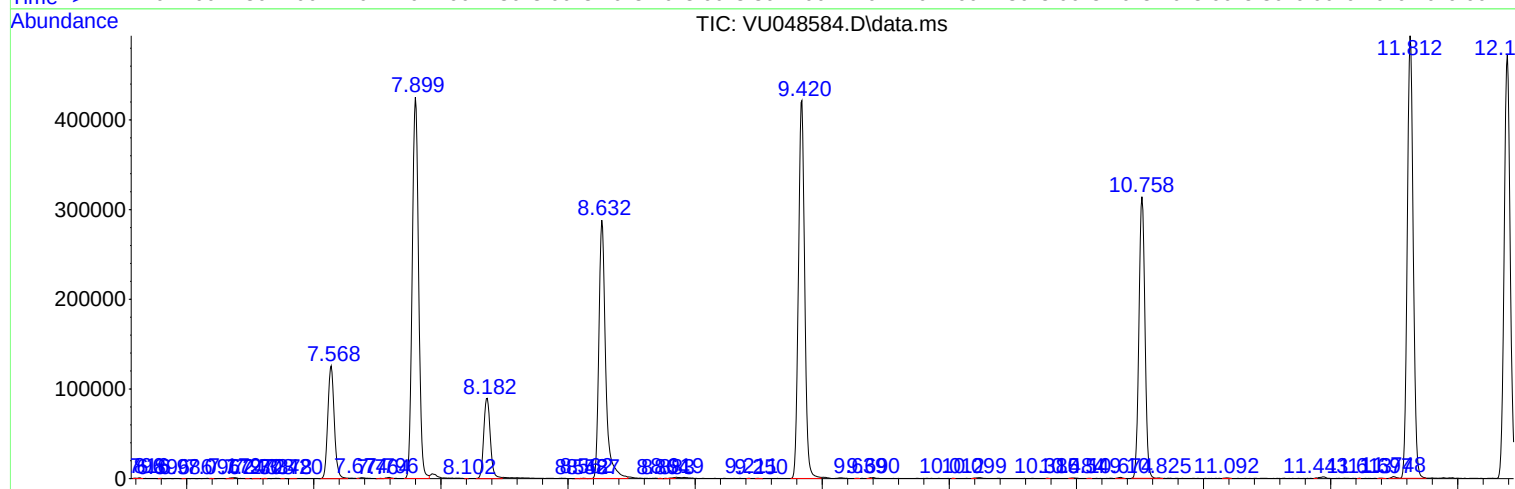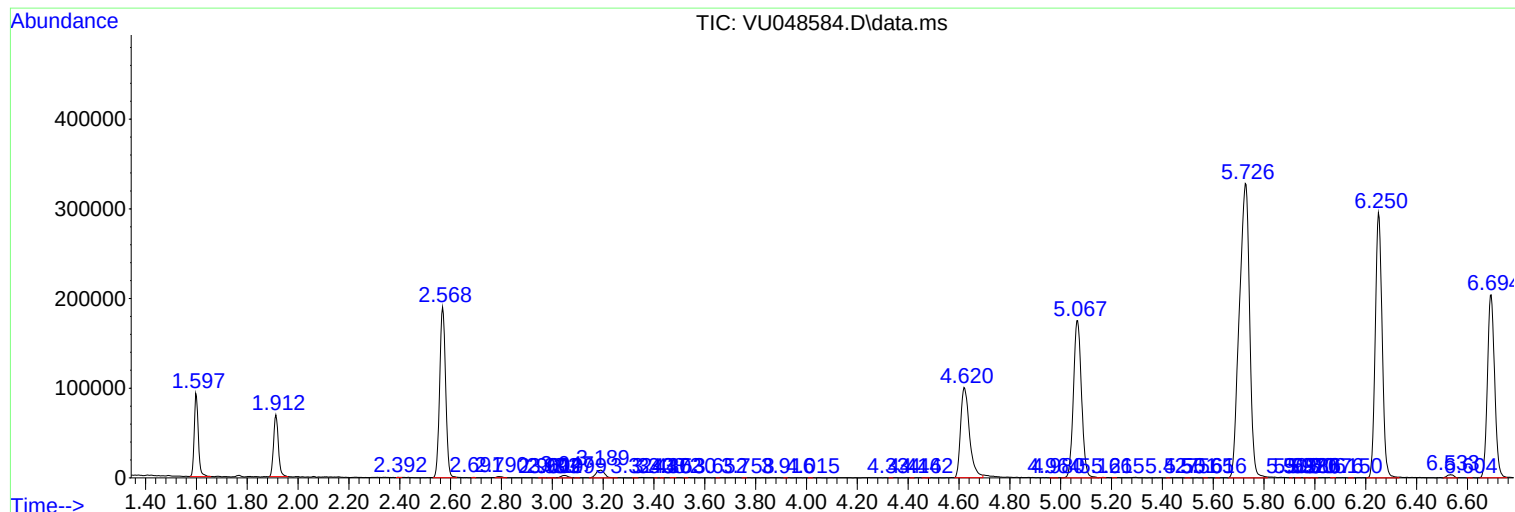

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
Data File : VU048584.D
Acq On : 16 May 2022 16:24
Operator : SY/MD
Sample : N2790-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
Data File : VU048584.D
Acq On : 16 May 2022 16:24
Operator : SY/MD
Sample : N2790-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc