


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051622\
 Data File : VU048575.D
 Acq On : 16 May 2022 09:57
 Operator : SY/MD
 Sample : BFB087
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB087

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis
 Last Update : Fri May 20 04:37:51 2022

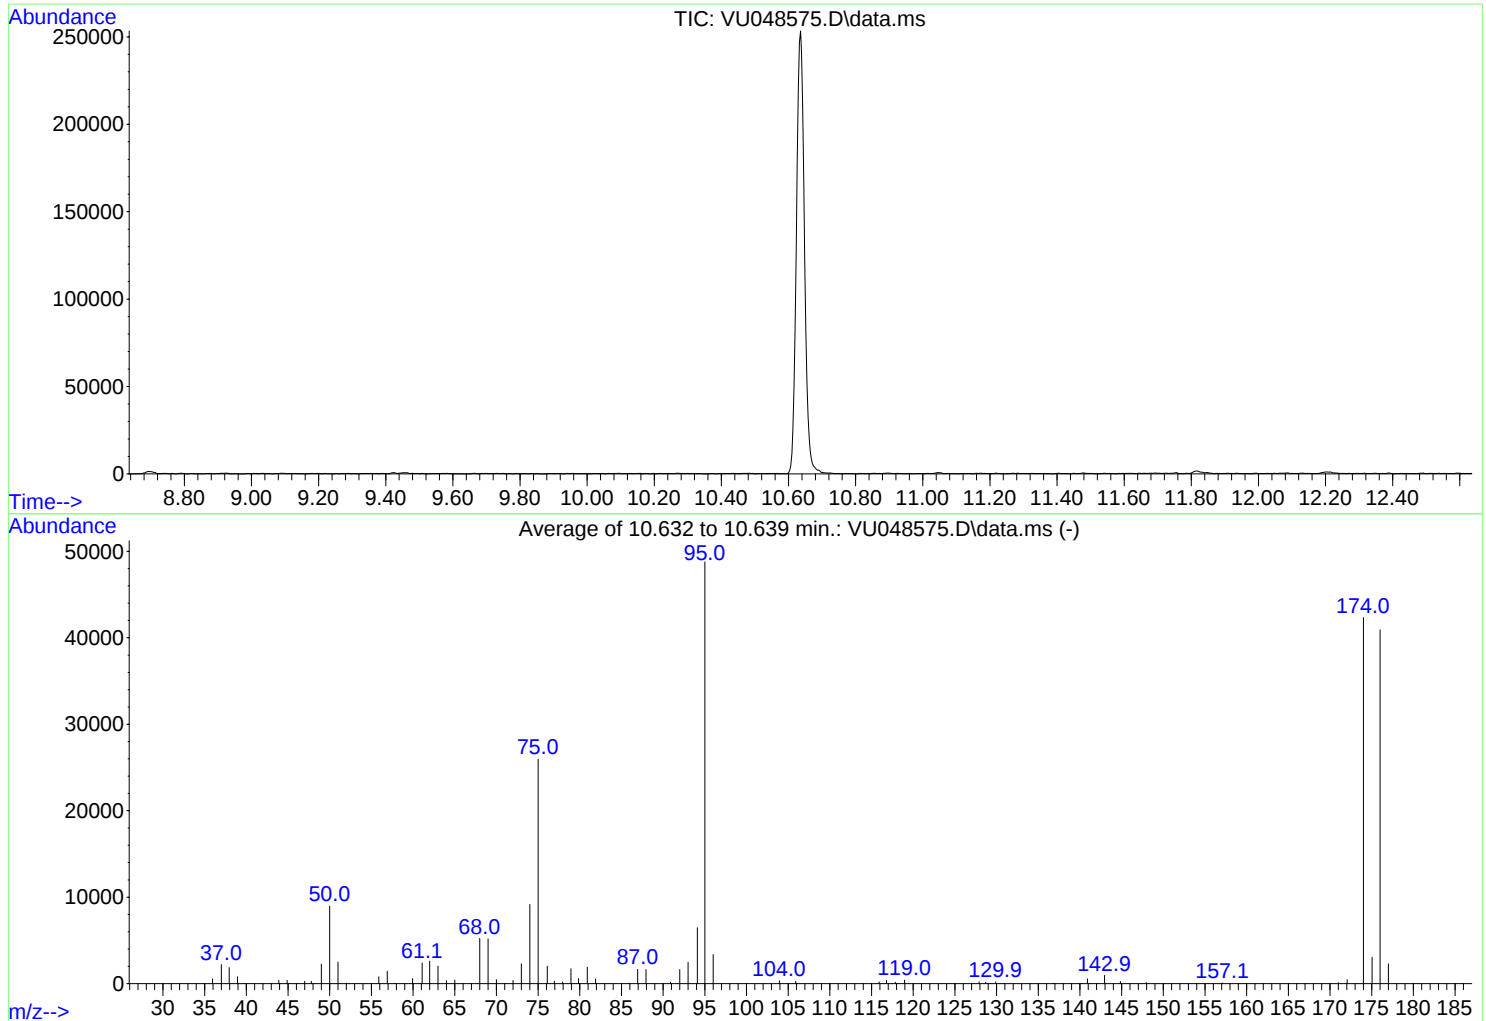

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	8953	PASS
75	95	30	80	53.2	25973	PASS
95	95	100	100	100.0	48784	PASS
96	95	5	9	6.9	3366	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	42333	PASS
175	174	5	9	7.2	3052	PASS
176	174	95	101	96.7	40915	PASS
177	176	5	9	5.6	2304	PASS

m/z	Abundance
44.00	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
36.00	582.0
37.00	2175.0
38.00	1934.0
38.90	718.0
39.70	122.0
43.90	479.0
44.90	452.0
47.00	307.0
47.80	266.0
49.00	2292.0
50.00	9142.0
51.00	2484.0
55.00	103.0
55.90	710.0
56.90	1436.0
59.90	582.0
61.10	2381.0
62.00	2895.0
63.00	1934.0
64.00	445.0
65.00	316.0
68.00	4947.0
69.00	5175.0
70.00	417.0
72.00	403.0
73.00	2291.0
74.00	9297.0
75.00	26176.0
76.10	2105.0
77.00	338.0
78.00	192.0
79.00	1652.0
79.90	615.0
80.90	1952.0
81.90	498.0
85.90	111.0
87.00	1710.0
88.00	1636.0
91.00	134.0
92.00	1702.0
93.00	2537.0
94.10	6546.0
95.00	49400.0
96.00	3415.0
104.00	285.0
105.90	278.0
115.90	205.0
116.80	343.0
117.80	118.0
118.90	386.0
127.90	191.0
128.70	139.0
129.90	197.0
136.80	106.0
140.80	567.0
143.00	907.0
144.90	277.0
148.00	136.0
171.00	122.0
172.10	447.0
174.00	41952.0
175.10	2703.0
176.00	40096.0
177.00	2438.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	552.0
37.00	2215.0
38.00	1895.0
39.00	846.0
43.90	471.0
44.90	384.0
47.00	306.0
47.80	295.0
49.00	2387.0
50.00	9161.0
51.00	2511.0
52.00	107.0
55.90	855.0
56.90	1508.0
59.90	588.0
61.10	2523.0
62.00	2639.0
63.00	2146.0
64.00	372.0
65.00	469.0
68.00	5362.0
69.00	5314.0
70.00	461.0
72.00	413.0
73.00	2364.0
74.00	9423.0
75.00	26680.0
76.10	2076.0
77.00	314.0
78.00	197.0
78.90	1776.0
79.80	615.0
80.90	1995.0
81.90	567.0
87.00	1639.0
88.00	1616.0
91.00	174.0
92.00	1677.0
93.00	2577.0
94.10	6646.0
95.00	49872.0
96.00	3413.0
103.90	335.0
105.90	272.0
115.90	222.0
116.80	413.0
117.90	161.0
119.00	416.0
127.90	215.0
128.70	170.0
129.90	223.0
140.90	560.0
142.90	986.0
144.80	256.0
148.00	133.0
157.10	118.0
171.00	106.0
172.00	479.0
174.00	43536.0
175.00	3120.0
176.00	41912.0
177.00	2295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087

m/z	Abundance
35.90	536.0
37.00	2206.0
37.90	1713.0
39.00	823.0
43.90	492.0
44.90	339.0
47.00	237.0
47.80	248.0
49.00	2117.0
50.00	8557.0
51.00	2500.0
52.00	117.0
55.90	830.0
56.90	1391.0
57.80	120.0
60.00	535.0
61.10	2255.0
62.00	2304.0
63.00	2012.0
64.00	263.0
65.00	514.0
68.00	5399.0
69.00	5039.0
70.00	492.0
72.00	305.0
73.00	2244.0
74.00	8759.0
75.00	25064.0
76.10	1899.0
76.90	254.0
77.90	190.0
78.90	1734.0
79.80	536.0
80.90	1783.0
81.90	547.0
86.90	1620.0
87.90	1612.0
90.80	192.0
92.00	1525.0
93.00	2344.0
94.10	6205.0
95.00	47080.0
96.00	3270.0
103.90	376.0
105.90	226.0
115.90	202.0
116.80	427.0
117.90	218.0
119.00	434.0
127.90	210.0
128.70	155.0
129.90	214.0
130.90	100.0
141.00	536.0
142.90	970.0
144.80	221.0
147.90	121.0
157.10	100.0
171.00	110.0
172.00	486.0
174.00	41512.0
175.00	3333.0
176.00	40736.0
177.00	2180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB087