
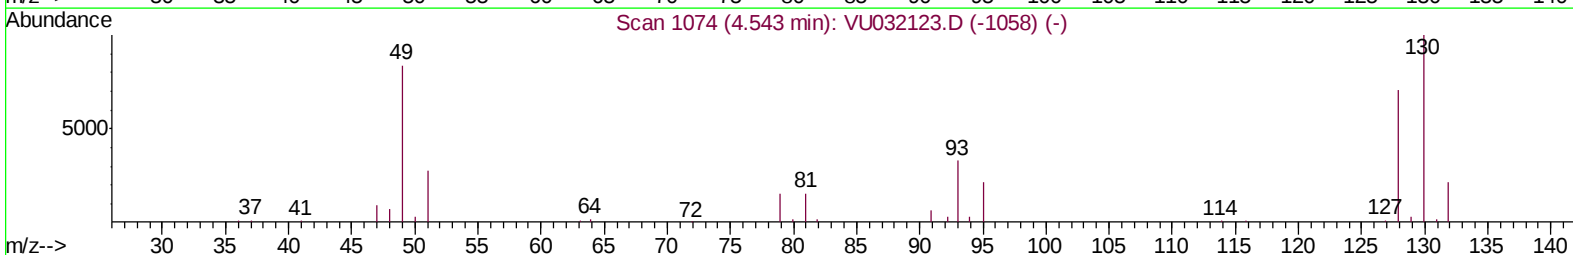
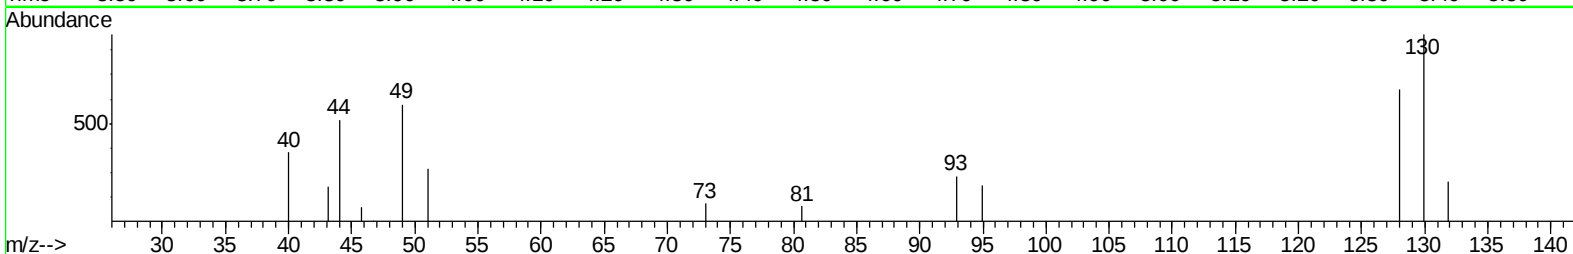


Data File : VU032132.D
Acq On : 18 May 2019 05:01
Operator : JC/SP
Sample : K2860-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Quant Time: May 18 05:50:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat May 18 05:45:56 2019
Response via : Initial Calibration

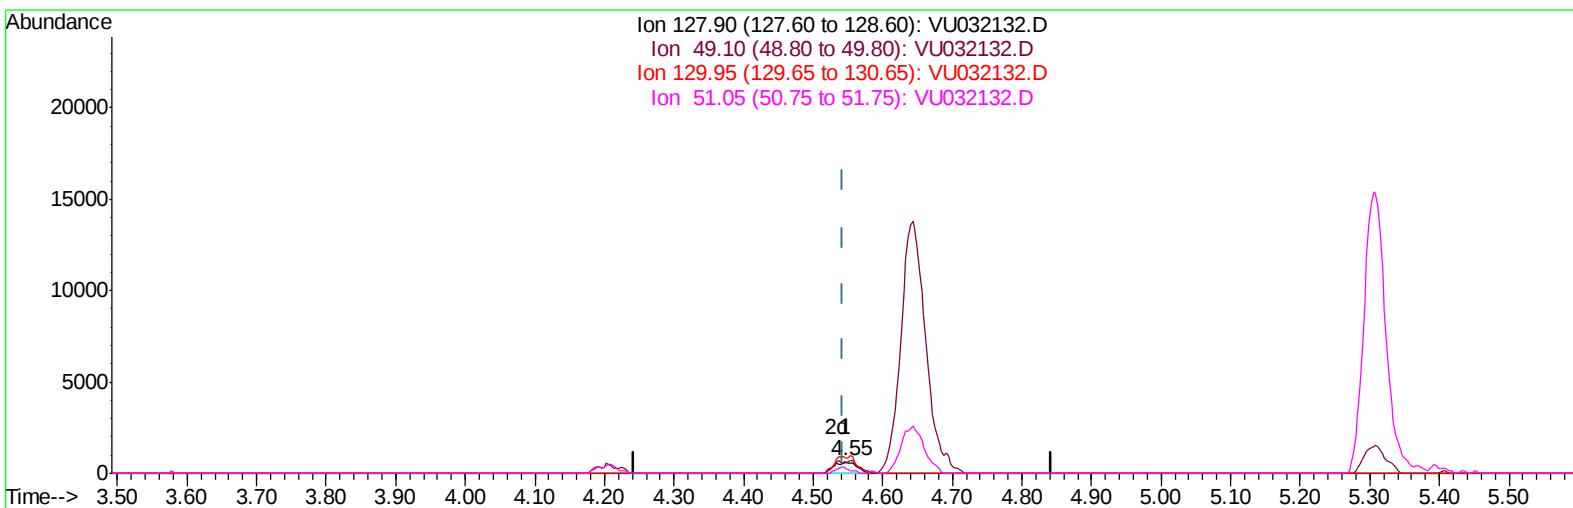

TIC: VU032132.D

(23) Bromochloromethane (T)

4.547min (+0.003) 0.23ug/L m

response 1442

Ion	Exp%	Act%
127.90	100	100
49.10	131.70	90.16#
129.95	129.00	134.84
51.05	44.10	49.38