

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051719\
 Data File : VU032131.D
 Acq On : 18 May 2019 04:36
 Operator : JC/SP
 Sample : K2860-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9W33

Quant Time: May 18 06:30:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 18 05:45:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	364533	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	367031	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	145618	5.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	109212	3.55	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.00%
7) Chloroethane-d5	1.68	69	96235	3.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.40%
11) 1,1-Dichloroethene-d2	2.27	63	158206	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	4.20	46	228767	37.95	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.90%
24) Chloroform-d	4.64	84	220229	4.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.60%
26) 1,2-Dichloroethane-d4	5.31	65	108106	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
32) Benzene-d6	5.33	84	448428	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.00%
36) 1,2-Dichloropropane-d6	6.32	67	131017	4.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.00%
41) Toluene-d8	7.56	98	368282	3.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.60%
43) trans-1,3-Dichloropropene-	7.85	79	41079	3.49	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.80%
46) 2-Hexanone-d5	8.31	63	197067	37.04	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.08%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	108634	4.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.20%
64) 1,2-Dichlorobenzene-d4	11.86	152	138506	4.49	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.80%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Vinyl chloride	1.40	62	13679	0.744	ug/L #	73
12) 1,1-Dichloroethene	2.28	96	8345	0.570	ug/L #	1
13) Acetone	2.33	43	101862	51.469	ug/L	98
17) Methyl tert-butyl Ether	3.00	73	14026	0.408	ug/L #	80
18) trans-1,2-Dichloroethene	2.97	96	32207	2.055	ug/L	98
22) cis-1,2-Dichloroethene	4.22	96	204934	13.294	ug/L	88
30) Cyclohexane	4.98	56	3696	0.188	ug/L #	76
33) Benzene	5.38	78	17447	0.310	ug/L	100
34) Trichloroethene	6.18	95	376952	24.658	ug/L	93
47) Tetrachloroethene	8.22	164	7483	0.655	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051719\  
Data File : VU032131.D  
Acq On    : 18 May 2019   04:36  
Operator  : JC/SP  
Sample    : K2860-06  
Misc      : 25.0mL/MSVOA U/WATER  
ALS Vial  : 35      Sample Multiplier: 1
```

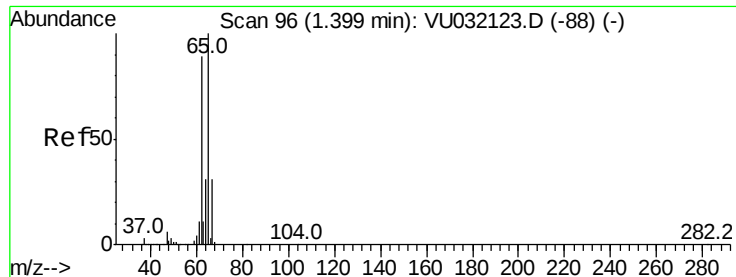

#5

Vinyl chloride

Concen: 0.744 ug/L

RT: 1.40 min Scan# 96

Delta R.T. 0.00 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36

Instrument :

MSVOA_U

ClientSampleId :





F9W33

Tot Ion: 62 Resp: 13679

Ion Ratio Lower Upper

62 100

64 51.0 24.8 46.1#

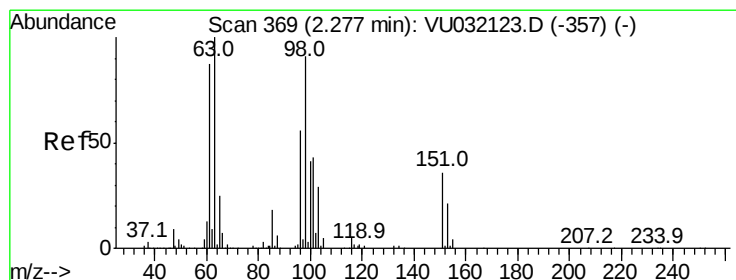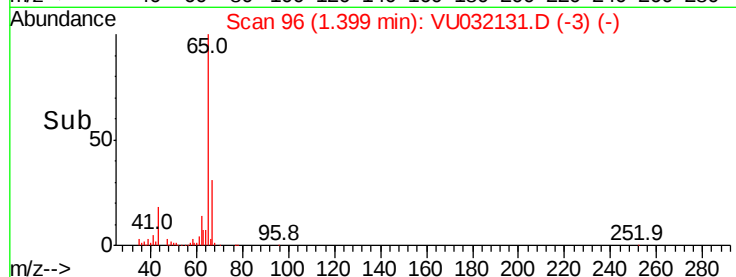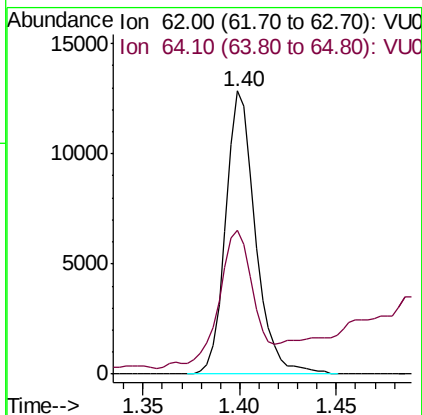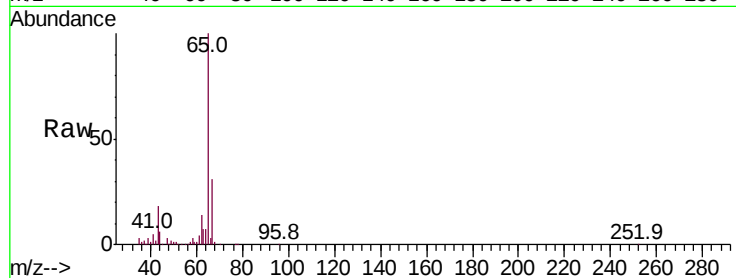

#12

1,1-Dichloroethene

Concen: 0.570 ug/L

RT: 2.28 min Scan# 370

Delta R.T. 0.00 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36




Tgt Ion: 96 Resp: 8345


Ion Ratio Lower Upper

96 100

61 229.1 111.7 207.5#

63 1014.1 152.2 282.6#

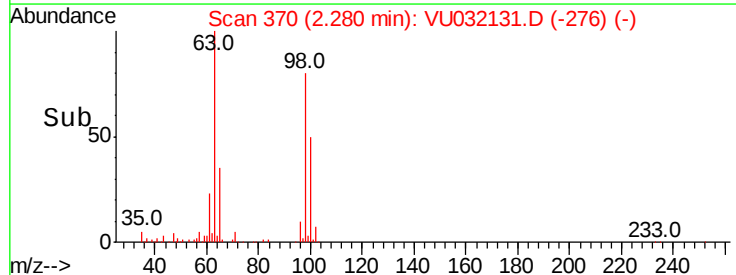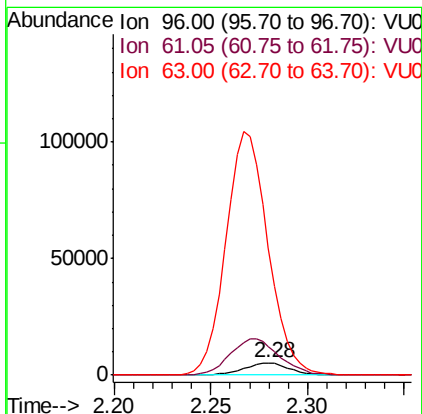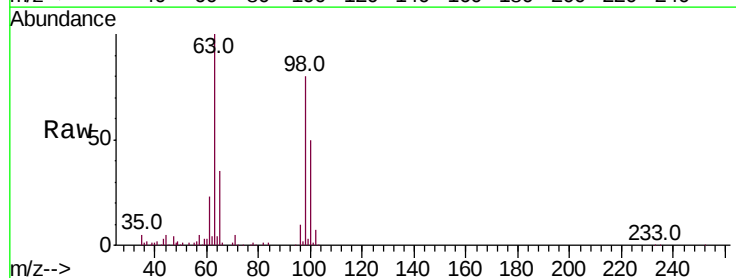

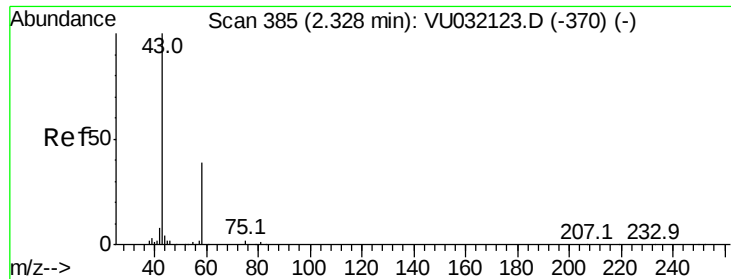

#13

Acetone

Concen: 51.469 ug/L

RT: 2.33 min Scan# 387

Delta R.T. 0.01 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36

Instrument :

MSVOA_U

ClientSampled :





F9W33

Tot Ion: 43 Resp: 101862

Ion Ratio Lower Upper

43 100

58 38.1 0.0 78.8

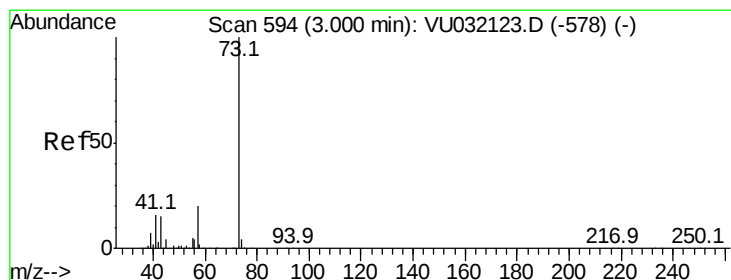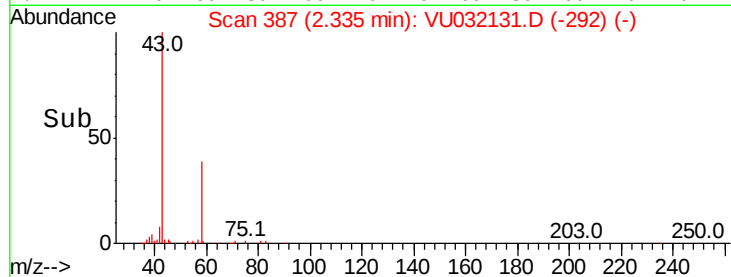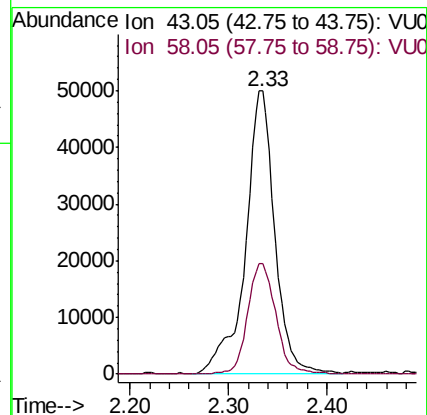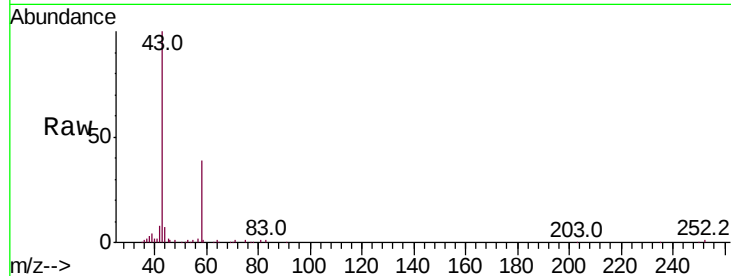

#17

Methyl tert-butyl Ether

Concen: 0.408 ug/L

RT: 3.00 min Scan# 594

Delta R.T. 0.00 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36




Tgt Ion: 73 Resp: 14026


Ion Ratio Lower Upper

73 100

43 23.6 13.0 19.6#

57 33.2 17.9 26.9#

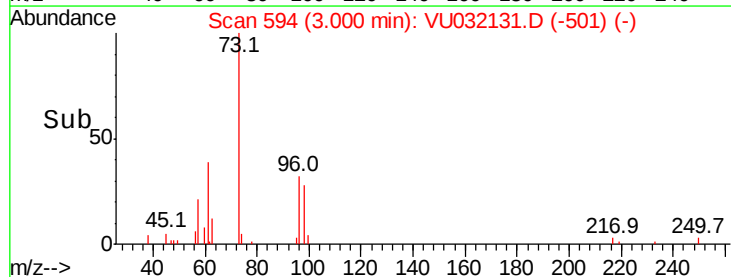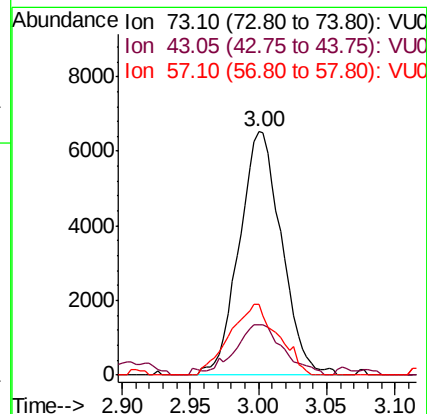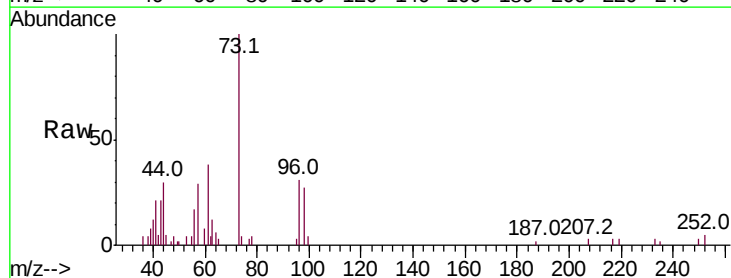

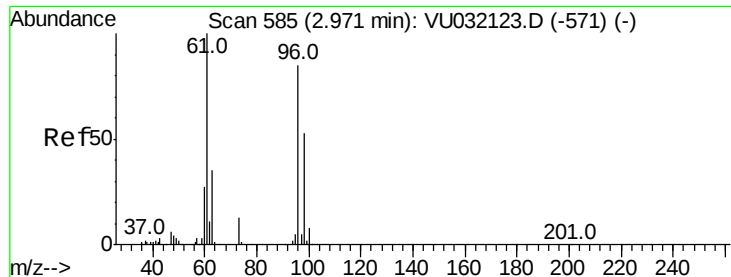

#18

trans-1,2-Dichloroethene

Concen: 2.055 ug/L

RT: 2.97 min Scan# 586

Delta R.T. 0.00 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36

Instrument :

MSVOA_U

ClientSampleId :

F9W33





Tot Ion: 96 Resp: 32207

Ion Ratio Lower Upper

96 100

61 121.1 86.5 160.7

98 62.4 43.5 80.9

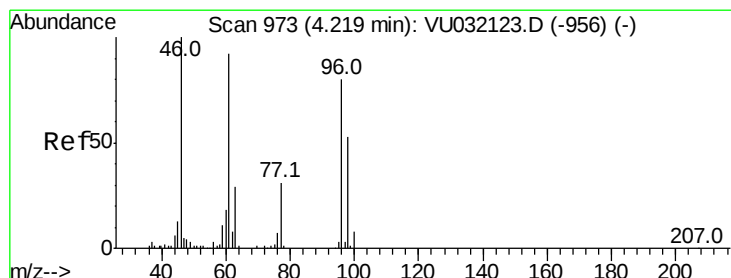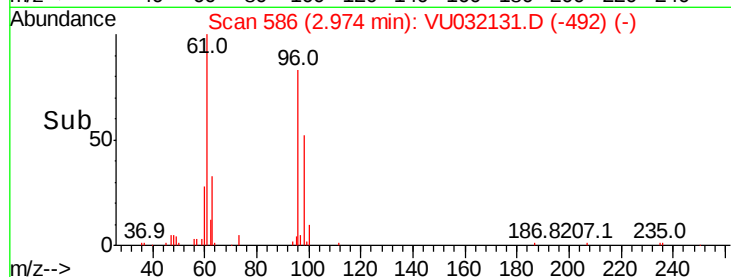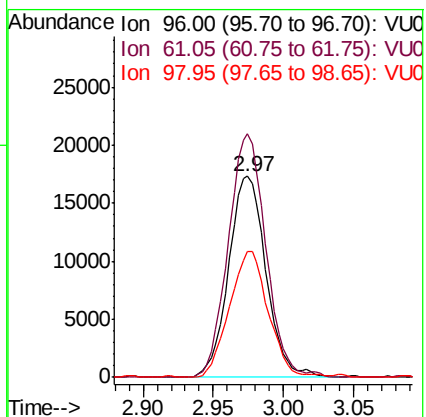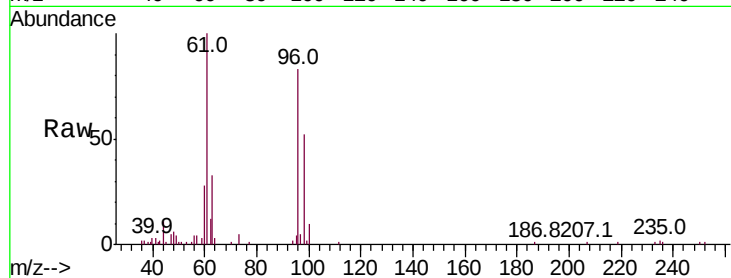

#22

cis-1,2-Dichloroethene

Concen: 13.294 ug/L

RT: 4.22 min Scan# 972

Delta R.T. -0.00 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36




Tgt Ion: 96 Resp: 204934


Ion Ratio Lower Upper

96 100

61 108.6 85.8 159.4

68 0.0 0.0 0.0

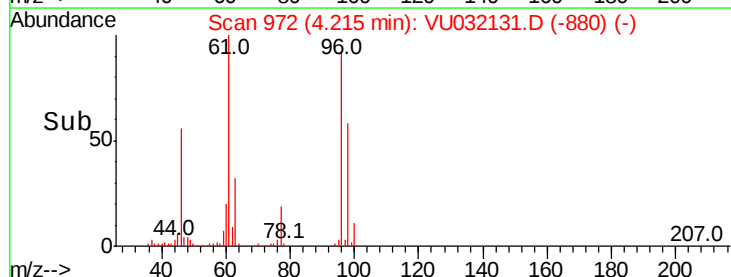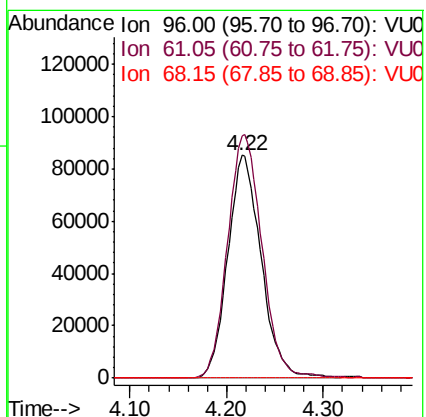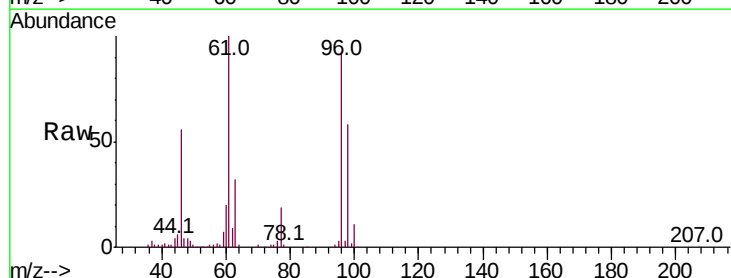


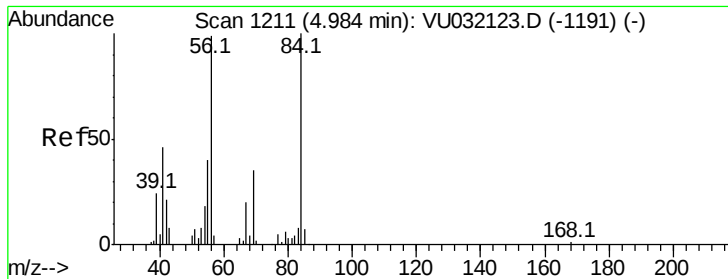




#30
Cyclohexane
Concen: 0.188 ug/L
RT: 4.98 min Scan# 1209
Delta R.T. -0.01 min
Lab File: VU032131.D
Acq: 18 May 2019 04:36

Instrument :
MSVOA_U
ClientSampleId :
F9W33

Tot Ion: 56 Resp: 3696
Ion Ratio Lower Upper
56 100
69 22.1 26.9 40.3#
84 119.9 76.6 115.0#

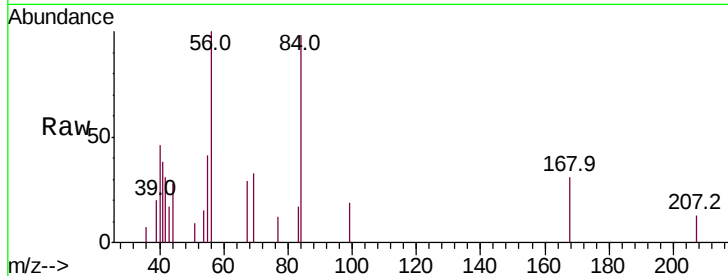


Abundance Ion 56.10 (55.80 to 56.80): VU0
Ion 69.15 (68.85 to 69.85): VU0
Ion 84.15 (83.85 to 84.85): VU0

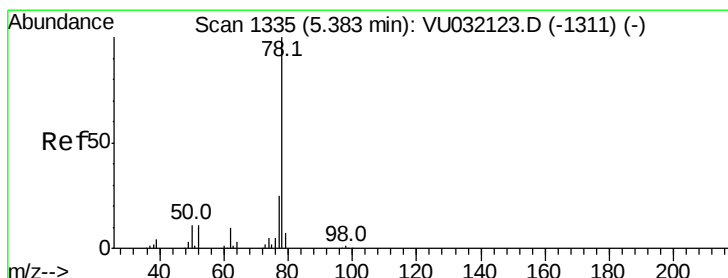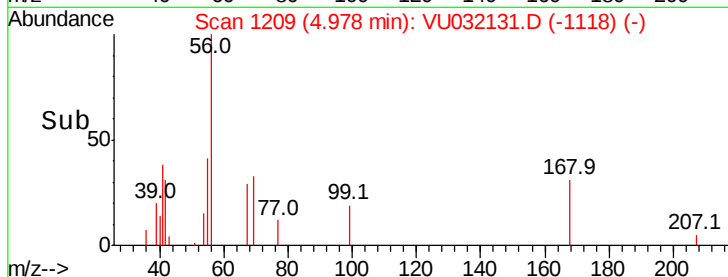
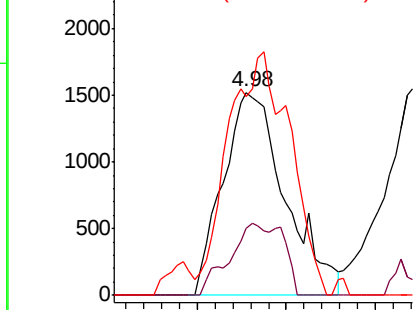



#33
Benzene
Concen: 0.310 ug/L
RT: 5.38 min Scan# 1335
Delta R.T. 0.00 min
Lab File: VU032131.D
Acq: 18 May 2019 04:36

Tgt Ion: 78 Resp: 17447

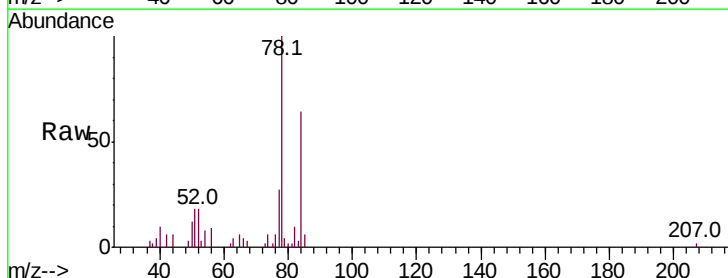

Abundance Ion 78.10 (77.80 to 78.80): VU0

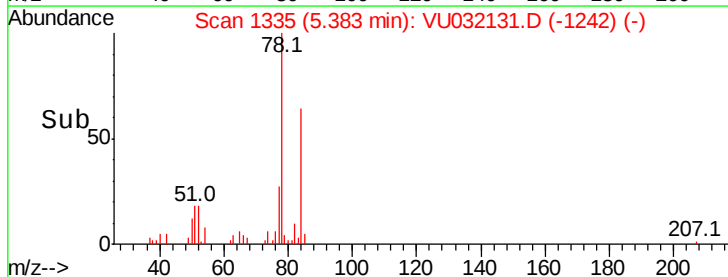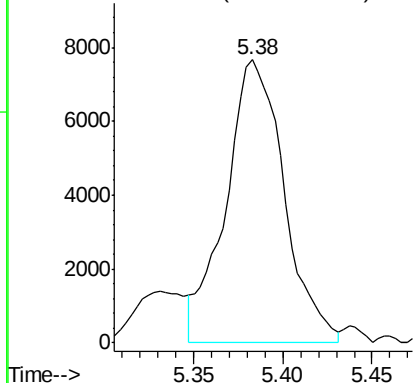

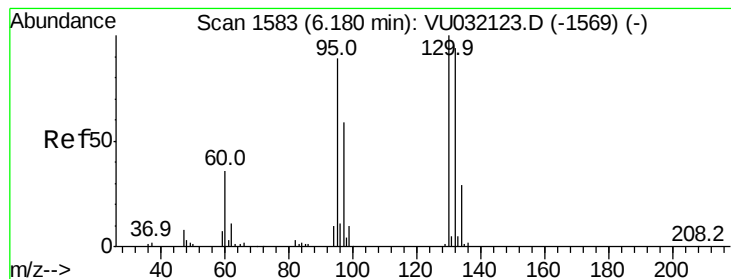

#34

Trichloroethene

Concen: 24.658 ug/L

RT: 6.18 min Scan# 1583

Delta R.T. 0.00 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36

Instrument :

MSVOA_U

ClientSampleId :

F9W33

Tot Ion: 95 Resp: 376952


Ion Ratio Lower Upper

95 100

97 65.3 45.2 84.0

132 104.4 66.1 122.7

130 104.0 66.7 123.9



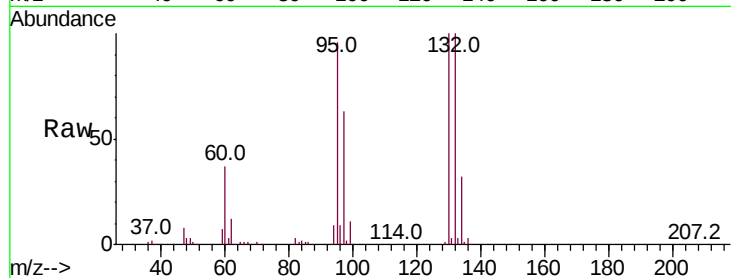


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

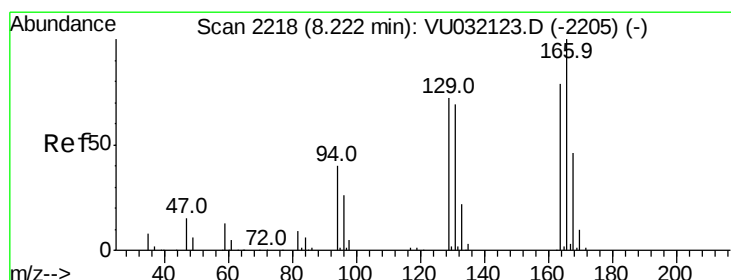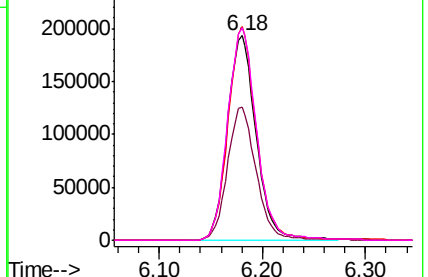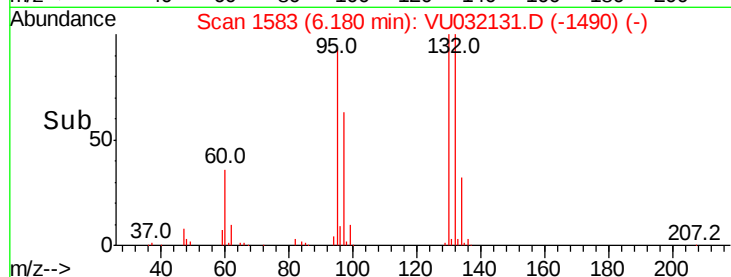

#47

Tetrachloroethene

Concen: 0.655 ug/L

RT: 8.22 min Scan# 2219

Delta R.T. 0.00 min

Lab File: VU032131.D

Acq: 18 May 2019 04:36

Tgt Ion: 164 Resp: 7483


Ion Ratio Lower Upper

164 100

129 82.0 70.3 130.5

131 94.7 64.5 119.9

166 125.0 92.3 171.5

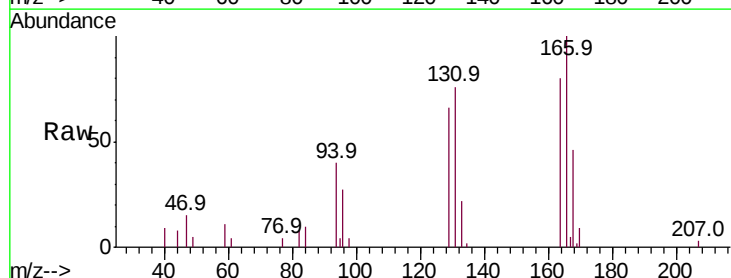

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

