


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051719\
 Data File : VU032099.D
 Acq On : 17 May 2019 14:17
 Operator : JC/SP
 Sample : BFB09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB09

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon May 20 12:58:56 2019

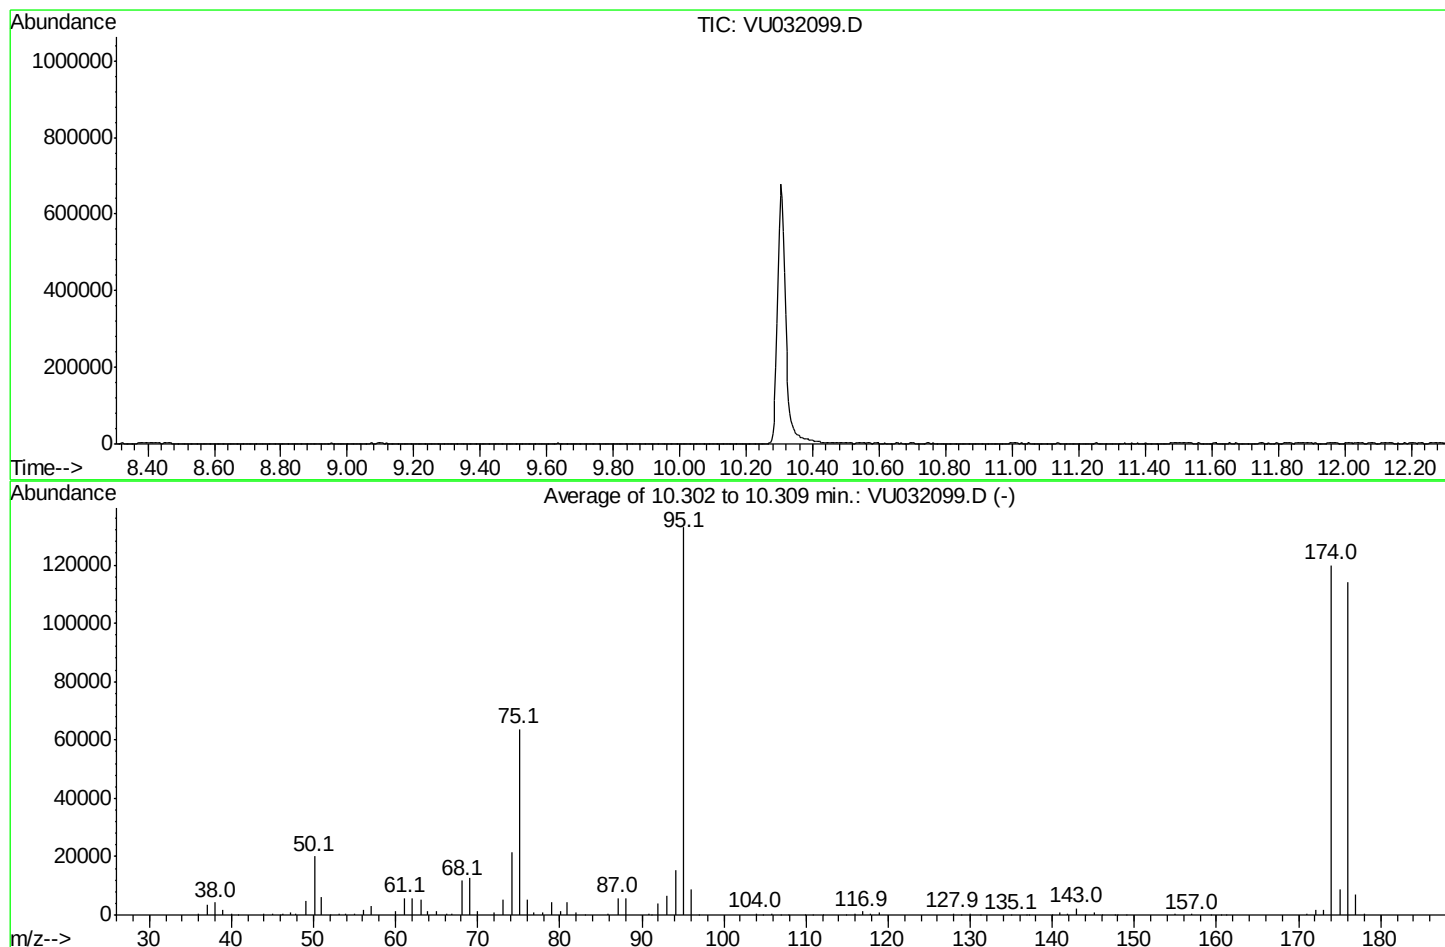

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	20024	PASS
75	95	30	80	47.9	63653	PASS
95	95	100	100	100.0	132872	PASS
96	95	5	9	6.5	8595	PASS
173	174	0.00	2	1.4	1734	PASS
174	95	50	120	90.3	119917	PASS
175	174	5	9	7.4	8908	PASS
176	174	95	101	95.3	114282	PASS
177	176	5	9	6.3	7156	PASS

Scan 2852 (10.260 min): VU032099.D
BFB09

m/z	Abundance
36.00	164.0
39.80	425.0
43.90	658.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.10	692.0
37.10	3460.0
38.00	4184.0
39.00	1741.0
40.10	477.0
44.00	1123.0
45.00	655.0
46.20	340.0
47.10	977.0
47.80	664.0
49.00	4633.0
50.10	20752.0
51.00	6155.0
52.10	224.0
53.10	270.0
53.90	283.0
55.00	272.0
56.10	1650.0
57.00	3037.0
60.00	1228.0
61.10	6104.0
62.00	5670.0
63.10	5663.0
64.00	1455.0
65.00	1463.0
66.20	308.0
66.90	409.0
68.10	11791.0
69.10	12328.0
70.00	1557.0
71.90	707.0
73.10	5289.0
74.10	21632.0
75.10	62712.0
76.00	5291.0
76.90	700.0
77.90	735.0
79.00	4032.0
80.10	1265.0
80.90	4489.0
81.90	1019.0
85.80	151.0
87.00	6121.0
88.00	6164.0
90.80	435.0
92.00	3982.0
93.00	7156.0
94.10	15466.0
95.10	132096.0
96.00	8587.0
97.00	153.0
104.00	520.0
104.70	154.0
105.90	537.0
107.90	130.0
110.90	145.0
112.00	100.0
114.90	190.0
116.00	441.0
116.90	1263.0
117.80	529.0
119.00	798.0
127.90	571.0
128.80	145.0
130.00	434.0
135.00	243.0
137.20	147.0
140.90	889.0
141.90	212.0
143.00	2397.0
145.00	1067.0
146.00	249.0
148.00	237.0
149.00	194.0
154.90	288.0
157.00	299.0
159.30	118.0
160.60	130.0
170.90	388.0
172.00	2059.0
173.10	2326.0
174.00	114720.0
175.10	8276.0
176.00	111928.0
177.00	6928.0
178.00	320.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.10	745.0
37.10	3520.0
38.00	4475.0
39.00	1721.0
40.10	431.0
40.80	159.0
43.90	1381.0
45.00	572.0
46.20	270.0
47.10	1098.0
47.90	599.0
49.00	5159.0
50.10	20768.0
51.00	6109.0
52.10	245.0
53.10	271.0
53.80	290.0
55.10	353.0
56.10	1631.0
57.00	3158.0
60.00	1283.0
61.10	5835.0
62.00	5613.0
63.10	5583.0
64.00	1307.0
65.00	1507.0
66.20	266.0
66.90	394.0
68.10	12082.0
69.10	13098.0
70.00	1610.0
72.00	829.0
73.10	5698.0
74.10	22208.0
75.10	65848.0
76.00	5534.0
76.90	767.0
78.00	780.0
79.00	4384.0
80.00	1194.0
80.90	4650.0
81.90	993.0
83.00	121.0
85.90	297.0
87.00	5881.0
88.00	5972.0
90.80	480.0
92.00	4031.0
93.00	6615.0
94.10	15902.0
95.10	136960.0
96.00	8849.0
97.00	159.0
104.00	638.0
104.80	164.0
105.90	543.0
106.90	103.0
107.80	100.0
110.90	186.0
114.90	178.0
116.00	526.0
116.90	1244.0
117.80	607.0
119.00	797.0
127.90	698.0
128.90	151.0
130.00	505.0
135.10	237.0
136.80	133.0
137.10	124.0
140.00	101.0
140.90	1022.0
141.90	263.0
143.00	2322.0
145.10	990.0
146.00	207.0
147.60	188.0
147.90	164.0
149.00	163.0
155.00	249.0
157.00	396.0
160.60	166.0
171.00	502.0
172.10	2014.0
173.10	2876.0
174.00	124576.0
175.10	9144.0
176.00	117696.0
177.00	7403.0
178.00	337.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09

m/z	Abundance
36.00	751.0
37.10	3364.0
38.10	4278.0
39.00	1652.0
40.00	428.0
40.80	186.0
43.90	1429.0
45.00	569.0
45.90	124.0
46.30	177.0
47.20	1010.0
47.90	595.0
49.00	4996.0
50.10	18552.0
51.00	5764.0
52.10	208.0
53.00	264.0
53.80	223.0
55.10	379.0
56.10	1387.0
57.00	3008.0
60.00	1179.0
61.10	5225.0
62.10	5356.0
63.00	5021.0
63.90	957.0
65.00	1278.0
66.20	172.0
66.90	298.0
68.10	11575.0
69.10	12533.0
70.00	1434.0
72.00	898.0
73.10	5497.0
74.10	20440.0
75.10	62400.0
76.00	5141.0
76.90	777.0
77.90	657.0
79.00	4429.0
80.00	1058.0
80.90	4517.0
82.00	791.0
83.00	127.0
85.90	417.0
87.10	5421.0
88.00	5276.0
90.80	418.0
91.20	367.0
92.00	3548.0
93.00	5667.0
94.10	14734.0
95.10	129560.0
96.00	8350.0
97.00	166.0
103.90	644.0
104.80	152.0
105.90	519.0
107.00	114.0
109.90	117.0
110.80	167.0
114.90	185.0
116.00	516.0
116.90	1051.0
117.90	546.0
119.00	743.0
127.90	678.0
129.00	166.0
130.00	512.0
131.20	155.0
135.10	219.0
136.80	173.0
140.00	120.0
141.00	1057.0
141.80	262.0
143.00	2105.0
144.00	215.0
145.10	860.0
146.00	244.0
147.60	246.0
155.00	213.0
157.00	396.0
160.60	132.0
161.10	108.0
171.10	500.0
172.00	1735.0
174.00	120456.0
175.10	9304.0
176.00	113224.0
177.00	7138.0
178.00	275.0

Instrument :
MSVOA_U
ClientSampleId :
BFB09