

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051721\
 Data File : VU043782.D
 Acq On : 17 May 2021 10:30
 Operator : SY/MD
 Sample : VU0517WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK151

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	97	rBV	117342	132318	16.23%	1.996%
2	1.919	172	180	190	rVB	84346	105748	12.97%	1.595%
3	2.575	371	384	401	rBV	189450	308026	37.77%	4.646%
4	3.054	522	533	546	rBV3	6270	11349	1.39%	0.171%
5	4.649	1012	1029	1058	rBV	71560	244235	29.95%	3.684%
6	5.073	1145	1161	1181	rBV2	145425	320876	39.35%	4.840%
7	5.736	1345	1367	1404	rBV2	309456	796990	97.73%	12.022%
8	6.260	1513	1530	1551	rBV	270744	521355	63.93%	7.864%
9	6.700	1652	1667	1688	rBV	185450	364154	44.65%	5.493%
10	7.575	1923	1939	1957	rBV2	92021	164328	20.15%	2.479%
11	7.906	2028	2042	2056	rBV	371088	640395	78.53%	9.660%
12	7.973	2058	2063	2082	rVB2	6274	11939	1.46%	0.180%
13	8.189	2118	2130	2153	rBV	58167	102573	12.58%	1.547%
14	8.645	2258	2272	2313	rBV	346320	815495	100.00%	12.301%
15	9.424	2500	2514	2550	rBV	393158	663176	81.32%	10.003%
16	10.764	2919	2931	2947	rBV	145768	240373	29.48%	3.626%
17	11.819	3246	3259	3277	rBV	387427	614617	75.37%	9.271%
18	12.202	3362	3378	3394	rBV	340086	562014	68.92%	8.478%
19	14.095	3956	3967	3977	rBV	6642	9484	1.16%	0.143%




Sum of corrected areas: 6629445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051721\
Data File : VU043782.D
Acq On : 17 May 2021 10:30
Operator : SY/MD
Sample : VU0517WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

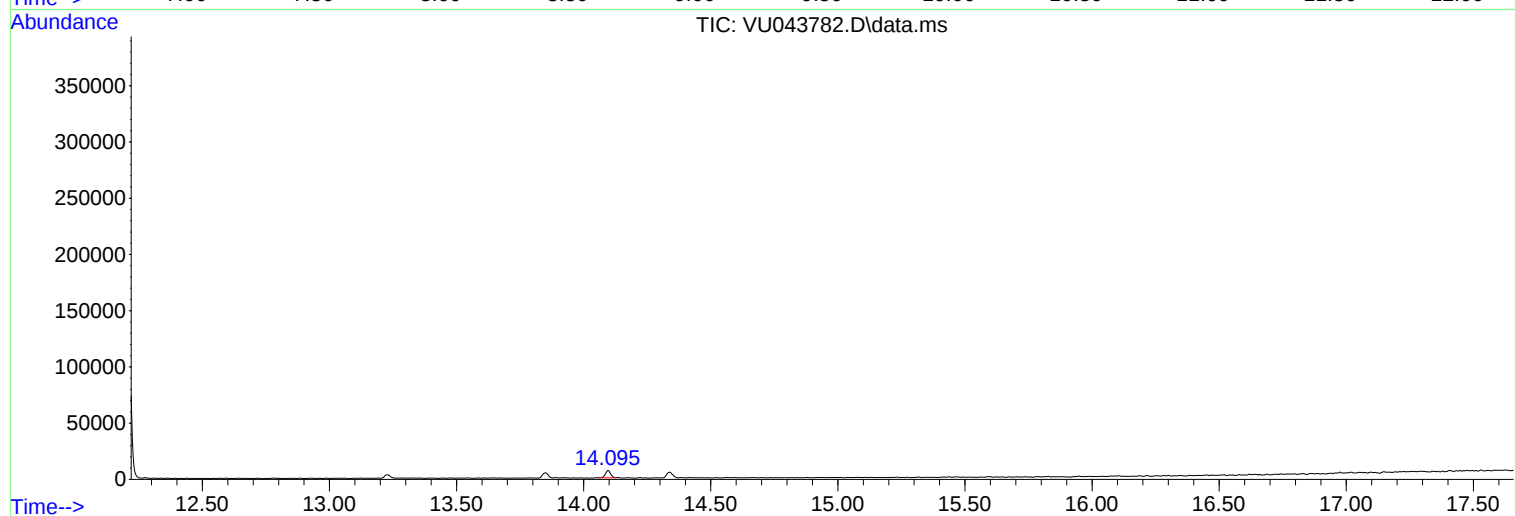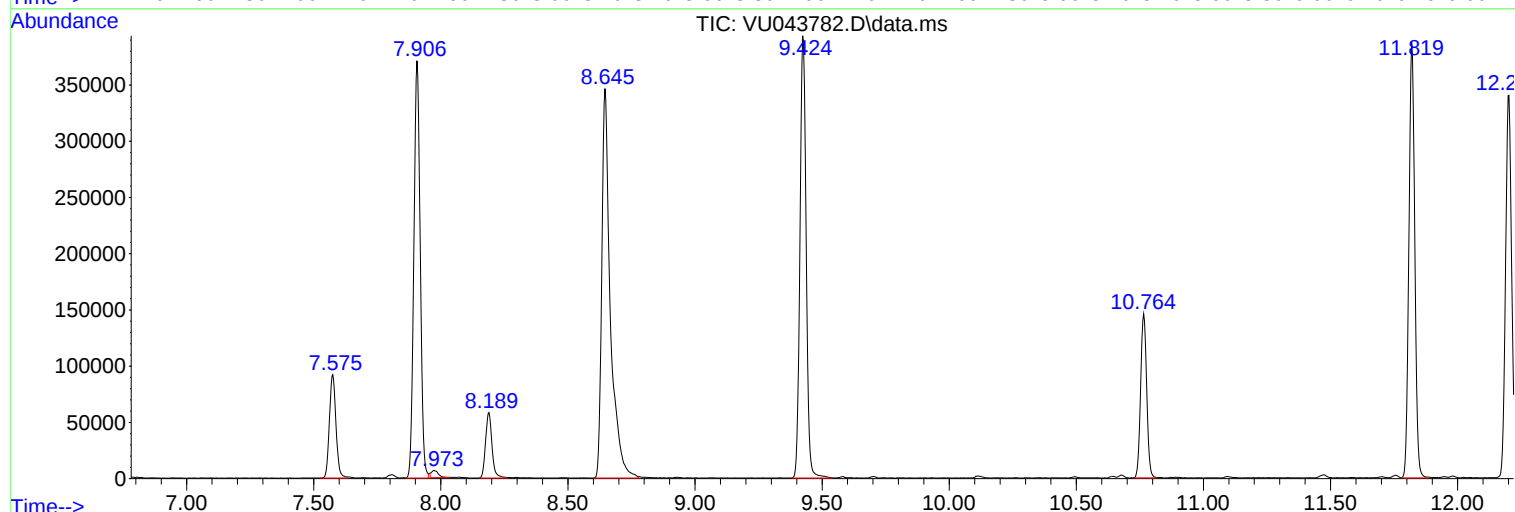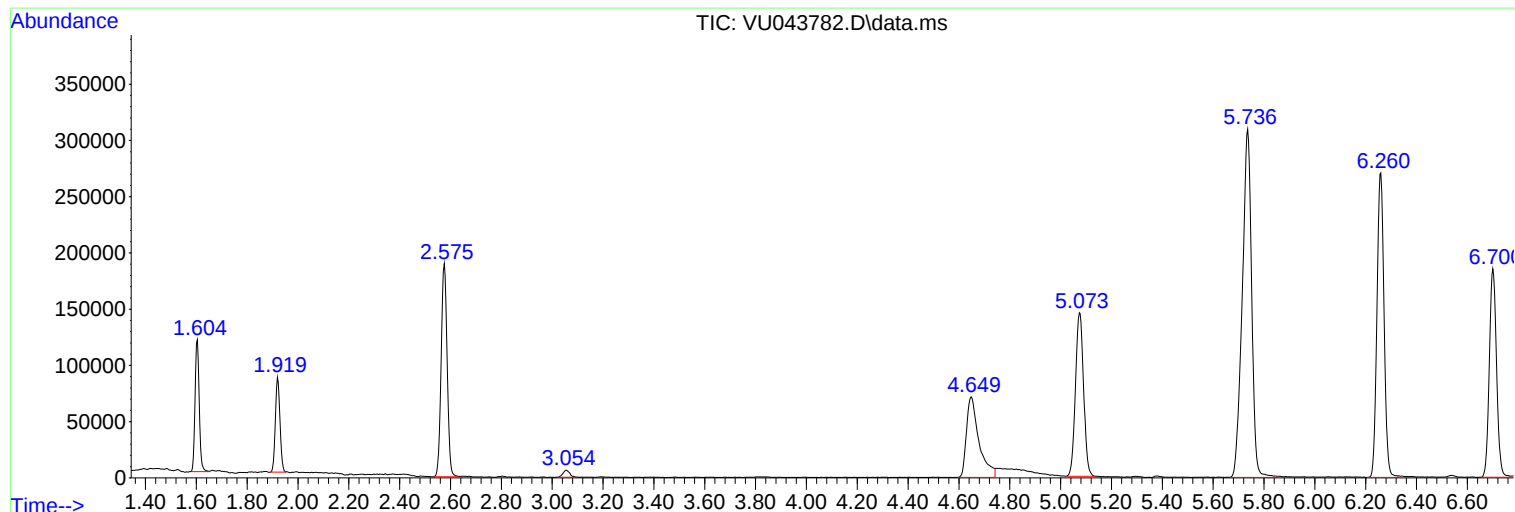

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051721\
Data File : VU043782.D
Acq On : 17 May 2021 10:30
Operator : SY/MD
Sample : VU0517WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051721\
Data File : VU043782.D
Acq On : 17 May 2021 10:30
Operator : SY/MD
Sample : VU0517WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK151

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
