
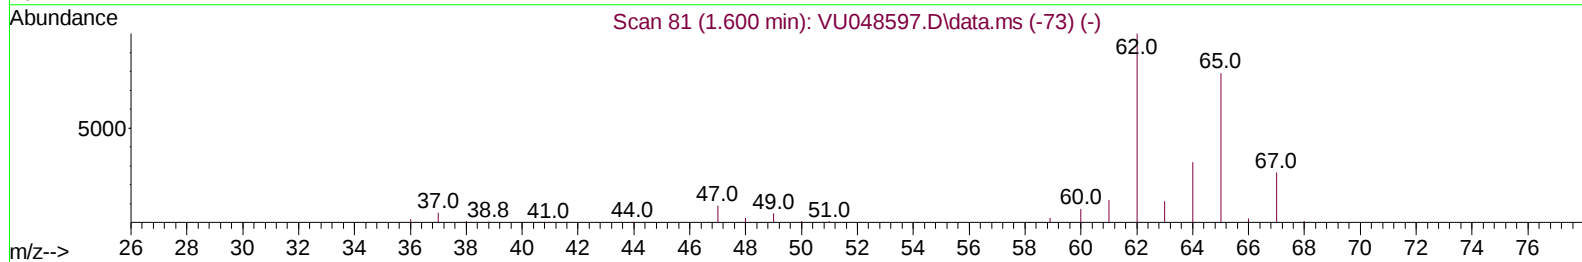
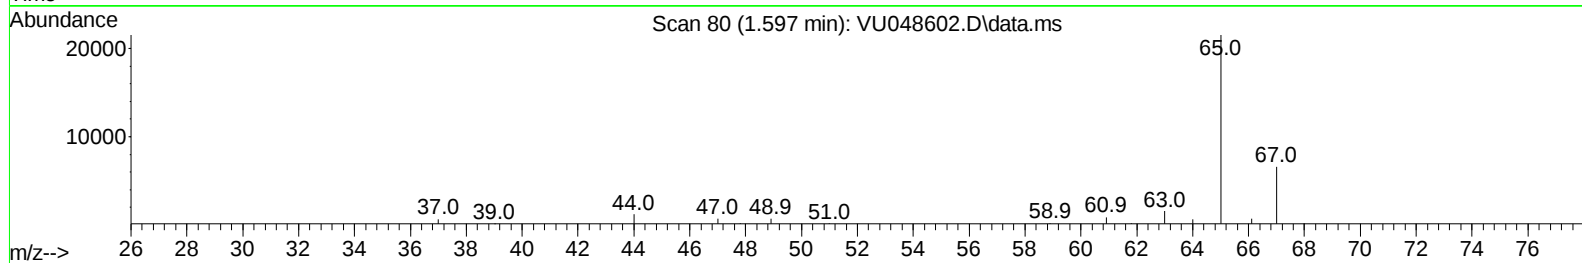


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051722\
 Data File : VU048602.D
 Acq On : 17 May 2022 15:25
 Operator : SY/MD
 Sample : N2766-18ME
 Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 18 05:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 18 05:17:36 2022
 Response via : Initial Calibration

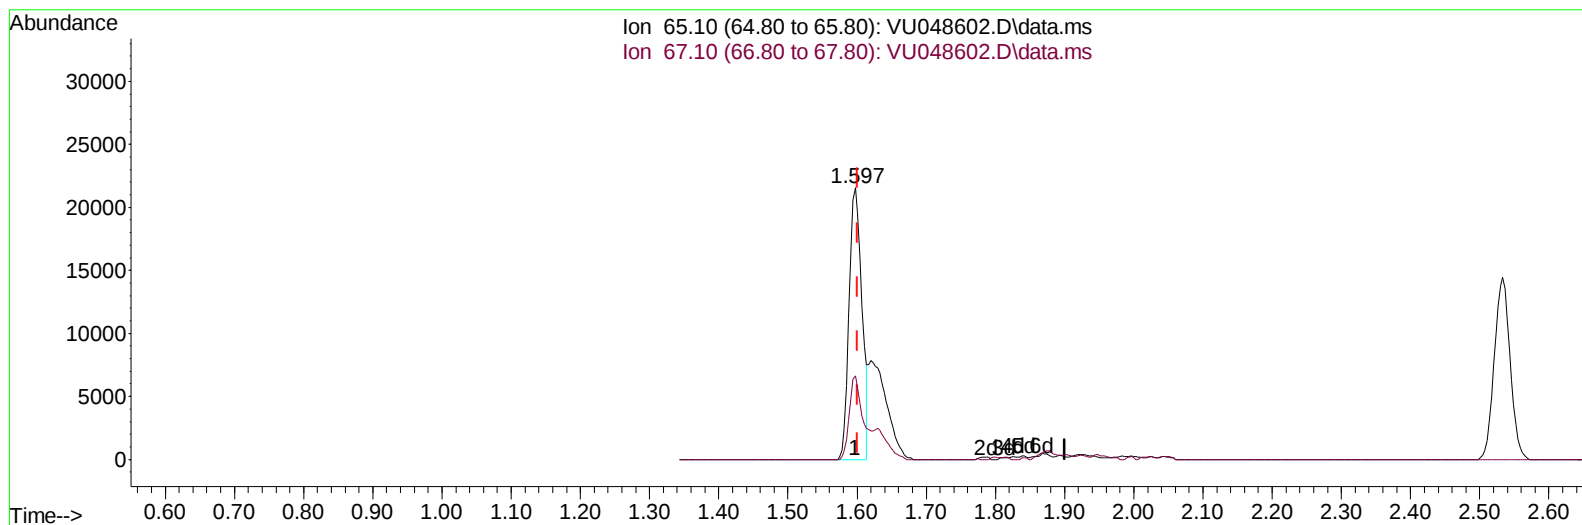




TIC: VU048602.D\data.ms

(4) Vinyl Chloride-d3 (S)**1.597min (-0.003) 20.08 ug/L****response 27676**

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	33.70	32.83
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051722\
 Data File : VU048602.D
 Acq On : 17 May 2022 15:25
 Operator : SY/MD
 Sample : N2766-18ME
 Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 18 05:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 18 05:17:36 2022
 Response via : Initial Calibration

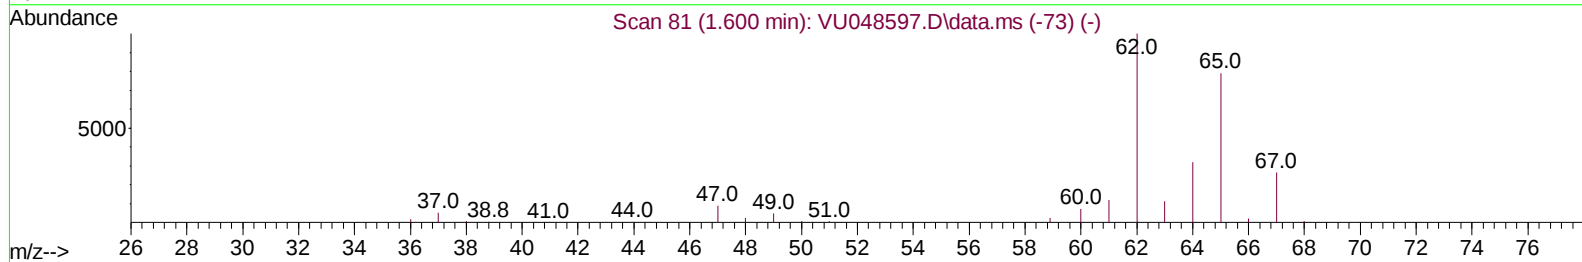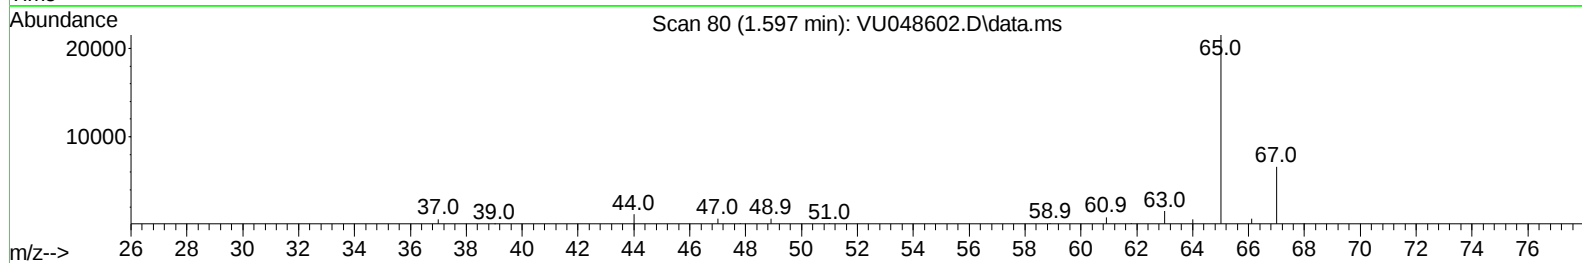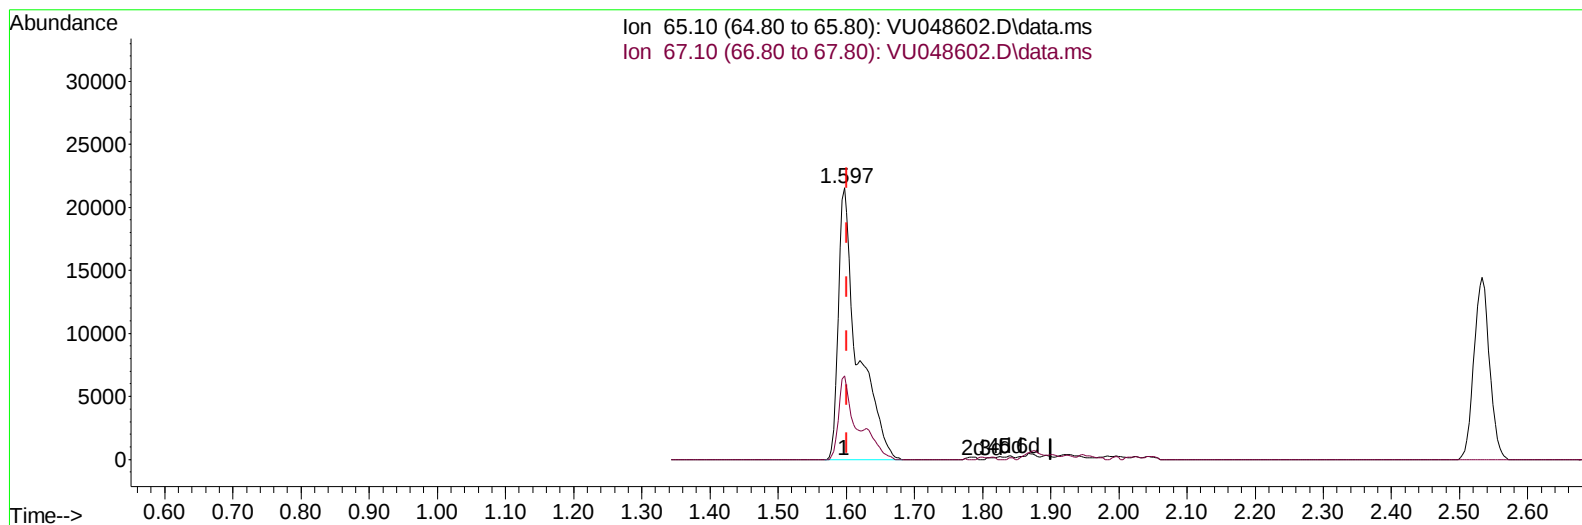




TIC: VU048602.D\data.ms

(4) Vinyl Chloride-d3 (S)**1.597min (-0.003) 30.66 ug/L m****response 42271**

Ion	Exp%	Act%
65.10	100.00	100.00
67.10	33.70	21.49#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051722\
Data File : VU048602.D
Acq On : 17 May 2022 15:25
Operator : SY/MD
Sample : N2766-18ME
Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 18 05:19:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 18 05:17:36 2022
Response via : Initial Calibration

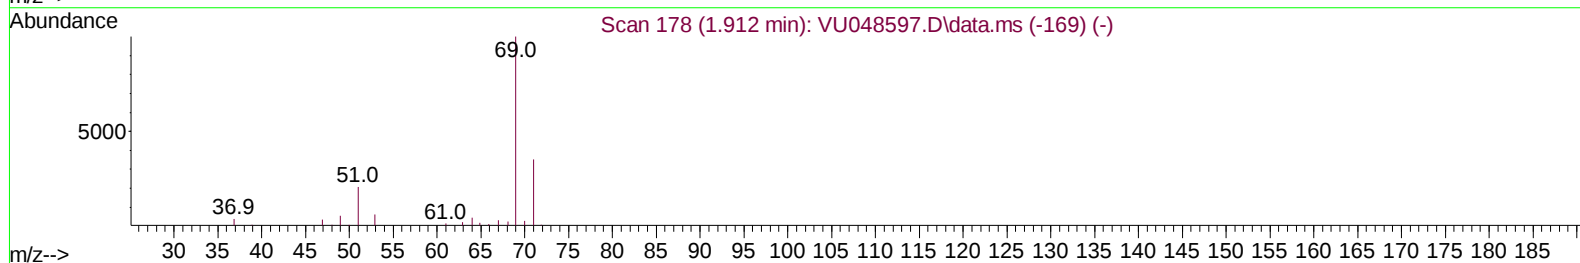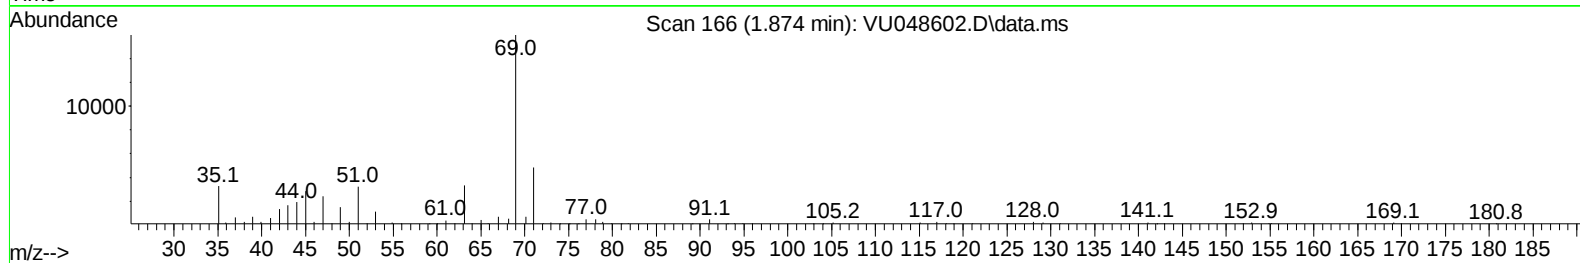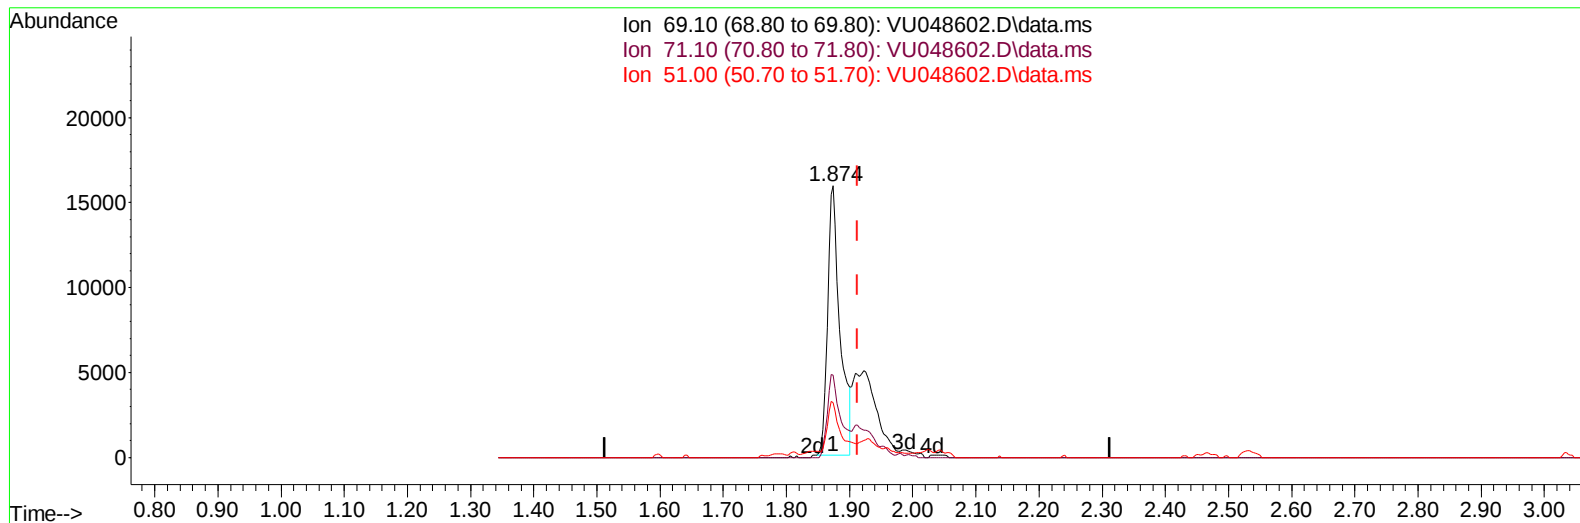

TIC: VU048602.D\data.ms

(7) Chloroethane-d5 (S)




1.874min (-0.038) 20.91 ug/L

response 21597

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.70	34.39
51.00	26.90	18.90
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051722\
Data File : VU048602.D
Acq On : 17 May 2022 15:25
Operator : SY/MD
Sample : N2766-18ME
Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 18 05:19:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 18 05:17:36 2022
Response via : Initial Calibration

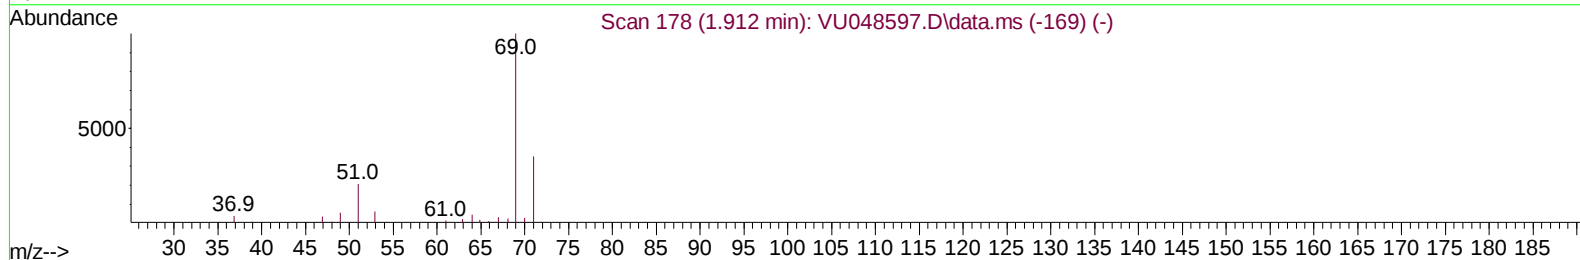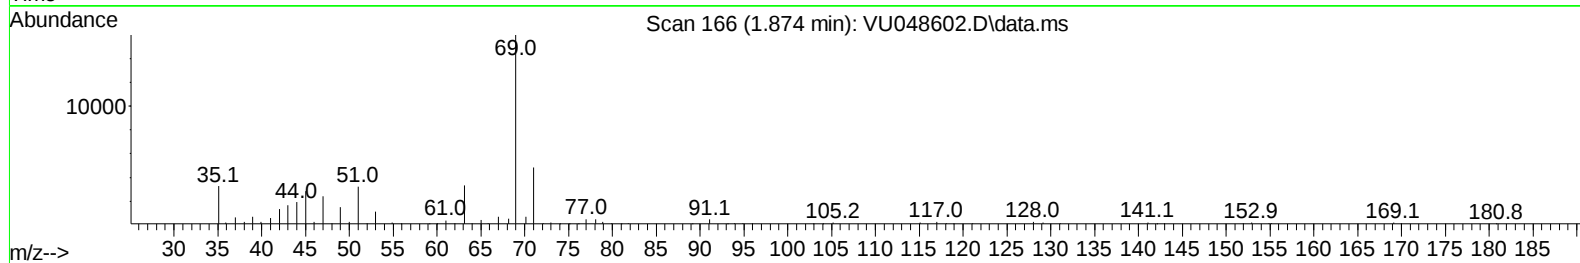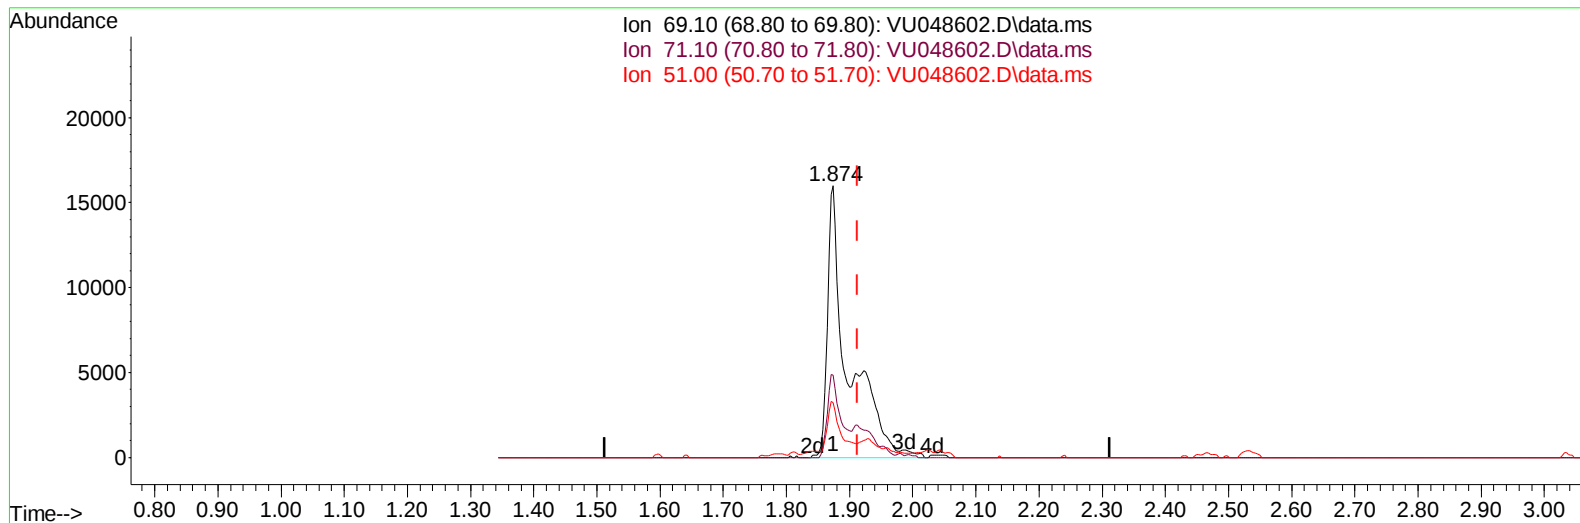

TIC: VU048602.D\data.ms

(7) Chloroethane-d5 (S)

1.874min (-0.038) 35.28 ug/L m

response 36437

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.70	20.39#
51.00	26.90	11.20#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051722\
 Data File : VU048602.D
 Acq On : 17 May 2022 15:25
 Operator : SY/MD
 Sample : N2766-18ME
 Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 18 05:19:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 18 05:17:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	225075	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	231601	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	141348	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	42271m	30.663	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	61.320%	
7) Chloroethane-d5	1.874	69	36437m	35.279	ug/L	-0.04
Spiked Amount 50.000	Range 70	- 130	Recovery	=	70.560%	
11) 1,1-Dichloroethene-d2	2.533	63	70336	22.560	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery	=	45.120%#	
21) 2-Butanone-d5	4.633	46	120502	91.854	ug/L	0.01
Spiked Amount 100.000	Range 40	- 130	Recovery	=	91.850%	
24) Chloroform-d	5.064	84	132603	38.065	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	76.120%	
26) 1,2-Dichloroethane-d4	5.700	65	100254	40.792	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	81.580%	
32) Benzene-d6	5.719	84	224659	34.855	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	69.700%#	
36) 1,2-Dichloropropane-d6	6.687	67	70385	37.197	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	74.400%	
41) Toluene-d8	7.896	98	211743	34.925	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	69.840%#	
43) trans-1,3-Dichloroprop...	8.182	79	43672	36.092	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	72.180%	
47) 2-Hexanone-d5	8.655	63	92983	89.602	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.600%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	133098	42.508	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.020%	
66) 1,2-Dichlorobenzene-d4	12.198	152	110355	38.191	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	76.380%#	
Target Compounds						
					Qvalue	
13) Acetone	2.642	43	2538	2.381	ug/L	49
22) 2-Butanone	4.716	43	15504	11.457	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051722\
Data File : VU048602.D
Acq On : 17 May 2022 15:25
Operator : SY/MD
Sample : N2766-18ME
Misc : 5.63g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 18 05:19:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 18 05:17:36 2022
Response via : Initial Calibration

