


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051722\
 Data File : VU048596.D
 Acq On : 17 May 2022 09:08
 Operator : SY/MD
 Sample : BFB088
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis
 Last Update : Fri May 20 04:37:51 2022

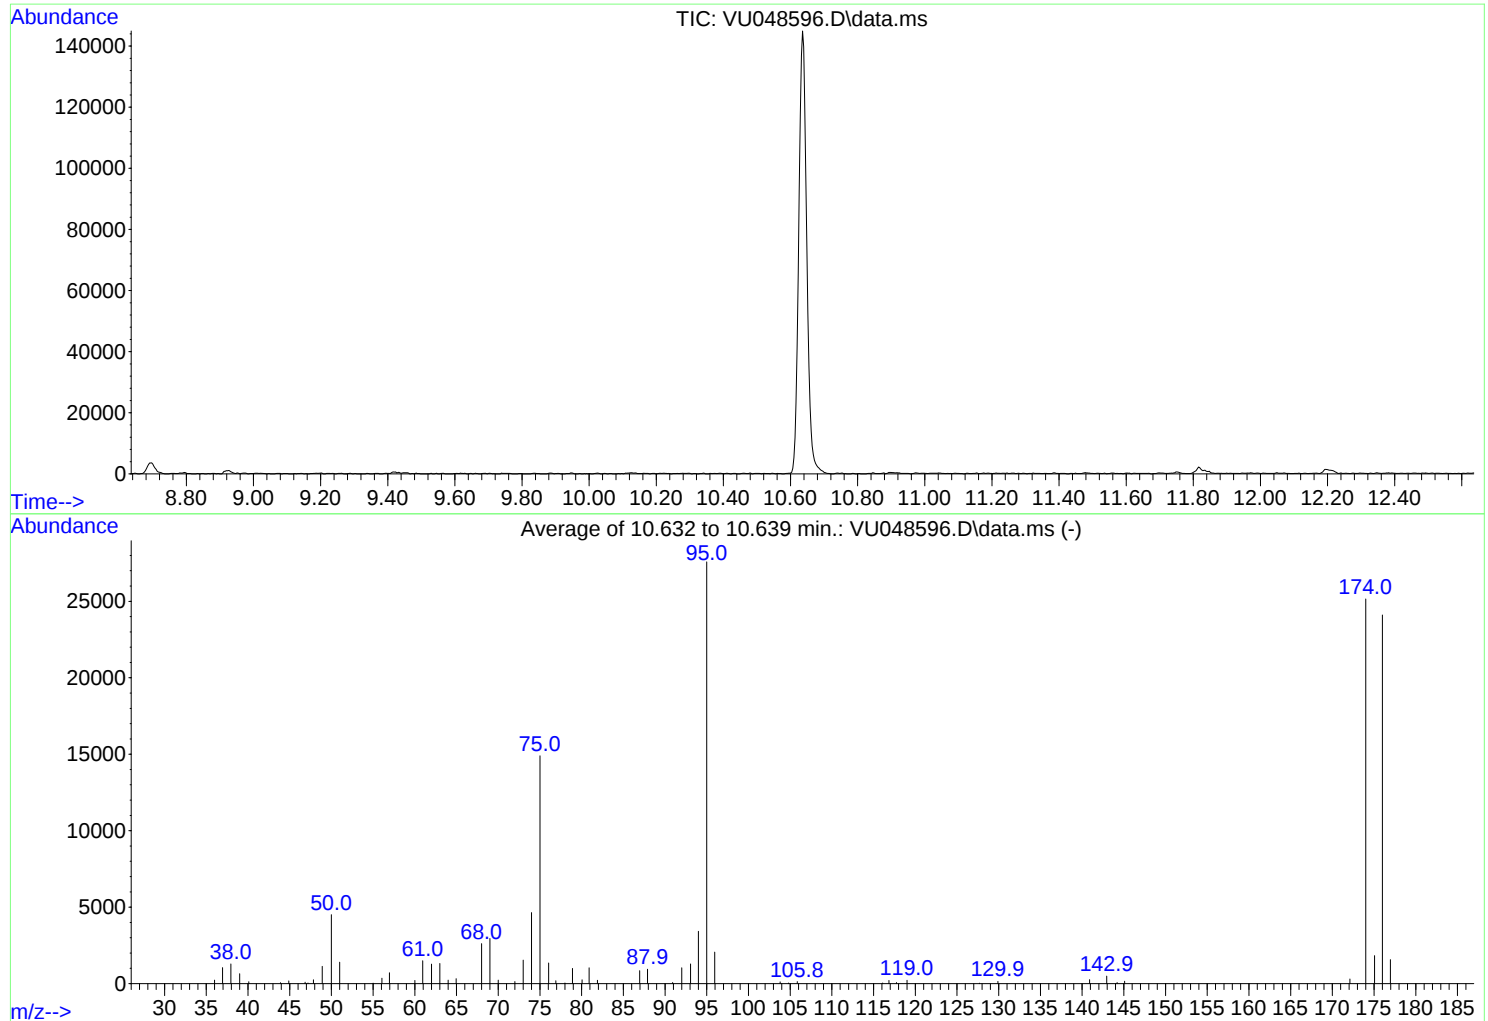

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	4508	PASS
75	95	30	80	54.0	14901	PASS
95	95	100	100	100.0	27581	PASS
96	95	5	9	7.5	2063	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.2	25147	PASS
175	174	5	9	7.3	1827	PASS
176	174	95	101	95.9	24109	PASS
177	176	5	9	6.5	1569	PASS

Scan 2879 (10.597 min): VU048596.D\data.ms
BFB088

m/z	Abundance
43.90	204.0

m/z	Abundance
36.00	186.0
36.90	1016.0
37.90	1235.0
39.00	607.0
40.10	120.0
43.90	234.0
44.90	227.0
46.80	159.0
47.80	283.0
48.90	1106.0
50.00	4530.0
51.00	1351.0
55.00	108.0
56.00	364.0
57.00	789.0
60.10	247.0
61.00	1524.0
62.00	1295.0
63.00	1213.0
64.00	206.0
64.90	323.0
68.00	2536.0
69.00	2768.0
70.00	221.0
72.00	178.0
73.00	1468.0
74.00	4641.0
75.00	14324.0
76.00	1232.0
76.90	188.0
78.00	126.0
78.90	1054.0
80.10	241.0
80.90	942.0
81.80	208.0
86.90	704.0
87.90	1044.0
92.00	938.0
93.00	1245.0
94.00	3280.0
95.00	26872.0
96.00	1918.0
105.80	136.0
116.10	114.0
116.80	247.0
117.80	127.0
119.00	227.0
129.90	142.0
140.90	249.0
142.90	463.0
145.10	150.0
172.10	280.0
174.00	24888.0
175.10	1679.0
176.00	23328.0
177.00	1530.0

m/z	Abundance
36.00	246.0
37.00	1058.0
38.00	1323.0
39.00	692.0
40.10	142.0
44.00	262.0
44.90	184.0
46.90	120.0
47.80	266.0
48.90	1189.0
50.00	4663.0
51.00	1451.0
56.10	344.0
57.00	724.0
60.00	210.0
61.00	1582.0
62.00	1316.0
63.00	1335.0
64.00	224.0
65.00	336.0
68.00	2706.0
69.00	3042.0
70.00	242.0
72.00	130.0
73.00	1619.0
74.00	4719.0
75.00	15361.0
76.00	1401.0
76.90	230.0
78.90	1003.0
80.00	251.0
80.90	1061.0
81.90	210.0
87.00	846.0
87.90	959.0
90.90	108.0
92.00	1102.0
93.10	1305.0
94.00	3522.0
95.00	28528.0
95.90	2131.0
103.80	153.0
105.90	155.0
116.80	200.0
117.70	103.0
119.00	242.0
129.90	141.0
140.90	255.0
142.90	514.0
144.20	103.0
145.10	180.0
172.10	314.0
174.00	25976.0
175.00	1875.0
176.00	24936.0
176.90	1610.0

m/z	Abundance
36.00	267.0
37.00	1057.0
38.00	1293.0
39.00	636.0
40.10	112.0
44.00	318.0
44.80	134.0
47.20	116.0
47.90	194.0
48.90	1100.0
50.00	4332.0
51.00	1416.0
56.10	372.0
56.90	610.0
59.90	184.0
60.90	1377.0
62.00	1214.0
63.00	1416.0
64.00	255.0
65.00	317.0
68.00	2603.0
69.00	3040.0
70.00	233.0
72.00	103.0
73.00	1528.0
74.00	4565.0
75.00	15017.0
76.10	1401.0
76.90	161.0
78.90	929.0
80.00	265.0
80.90	1089.0
82.00	254.0
87.00	983.0
87.90	807.0
90.90	127.0
92.00	1053.0
93.10	1310.0
94.00	3460.0
95.00	27344.0
95.90	2141.0
103.80	180.0
104.80	113.0
105.90	119.0
116.90	185.0
119.00	207.0
127.70	105.0
129.90	161.0
140.90	284.0
143.00	505.0
144.20	126.0
145.10	157.0
172.10	327.0
174.00	24576.0
175.00	1927.0
176.00	24064.0
176.90	1568.0