

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU051820\
 Data File : VU038215.D
 Acq On : 18 May 2020 13:16
 Operator : JC/MD
 Sample : L2657-01DL 5X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFST4DL

Quant Time: May 18 22:55:08 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon May 18 22:23:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	381706	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	374275	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	179127	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	119071	3.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.20%
7) Chloroethane-d5	1.92	69	106068	3.51	ug/L	-0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.20%
11) 1,1-Dichloroethene-d2	2.58	63	147174	2.52	ug/L	-0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.40%#
20) 2-Butanone-d5	4.67	46	446190	51.80	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.60%
24) Chloroform-d	5.10	84	209014	3.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.80%
26) 1,2-Dichloroethane-d4	5.74	65	131994	4.35	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.00%
32) Benzene-d6	5.76	84	429949	3.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.60%
36) 1,2-Dichloropropane-d6	6.72	67	150638	4.16	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.20%
41) Toluene-d8	7.92	98	370938	3.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.60%
43) trans-1,3-Dichloropropene-	8.20	79	57078	3.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.80%
46) 2-Hexanone-d5	8.66	63	347799	50.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.58%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	131305	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	148217	4.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.00%

Target Compounds


					Ovalue
2) Dichlorodifluoromethane	1.39	85	6511	0.187 ug/L	99
9) Trichlorofluoromethane	2.14	101	44284	1.051 ug/L	97
12) 1,1-Dichloroethene	2.59	96	5204	0.196 ug/L #	1
17) Methyl tert-butyl Ether	3.40	73	9166	0.125 ug/L	94
22) cis-1,2-Dichloroethene	4.70	96	24000	0.770 ug/L	99
34) Trichloroethene	6.57	95	221432	7.387 ug/L	99
47) Tetrachloroethene	8.57	164	156504	7.464 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU051820\
Data File : VU038215.D
Acq On : 18 May 2020 13:16
Operator : JC/MD
Sample : L2657-01DL 5X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFST4DL

Quant Time: May 18 22:55:08 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon May 18 22:23:30 2020
Response via : Initial Calibration

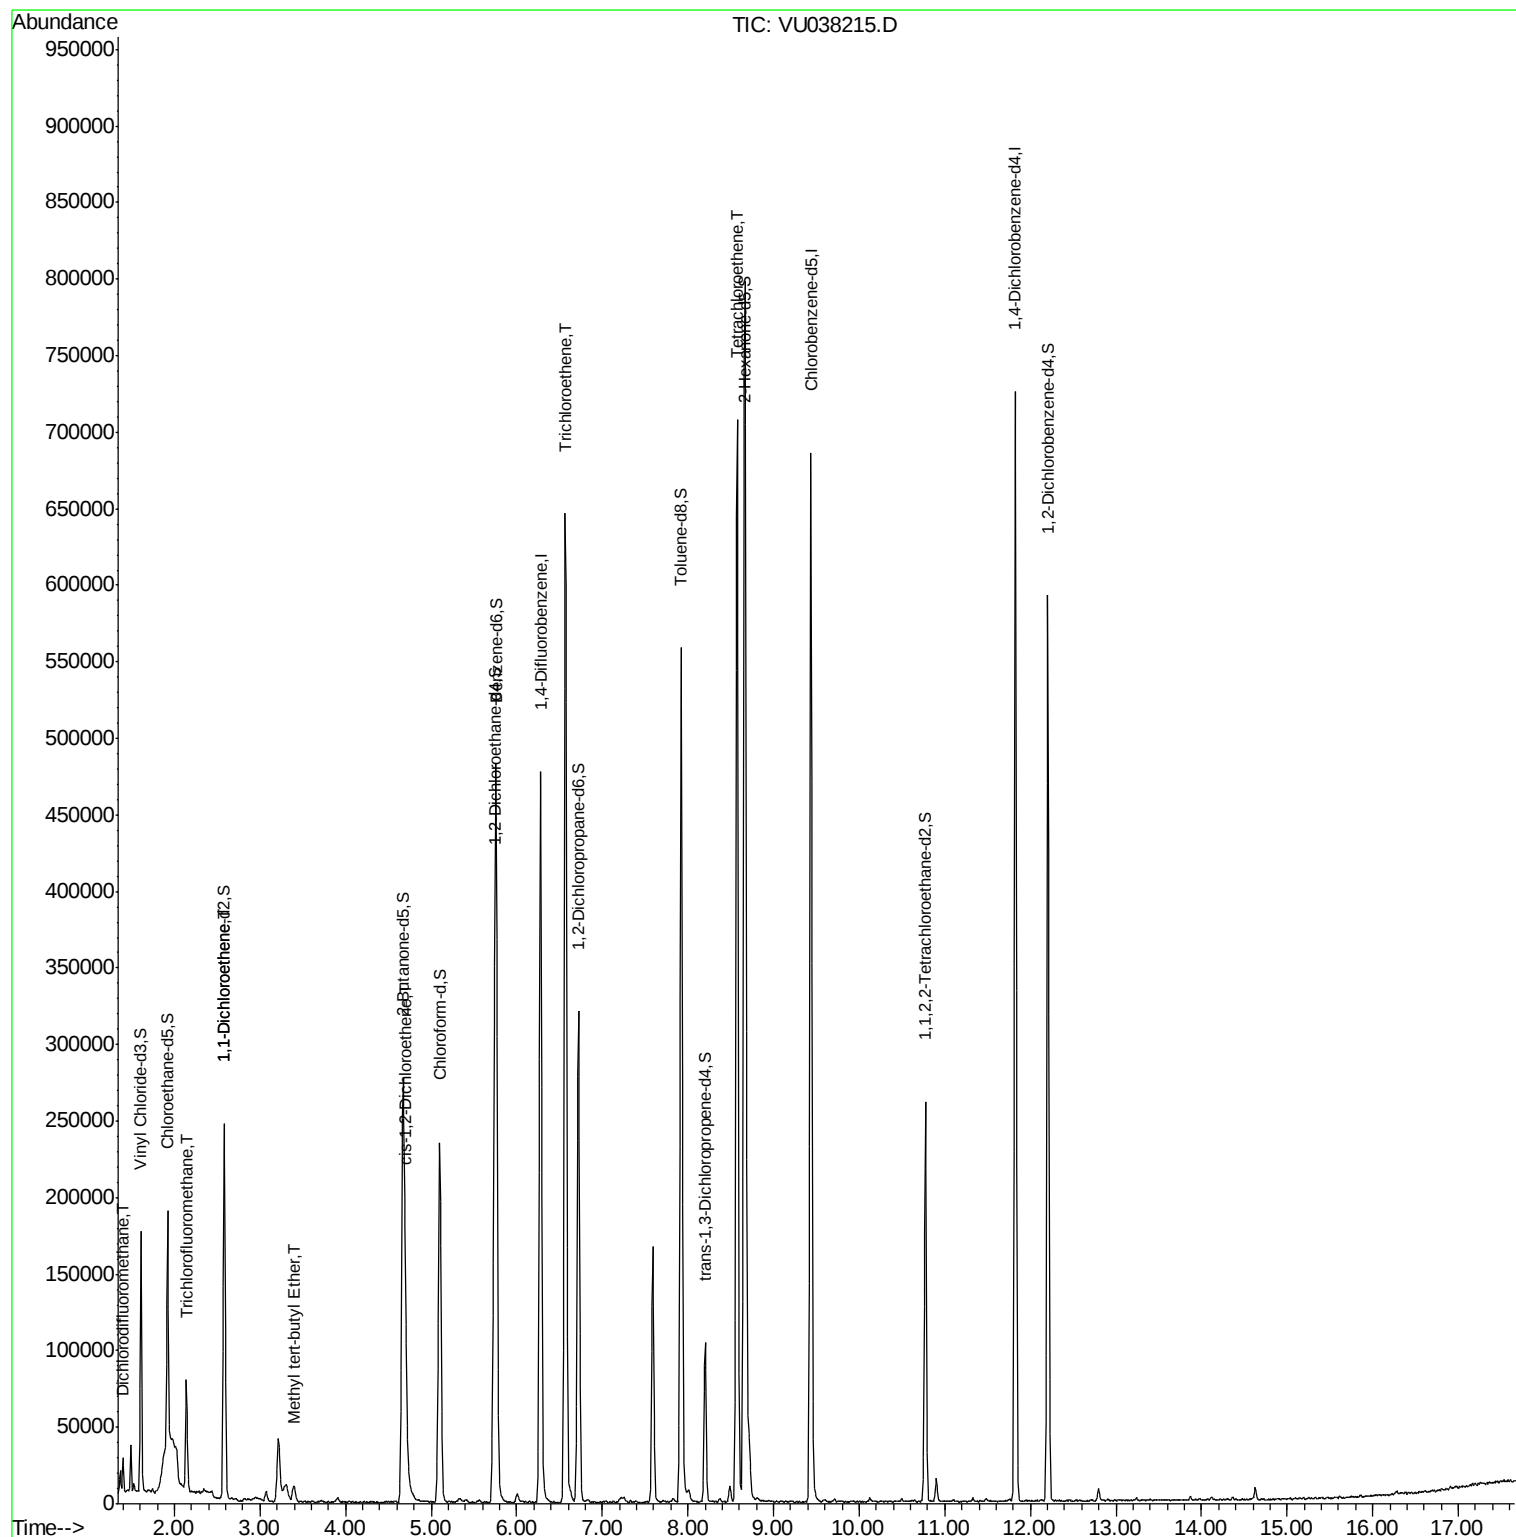

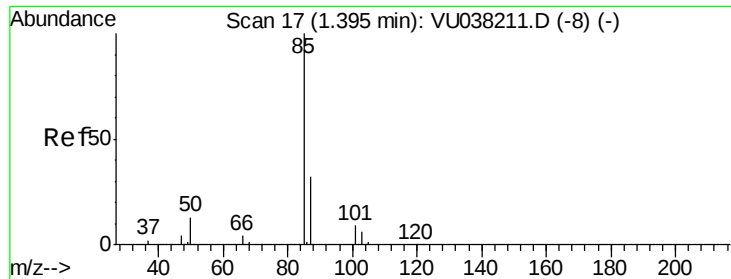

#2

Dichlorodifluoromethane

Concen: 0.187 ug/L

RT: 1.39 min Scan# 17

Delta R.T. 0.00 min

Lab File: VU038215.D

Acq: 18 May 2020 13:16

Instrument :

MSVOA_U

ClientSampleId :


BFST4DL

Tot Ion: 85 Resp: 6511

Ion Ratio Lower Upper




85 100

87 33.2 26.2 39.4

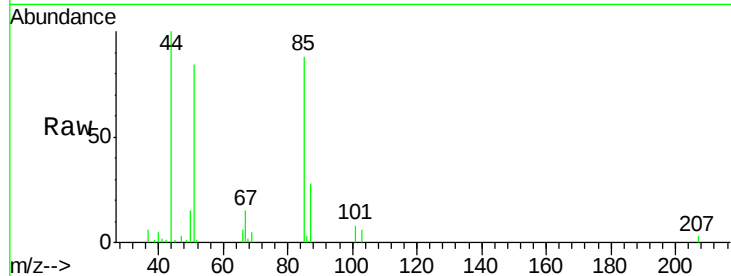

Abundance Ion 85.00 (84.70 to 85.70): VU038215.D (-1) (-)

Ion 87.00 (86.70 to 87.70): VU038215.D (-1) (-)

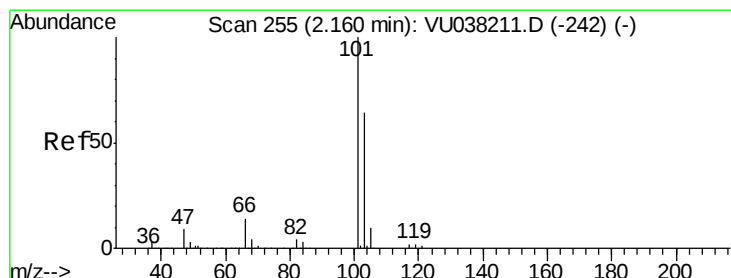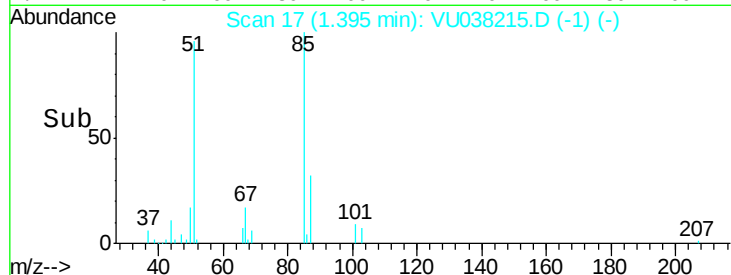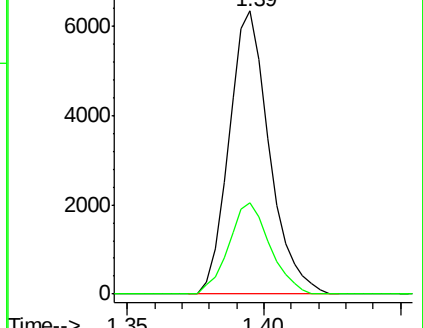

#9

Trichlorofluoromethane

Concen: 1.051 ug/L

RT: 2.14 min Scan# 249

Delta R.T. -0.02 min

Lab File: VU038215.D


Acq: 18 May 2020 13:16

Tgt Ion: 101 Resp: 44284

Ion Ratio Lower Upper



101 100


103 66.3 51.0 76.4

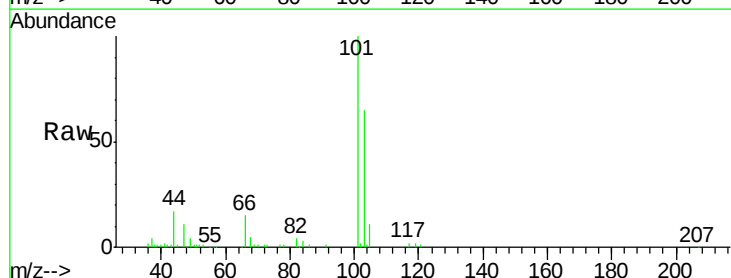

Abundance Ion 101.00 (100.70 to 101.70): VU038215.D (-162) (-)

Ion 103.00 (102.70 to 103.70): VU038215.D (-162) (-)

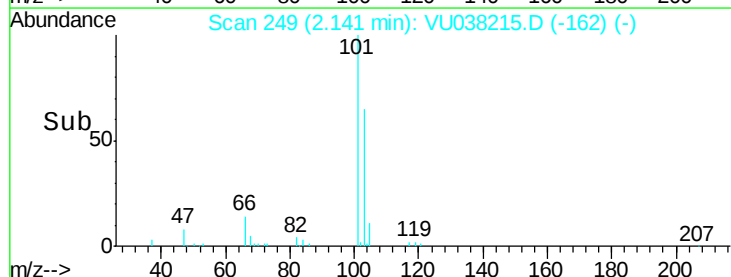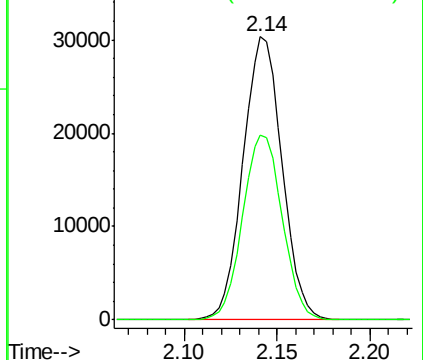

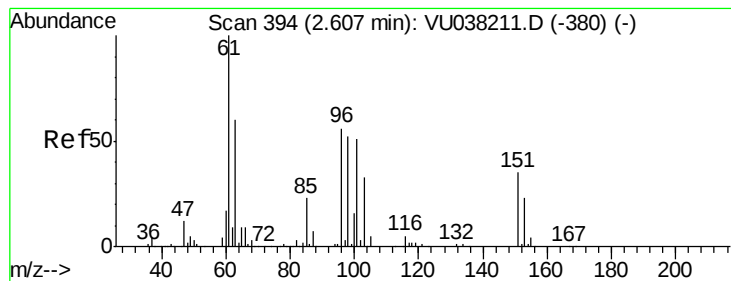

#12

1,1-Dichloroethene

Concen: 0.196 ug/L

RT: 2.59 min Scan# 390

Delta R.T. -0.01 min

Lab File: VU038215.D

Acq: 18 May 2020 13:16

Instrument :

MSVOA_U

ClientSampleId :

BFST4DL





Tot Ion: 96 Resp: 5204

Ion Ratio Lower Upper

96 100

61 347.9 126.2 234.4#

63 1771.5 96.9 179.9#

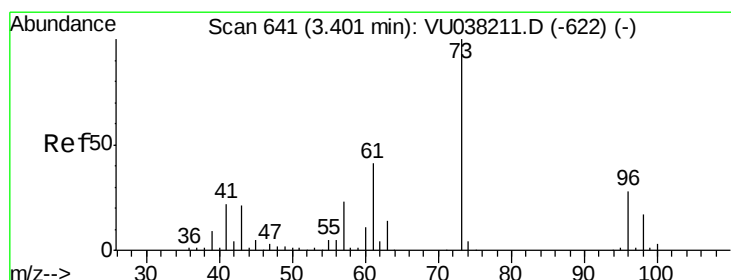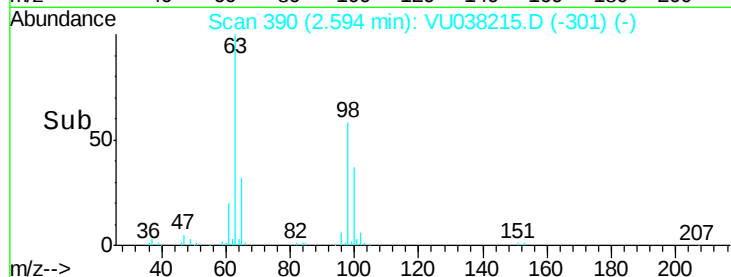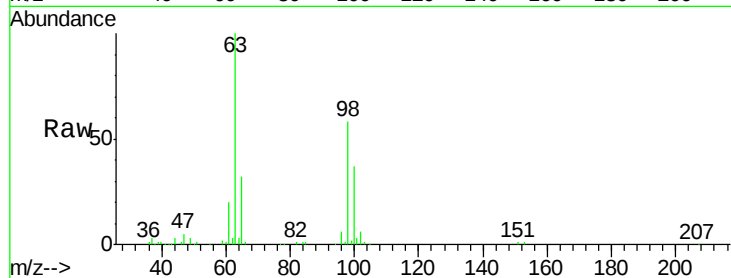

#17

Methyl tert-butyl Ether

Concen: 0.125 ug/L

RT: 3.40 min Scan# 641

Delta R.T. 0.00 min

Lab File: VU038215.D

Acq: 18 May 2020 13:16



Tgt Ion: 73 Resp: 9166


Ion Ratio Lower Upper

73 100

43 17.0 16.9 25.3

57 24.5 18.2 27.2

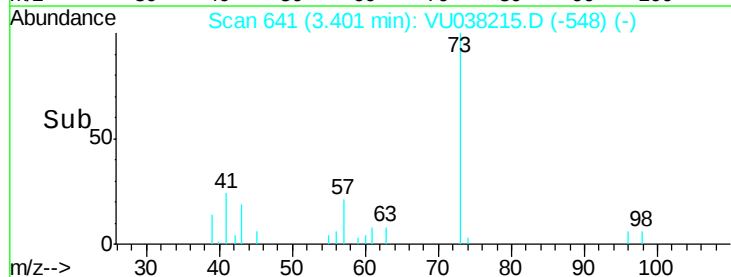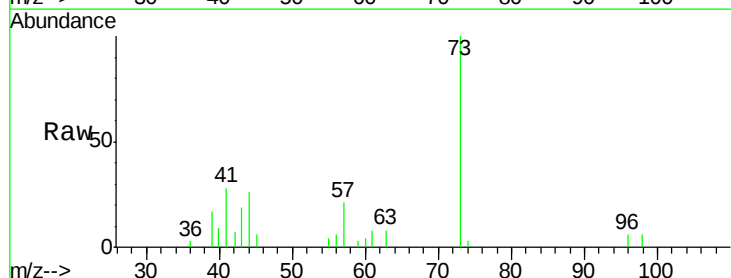

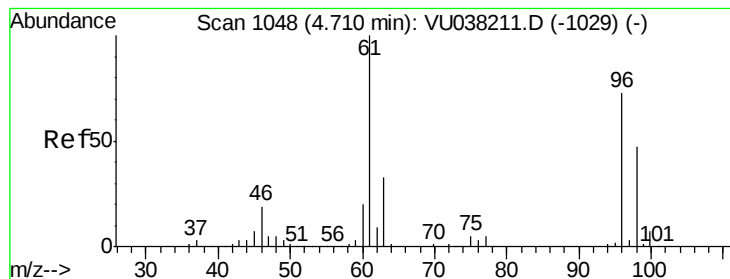

#22

cis-1,2-Dichloroethene

Concen: 0.770 ug/L

RT: 4.70 min Scan# 1046

Delta R.T. -0.01 min

Lab File: VU038215.D

Acq: 18 May 2020 13:16

Instrument :

MSVOA_U

ClientSampleId :

BFST4DL


Tot Ion: 96 Resp: 24000

Ion Ratio Lower Upper

96 100

61 136.8 95.3 176.9




68 0.0 0.0 0.0

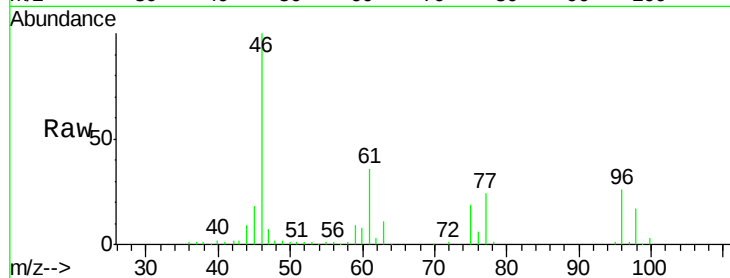

Abundance Ion 96.00 (95.70 to 96.70): VU038215.D (-1535) (-)

Ion 61.05 (60.75 to 61.75): VU038215.D (-1535) (-)

Ion 68.15 (67.85 to 68.85): VU038215.D (-1535) (-)

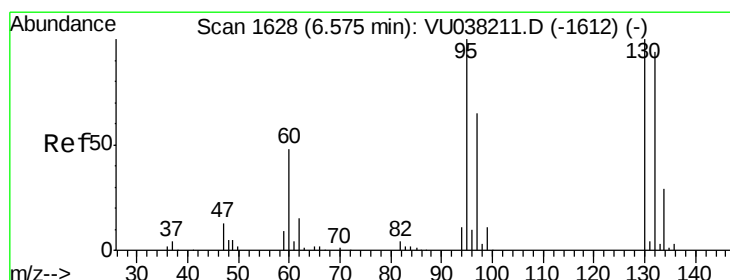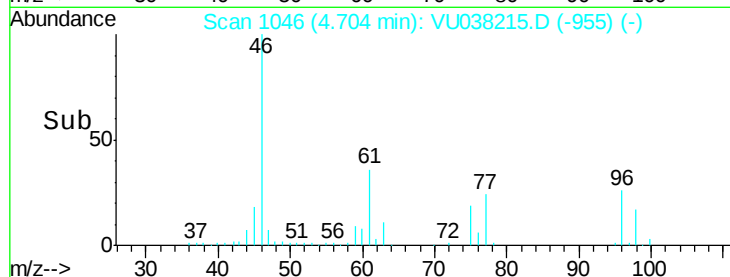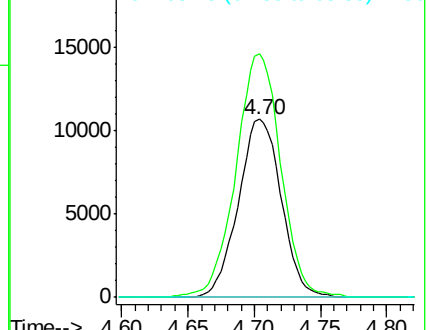

#34

Trichloroethene

Concen: 7.387 ug/L

RT: 6.57 min Scan# 1626

Delta R.T. -0.01 min

Lab File: VU038215.D

Acq: 18 May 2020 13:16

Tgt Ion: 95 Resp: 221432


Ion Ratio Lower Upper

95 100

97 65.1 44.9 83.3

132 91.3 63.3 117.5

130 94.4 65.7 122.1


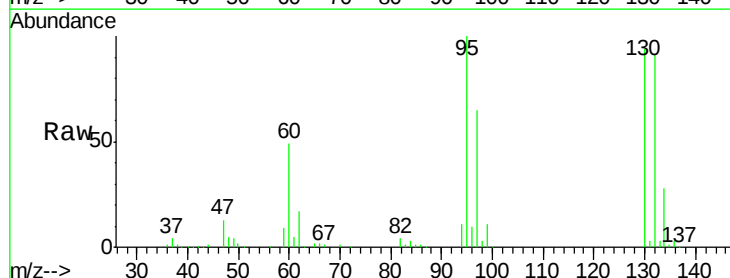



Abundance Ion 95.00 (94.70 to 95.70): VU038215.D (-1535) (-)

Ion 96.95 (96.65 to 97.65): VU038215.D (-1535) (-)

Ion 131.95 (131.65 to 132.65): VU038215.D (-1535) (-)

Ion 129.95 (129.65 to 130.65): VU038215.D (-1535) (-)

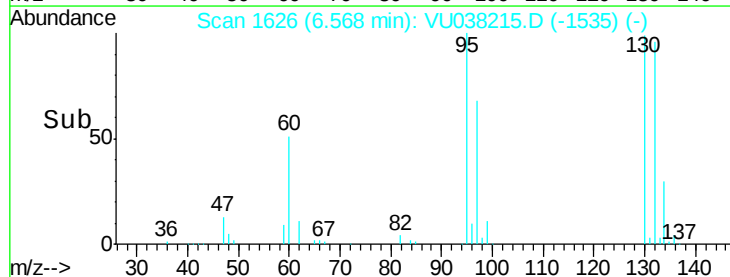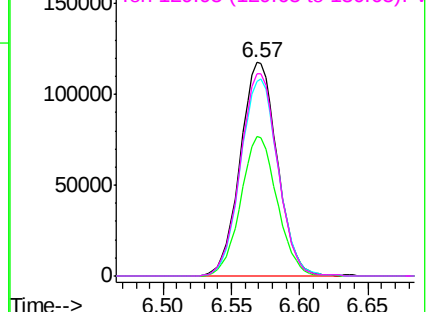

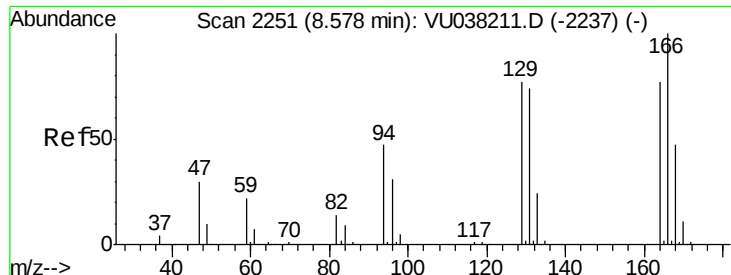

#47

Tetrachloroethene

Concen: 7.464 ug/L

RT: 8.57 min Scan# 2250

Delta R.T. -0.00 min

Lab File: VU038215.D

Acq: 18 May 2020 13:16

Instrument :

MSVOA_U

ClientSampleId :

BFST4DL

Tot Ion:164 Resp: 156504


Ion Ratio Lower Upper

164 100

129 99.1 68.8 127.8

131 94.4 66.8 124.2

166 132.0 88.9 165.1

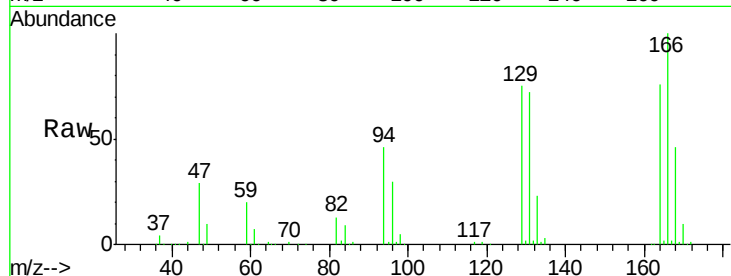

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

