


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051820\
 Data File : VU038210.D
 Acq On : 18 May 2020 09:04
 Operator : JC/MD
 Sample : BFB25
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB25

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue May 19 11:13:54 2020

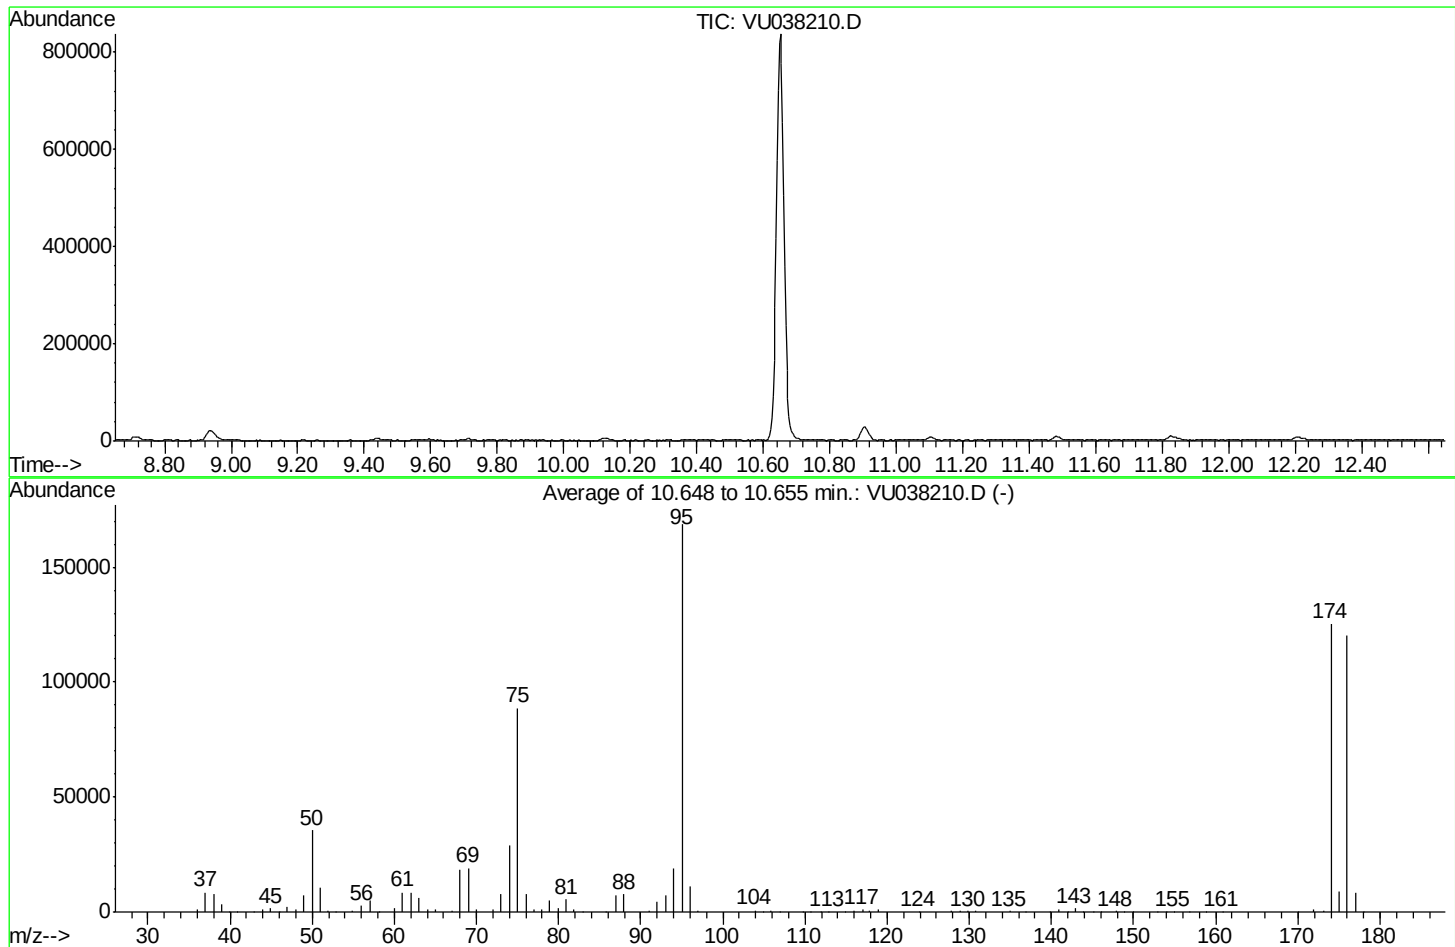

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	35370	PASS
75	95	30	80	52.6	88629	PASS
95	95	100	100	100.0	168597	PASS
96	95	5	9	6.7	11319	PASS
173	174	0.00	2	0.5	595	PASS
174	95	50	120	74.3	125264	PASS
175	174	5	9	7.3	9082	PASS
176	174	95	101	96.1	120376	PASS
177	176	5	9	6.8	8150	PASS

m/z	Abundance
36.10	1367.0
37.00	8955.0
38.00	8385.0
39.00	3330.0
39.90	365.0
40.90	128.0
42.90	239.0
44.00	2118.0
45.00	1415.0
47.00	2186.0
47.90	974.0
49.00	7820.0
50.00	36400.0
51.00	10950.0
51.90	495.0
52.80	104.0
54.90	534.0
56.00	2852.0
57.00	5073.0
58.10	174.0
60.00	1526.0
61.00	8674.0
62.00	8825.0
63.00	6291.0
64.00	912.0
65.00	1101.0
67.00	479.0
68.00	18544.0
69.00	19512.0
70.00	1493.0
72.00	1191.0
73.00	7983.0
74.00	30304.0
75.00	90288.0
76.00	8192.0
77.00	1178.0
77.90	966.0
78.90	4986.0
80.00	1601.0
80.90	5585.0
81.90	1137.0
82.90	156.0
85.80	308.0
87.00	7799.0
87.90	7756.0
90.90	554.0
92.00	4480.0
93.00	7635.0
94.00	18968.0
95.00	169344.0
96.00	11674.0
97.00	363.0
103.90	739.0
104.90	185.0
105.90	659.0
106.90	190.0
109.70	108.0
112.80	130.0
114.80	121.0
116.00	499.0
117.00	1086.0
117.90	631.0
119.00	1034.0
123.90	161.0
127.80	350.0
128.90	303.0
129.90	513.0
130.80	323.0
134.90	325.0
136.90	252.0
139.80	130.0
141.00	1481.0
142.10	228.0
142.90	1565.0
143.80	115.0
145.10	252.0
146.00	185.0
147.90	412.0
148.80	102.0
152.80	159.0
154.00	101.0
154.90	164.0
156.90	146.0
158.90	171.0
160.80	112.0
170.00	127.0
171.90	1040.0
173.10	1786.0
174.00	122608.0
175.00	9113.0
176.00	118480.0
177.00	8349.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

177.90

248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	1398.0
37.00	8718.0
38.00	8146.0
39.00	3211.0
40.00	392.0
40.90	120.0
42.90	251.0
44.00	2131.0
44.90	1477.0
46.10	185.0
47.00	2072.0
47.90	963.0
49.00	7719.0
50.00	36688.0
51.00	11206.0
51.90	479.0
54.90	457.0
56.00	2643.0
57.00	5217.0
58.10	197.0
60.00	1501.0
61.00	8901.0
62.00	8892.0
63.00	6261.0
64.00	1082.0
65.00	1096.0
67.10	483.0
68.00	18944.0
69.00	19664.0
70.00	1448.0
72.00	1135.0
73.00	8016.0
74.00	29904.0
75.00	91808.0
76.00	8089.0
77.00	1161.0
77.90	972.0
78.90	5319.0
79.90	1667.0
80.90	5597.0
81.90	1243.0
82.90	201.0
85.80	314.0
87.00	7738.0
88.00	7987.0
91.00	581.0
92.00	4493.0
93.00	7634.0
94.00	19472.0
95.00	173888.0
96.00	11659.0
97.00	356.0
103.90	748.0
104.80	194.0
105.90	666.0
106.90	180.0
110.70	121.0
112.80	123.0
114.90	221.0
115.90	522.0
117.00	1063.0
117.90	574.0
118.90	1069.0
123.90	129.0
127.80	382.0
128.90	337.0
129.90	494.0
130.80	418.0
134.90	336.0
136.90	266.0
141.00	1349.0
142.00	223.0
142.90	1445.0
143.80	120.0
145.00	212.0
146.00	184.0
147.90	391.0
148.80	139.0
152.90	176.0
153.90	133.0
154.90	219.0
156.90	167.0
158.90	197.0
160.80	158.0
170.00	129.0
171.90	1138.0
174.00	129376.0
175.00	9398.0
176.00	124312.0
177.00	8461.0
178.00	272.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	1223.0
37.00	7523.0
38.00	7370.0
39.00	2888.0
40.00	406.0
40.90	141.0
42.90	220.0
44.00	2136.0
44.90	1491.0
46.00	180.0
47.00	1991.0
48.00	943.0
49.00	6843.0
50.00	33024.0
51.00	10329.0
52.00	457.0
54.90	312.0
56.00	2225.0
57.00	4759.0
58.20	152.0
60.00	1403.0
61.00	8236.0
62.00	7882.0
63.00	5699.0
64.00	1022.0
65.10	983.0
67.10	459.0
68.00	17544.0
69.00	18064.0
70.00	1306.0
72.00	1028.0
73.00	7302.0
74.00	26696.0
75.00	83792.0
76.00	7284.0
77.00	946.0
77.90	843.0
78.90	5176.0
79.90	1592.0
80.90	4991.0
81.90	1183.0
82.90	164.0
85.80	247.0
86.90	6878.0
88.00	7426.0
91.00	471.0
92.00	4243.0
93.00	6802.0
94.00	18216.0
95.00	162560.0
96.00	10626.0
97.00	347.0
104.00	673.0
104.80	186.0
105.90	541.0
106.90	138.0
110.70	120.0
111.90	112.0
114.90	299.0
115.90	510.0
117.00	887.0
117.90	529.0
118.90	878.0
123.80	122.0
127.90	407.0
128.90	322.0
129.90	411.0
130.80	398.0
134.90	301.0
136.90	273.0
140.90	1134.0
141.90	198.0
142.90	1304.0
143.80	122.0
145.00	171.0
146.00	176.0
147.90	326.0
148.90	114.0
149.90	126.0
152.90	157.0
153.90	139.0
154.90	286.0
156.80	155.0
158.80	174.0
160.80	168.0
172.00	1145.0
174.00	123808.0
175.00	8735.0
176.00	118336.0
177.00	7642.0
177.90	271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Scan 2881 (10.603 min): VU038210.D
BFB25

m/z	Abundance
39.90	181.0
41.20	189.0
44.00	1083.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25