

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051821\
 Data File : VU043814.D
 Acq On : 18 May 2021 15:20
 Operator : SY/MD
 Sample : M2444-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG1Z4

Quant Time: May 19 01:42:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 19 01:40:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	228152	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	229483	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	107811	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	72570	4.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.20%
7) Chloroethane-d5	1.919	69	49297	4.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.00%
11) 1,1-Dichloroethene-d2	2.572	65	30366	4.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.00%
20) 2-Butanone-d5	4.642	46	183361	57.32	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.64%
24) Chloroform-d	5.073	84	131991	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
26) 1,2-Dichloroethane-d4	5.710	65	66758	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.735	84	272971	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.60%
36) 1,2-Dichloropropane-d6	6.700	67	87159	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.906	98	231002	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloroprop...	8.185	79	29513	4.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.60%
46) 2-Hexanone-d5	8.642	63	143129	46.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.18%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	68621	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
66) 1,2-Dichlorobenzene-d4	12.201	152	92026	5.12	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.40%
Target Compounds					Qvalue	
13) Acetone	2.655	43	5160	2.54	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051821\
Data File : VU043814.D
Acq On : 18 May 2021 15:20
Operator : SY/MD
Sample : M2444-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG1Z4

Quant Time: May 19 01:42:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 19 01:40:07 2021
Response via : Initial Calibration

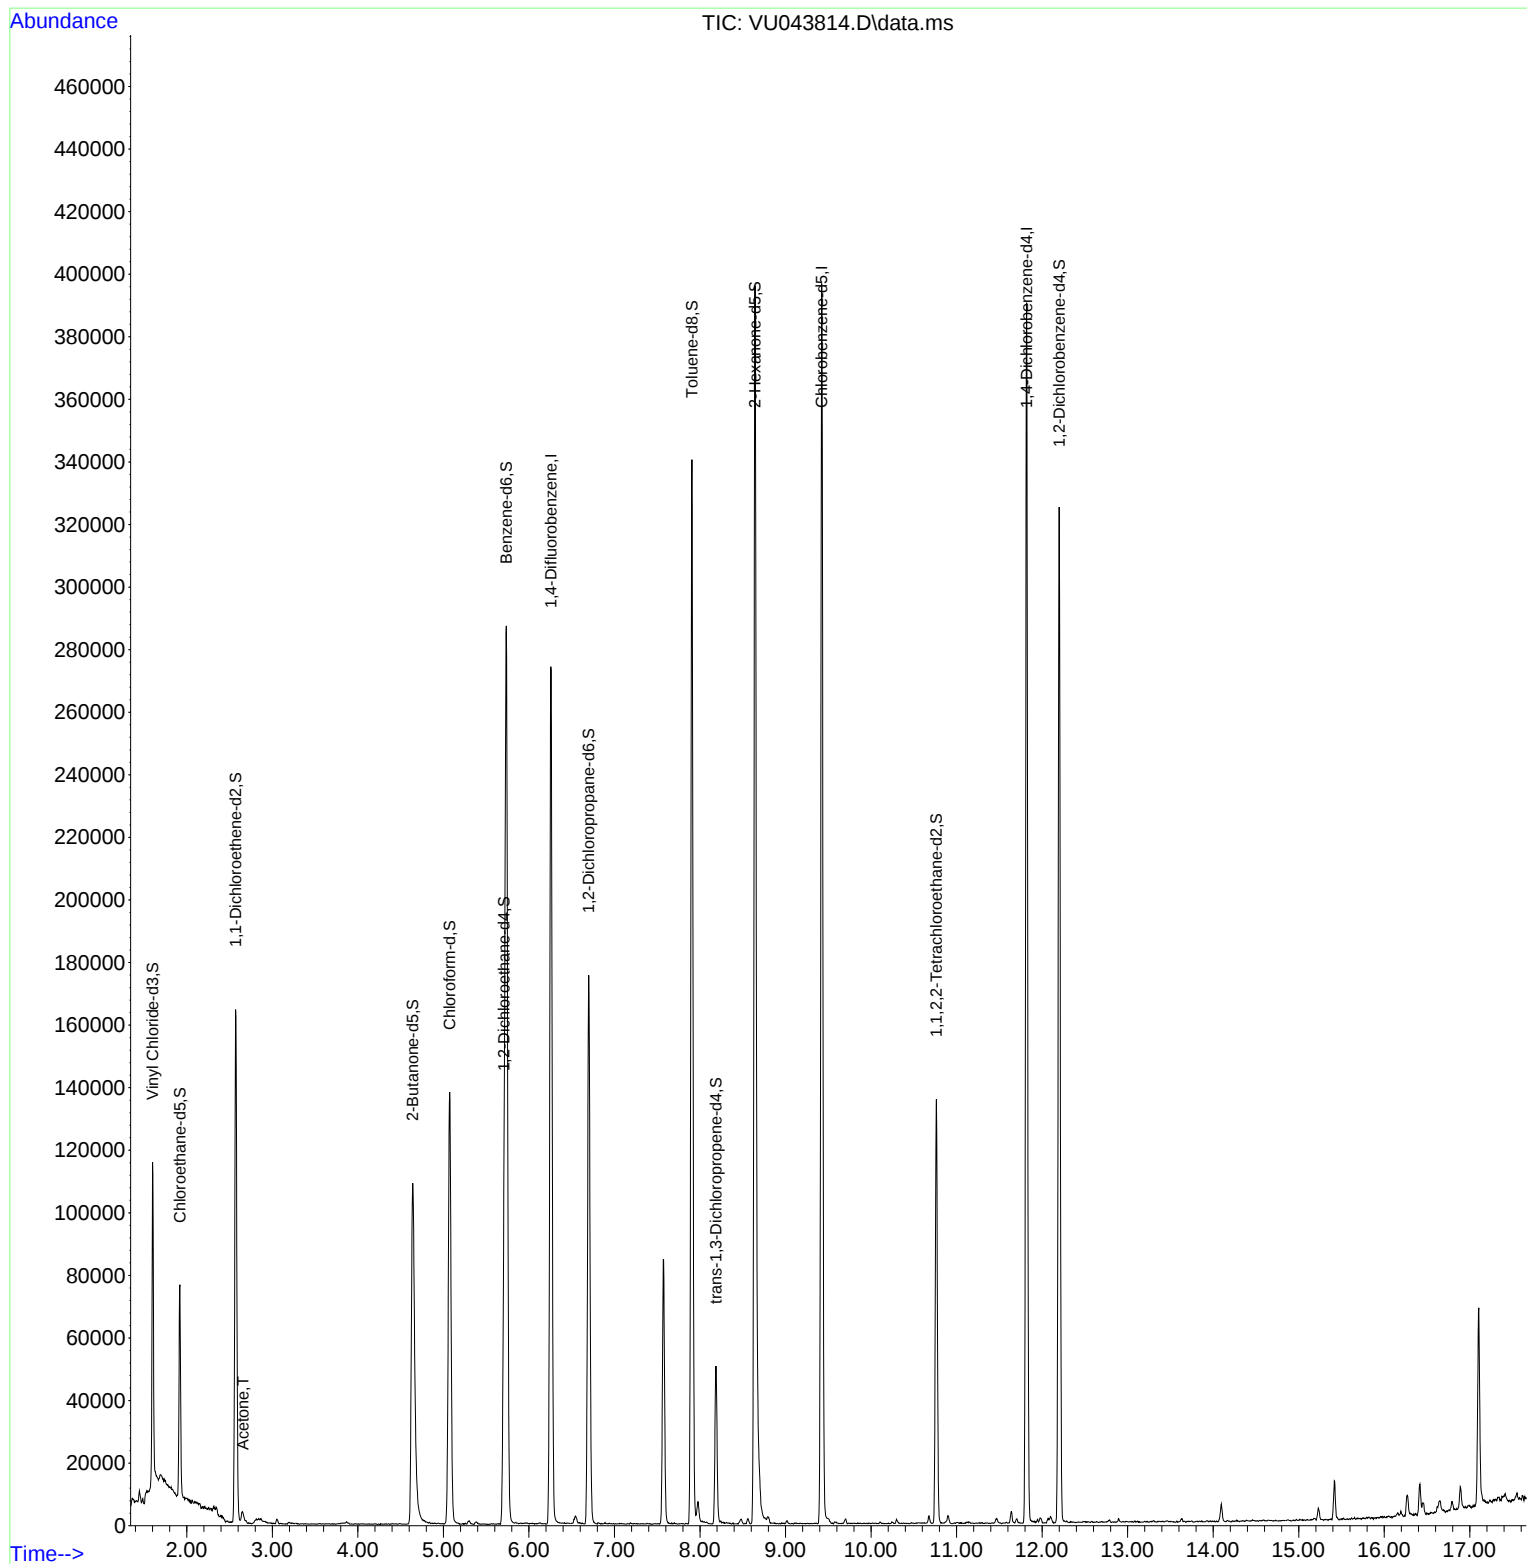

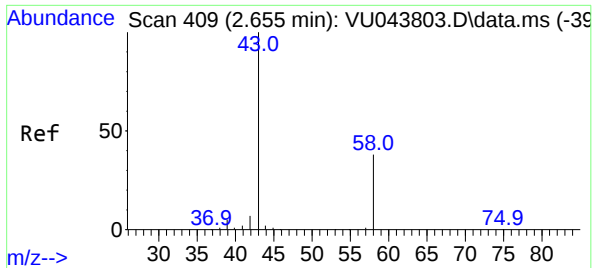

#13
Acetone
Concen: 2.54 ug/L
RT: 2.655 min Scan# 409
Delta R.T. -0.000 min
Lab File: VU043814.D
Acq: 18 May 2021 15:20

Instrument :
MSVOA_U
ClientSampleId :
BG1Z4

Tgt Ion: 43 Resp: 5160

Ion	Ratio	Lower	Upper
43	100		
58	29.6	0.0	71.6

