

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051821\
 Data File : VU043816.D
 Acq On : 18 May 2021 16:17
 Operator : SY/MD
 Sample : M2396-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	94	rBV	104054	116800	15.32%	1.859%
2	1.919	171	180	193	rVB	73472	94538	12.40%	1.505%
3	2.571	371	383	401	rBV	175276	283780	37.22%	4.516%
4	3.054	521	533	549	rBV	20081	37095	4.87%	0.590%
5	4.645	1013	1028	1053	rBV	71496	227669	29.86%	3.623%
6	5.073	1145	1161	1183	rVB	138310	306009	40.14%	4.870%
7	5.735	1345	1367	1391	rBV2	289434	739109	96.95%	11.763%
8	6.256	1515	1529	1551	rBV	269150	514531	67.49%	8.189%
9	6.700	1648	1667	1689	rBV	175991	341697	44.82%	5.438%
10	7.574	1926	1939	1968	rVB	85049	150065	19.68%	2.388%
11	7.906	2025	2042	2059	rBV	346854	591298	77.56%	9.410%
12	7.976	2059	2064	2080	rVB2	5781	9210	1.21%	0.147%
13	8.185	2118	2129	2146	rBV	51270	89841	11.78%	1.430%
14	8.645	2258	2272	2316	rBV	343168	762343	100.00%	12.132%
15	9.423	2500	2514	2535	rBV	386663	646239	84.77%	10.285%
16	10.764	2918	2931	2948	rBV	135479	224163	29.40%	3.567%
17	11.819	3247	3259	3277	rBV	380299	599372	78.62%	9.539%
18	12.066	3326	3336	3345	rBV6	4321	8040	1.05%	0.128%
19	12.201	3361	3378	3400	rVB	327329	528812	69.37%	8.416%
20	17.105	4895	4903	4913	rBV5	7016	12954	1.70%	0.206%




Sum of corrected areas: 6283565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051821\
Data File : VU043816.D
Acq On : 18 May 2021 16:17
Operator : SY/MD
Sample : M2396-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

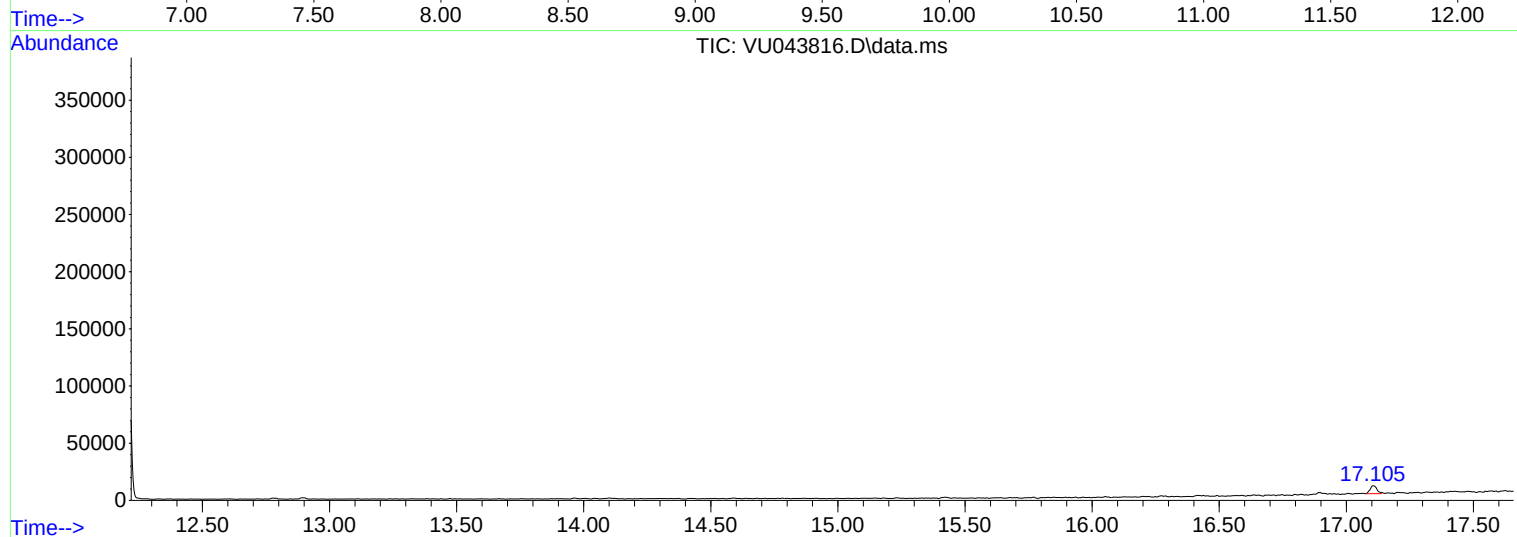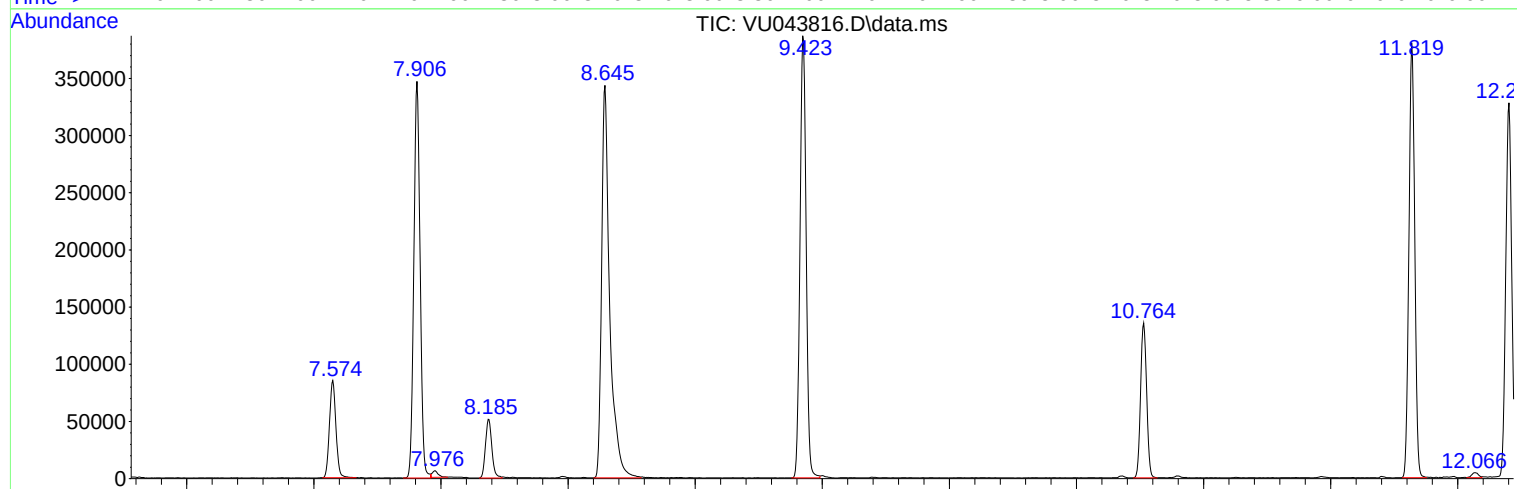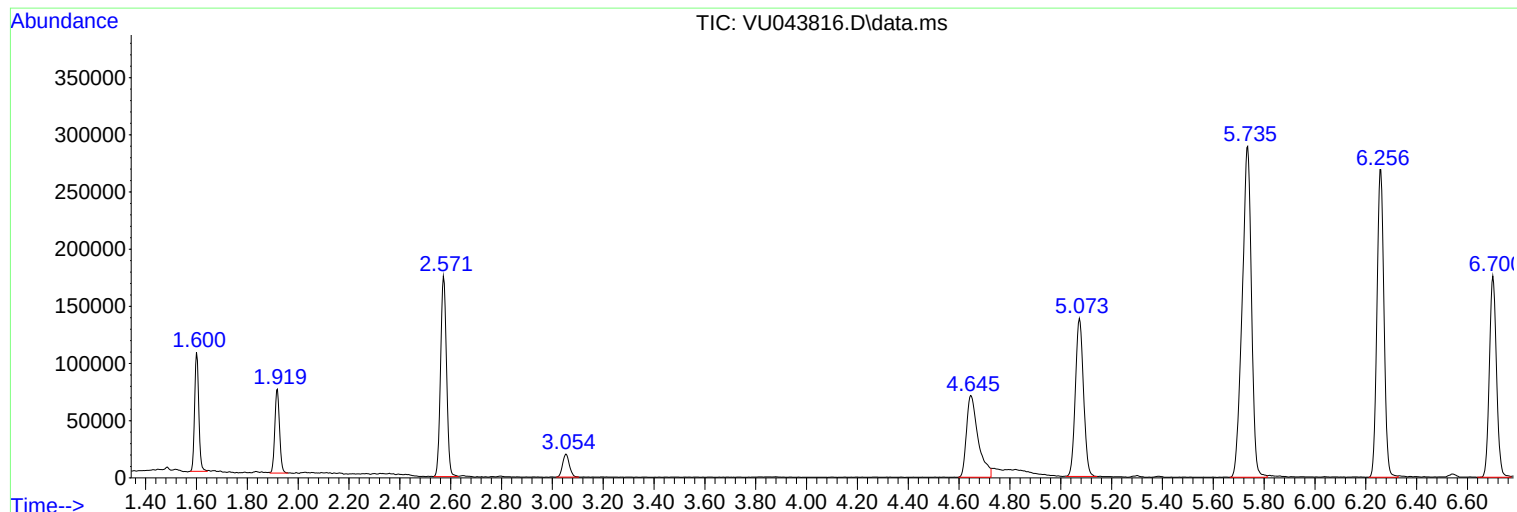

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051821\
Data File : VU043816.D
Acq On : 18 May 2021 16:17
Operator : SY/MD
Sample : M2396-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051821\
Data File : VU043816.D
Acq On : 18 May 2021 16:17
Operator : SY/MD
Sample : M2396-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
