
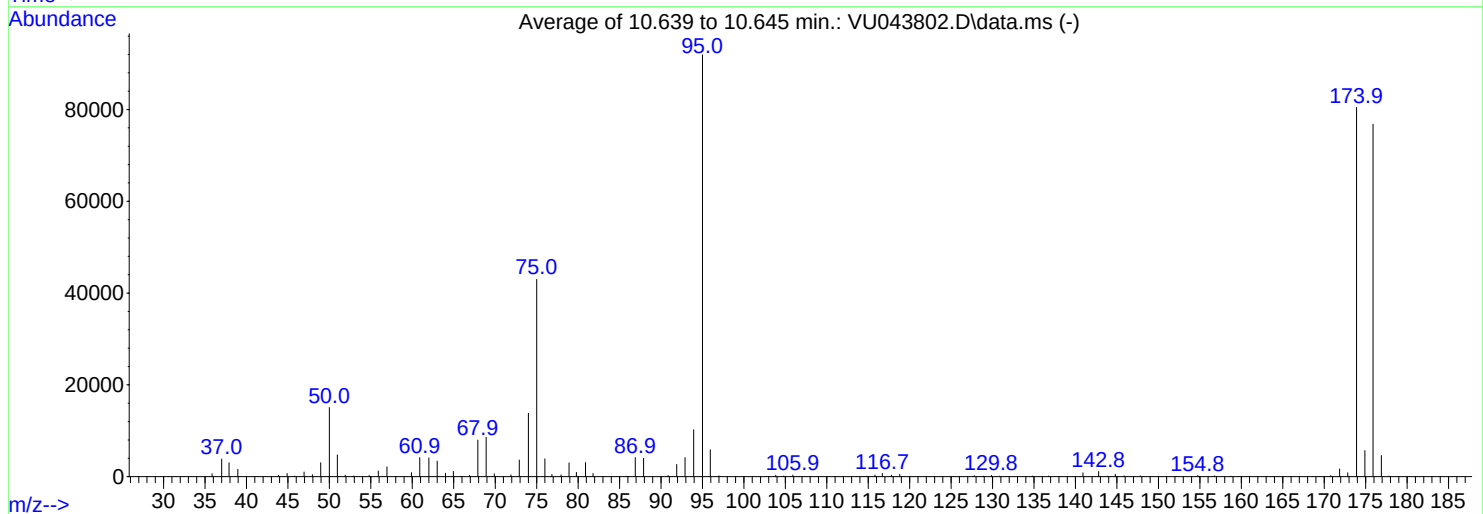


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051821\
 Data File : VU043802.D
 Acq On : 18 May 2021 08:44
 Operator : SY/MD
 Sample : BFB46
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB146

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 19 01:40:07 2021

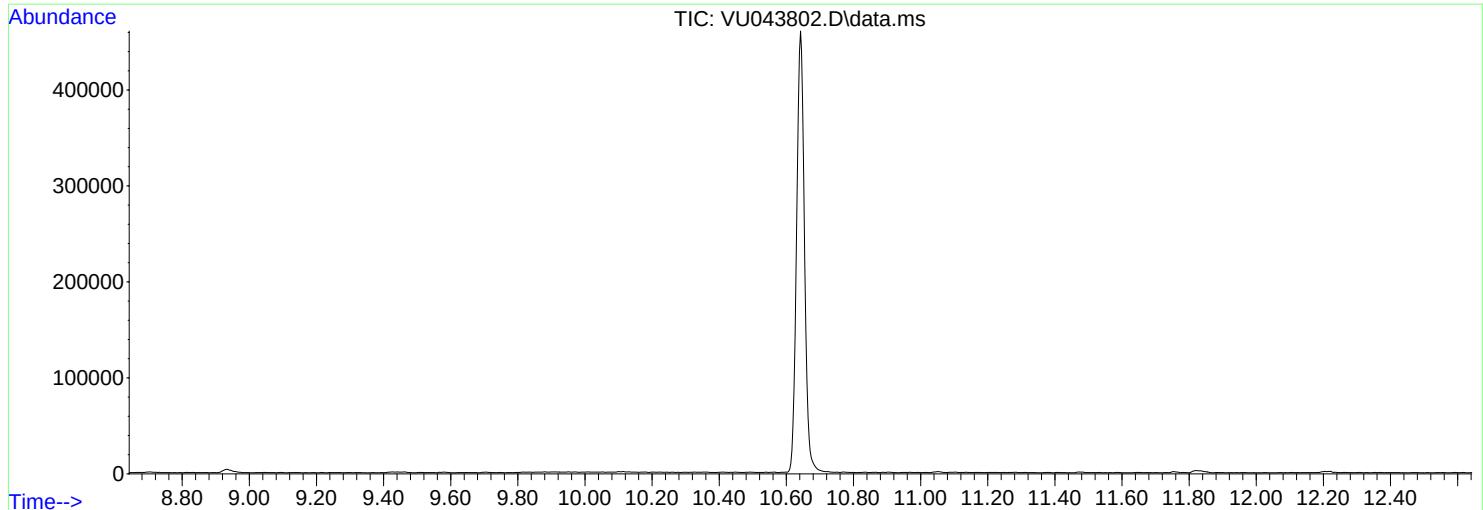

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	15081	PASS
75	95	30	80	46.8	43008	PASS
95	95	100	100	100.0	91917	PASS
96	95	5	9	6.4	5861	PASS
173	174	0.00	2	1.0	839	PASS
174	95	50	120	87.5	80472	PASS
175	174	5	9	7.1	5678	PASS
176	174	95	101	95.4	76800	PASS
177	176	5	9	6.0	4598	PASS

m/z	Abundance
35.90	1353.0
37.00	3993.0
38.00	3425.0
39.00	1657.0
40.00	217.0
43.90	851.0
44.90	707.0
45.80	131.0
47.00	1022.0
47.90	433.0
49.00	3104.0
50.00	15610.0
51.00	4878.0
51.90	324.0
52.90	138.0
54.80	256.0
55.90	1248.0
57.00	2215.0
59.90	921.0
60.90	4331.0
62.00	4237.0
63.00	3515.0
64.00	758.0
64.90	1206.0
65.80	105.0
66.90	256.0
67.90	8212.0
68.90	8791.0
69.90	653.0
71.90	428.0
72.90	3758.0
74.00	14348.0
75.00	44360.0
76.00	4037.0
76.80	514.0
78.00	423.0
78.90	3107.0
79.80	959.0
80.90	3177.0
81.80	695.0
85.80	132.0
86.90	4291.0
87.90	4208.0
90.80	232.0
91.90	2730.0
92.90	4316.0
93.90	10594.0
95.00	94984.0
95.90	6004.0
97.00	187.0
103.80	340.0
104.80	135.0
105.90	370.0
114.80	111.0
115.80	363.0
116.70	709.0
117.80	336.0
118.80	520.0
127.80	232.0
128.90	121.0
129.90	311.0
130.80	119.0
134.80	163.0
136.80	154.0
140.90	879.0
142.80	1134.0
143.90	120.0
144.80	555.0
145.80	201.0
147.80	172.0
154.80	240.0
156.70	174.0
158.70	127.0
161.00	101.0
170.80	250.0
171.80	1667.0
172.80	854.0
173.90	82928.0
174.90	5814.0
175.90	79312.0
176.90	4726.0
177.80	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	703.0
37.90	281.0
39.90	272.0
43.80	503.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	1362.0
37.00	3597.0
37.90	3205.0
39.00	1606.0
39.90	225.0
44.00	806.0
44.90	621.0
45.80	127.0
46.90	968.0
47.90	462.0
49.00	2951.0
50.00	14864.0
50.90	4577.0
51.90	316.0
52.90	148.0
54.80	189.0
55.90	1145.0
57.00	2063.0
59.90	888.0
60.90	3938.0
62.00	3787.0
63.00	3222.0
64.00	673.0
64.90	1167.0
66.90	241.0
67.90	7717.0
68.90	8218.0
69.90	596.0
71.90	367.0
72.90	3551.0
74.00	13516.0
75.00	42336.0
76.00	3683.0
76.90	515.0
78.00	446.0
78.90	2977.0
79.80	910.0
80.90	2969.0
81.80	660.0
85.80	160.0
86.90	4033.0
87.90	3896.0
90.80	240.0
91.90	2623.0
92.90	4025.0
94.00	9982.0
95.00	89152.0
95.90	5898.0
97.00	177.0
103.80	305.0
104.80	138.0
105.90	291.0
106.70	115.0
114.90	115.0
115.80	289.0
116.70	690.0
117.80	327.0
118.80	501.0
127.80	231.0
128.90	136.0
129.80	290.0
130.80	108.0
134.80	158.0
136.70	136.0
140.90	881.0
142.80	1053.0
143.90	108.0
144.80	516.0
145.90	180.0
147.80	182.0
154.80	237.0
156.70	177.0
158.80	104.0
161.00	106.0
170.80	282.0
171.90	1762.0
172.80	815.0
173.90	81144.0
174.90	5475.0
175.90	77760.0
176.90	4486.0
177.80	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	1291.0
37.00	3914.0
38.00	3334.0
38.90	1569.0
40.00	213.0
43.90	817.0
44.90	730.0
45.80	152.0
47.00	997.0
48.00	411.0
48.90	3077.0
50.00	14768.0
51.00	4734.0
51.90	286.0
52.90	139.0
54.80	282.0
55.90	1266.0
56.90	2105.0
58.10	108.0
59.90	771.0
60.90	4227.0
62.00	4240.0
63.00	3417.0
64.00	735.0
65.00	1128.0
65.80	106.0
66.90	239.0
67.90	8002.0
68.90	8712.0
69.90	655.0
71.90	411.0
72.90	3607.0
74.00	13597.0
75.00	42328.0
76.00	3954.0
76.90	455.0
77.90	335.0
78.90	2947.0
79.80	979.0
80.90	3111.0
81.80	722.0
86.10	184.0
86.90	4092.0
87.90	3984.0
90.90	268.0
91.90	2585.0
92.90	4133.0
93.90	10129.0
95.00	91616.0
96.00	5681.0
97.00	167.0
103.90	315.0
104.80	135.0
105.90	399.0
114.80	102.0
115.80	382.0
116.70	652.0
117.80	274.0
118.80	525.0
127.80	209.0
128.90	102.0
129.90	267.0
130.90	103.0
134.80	134.0
136.80	169.0
140.90	777.0
142.80	1151.0
143.90	127.0
144.80	534.0
145.80	186.0
147.80	157.0
154.70	235.0
156.80	160.0
158.70	130.0
170.80	224.0
171.80	1582.0
172.90	848.0
173.90	77344.0
174.90	5745.0
175.90	73328.0
176.90	4582.0
177.80	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146