




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
 Data File : VU048610.D
 Acq On : 18 May 2022 13:48
 Operator : SY/MD
 Sample : N2843-22ME
 Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4K2ME

Manual IntegrationsAPPROVED

Quant Time: May 19 06:03:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 19 06:01:59 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/19/2022
 Supervised By :Mahesh Dadoda 05/24/2022

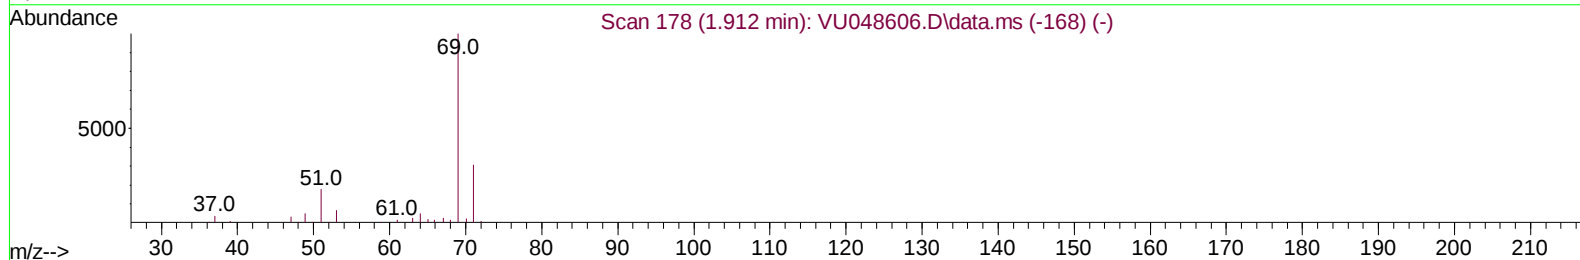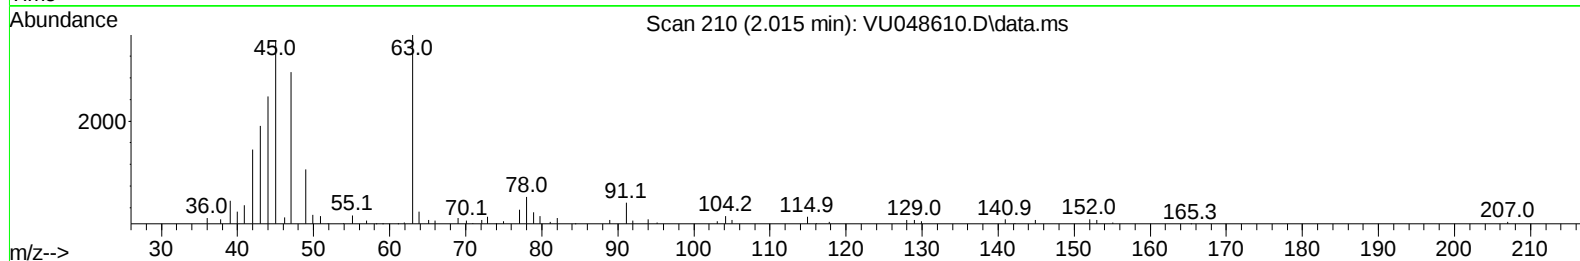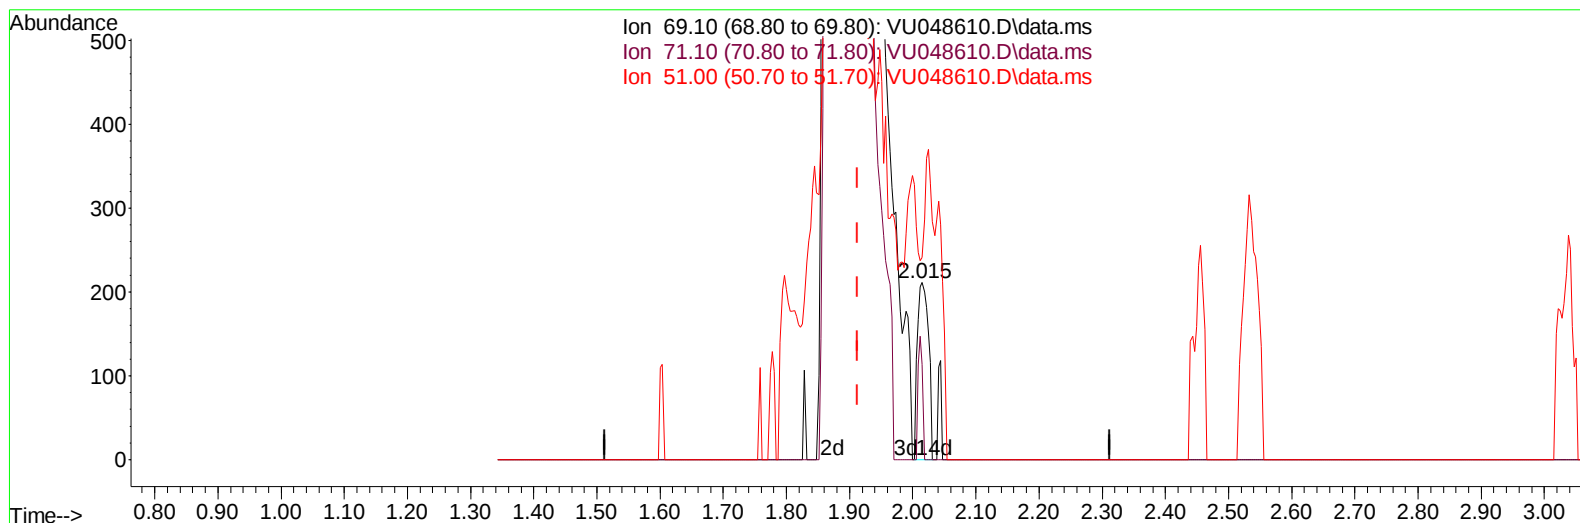

TIC: VU048610.D\data.ms

(7) Chloroethane-d5 (S)

2.015min (+ 0.103) 0.31 ug/L

response 261

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.70	27.59
51.00	26.90	33.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
Data File : VU048610.D
Acq On : 18 May 2022 13:48
Operator : SY/MD
Sample : N2843-22ME
Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4K2ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/19/2022
Supervised By :Mahesh Dadoda 05/24/2022

Quant Time: May 19 06:03:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 19 06:01:59 2022
Response via : Initial Calibration

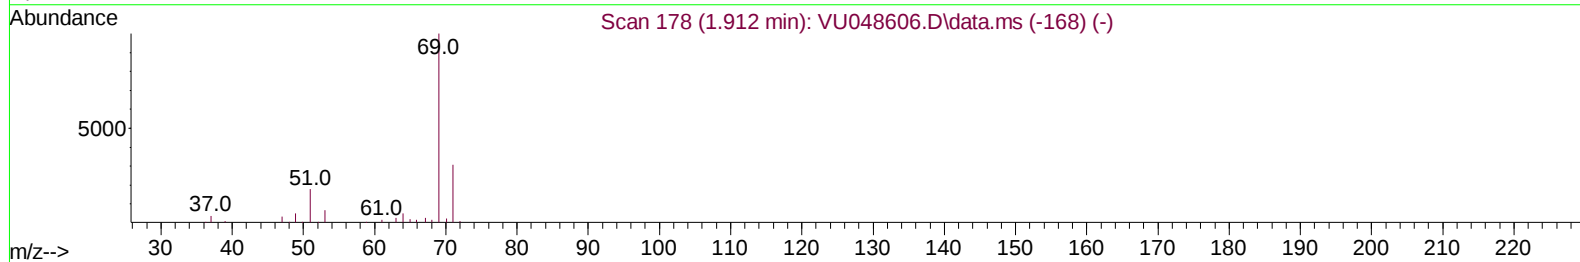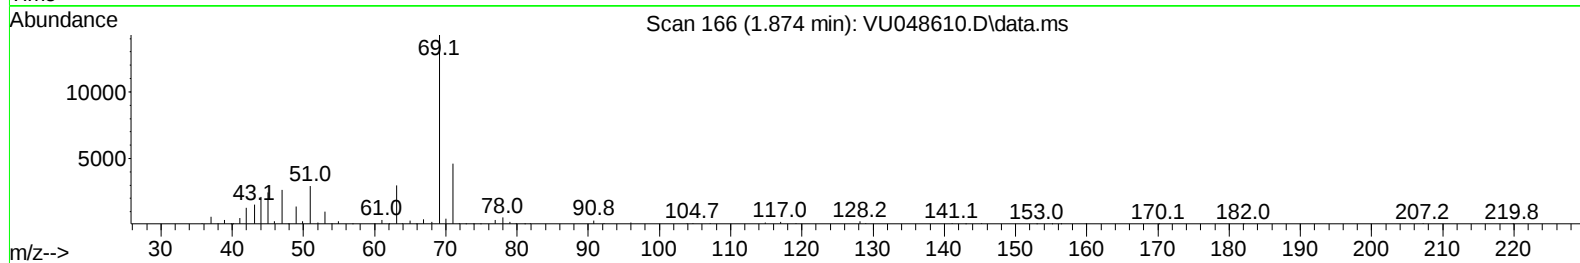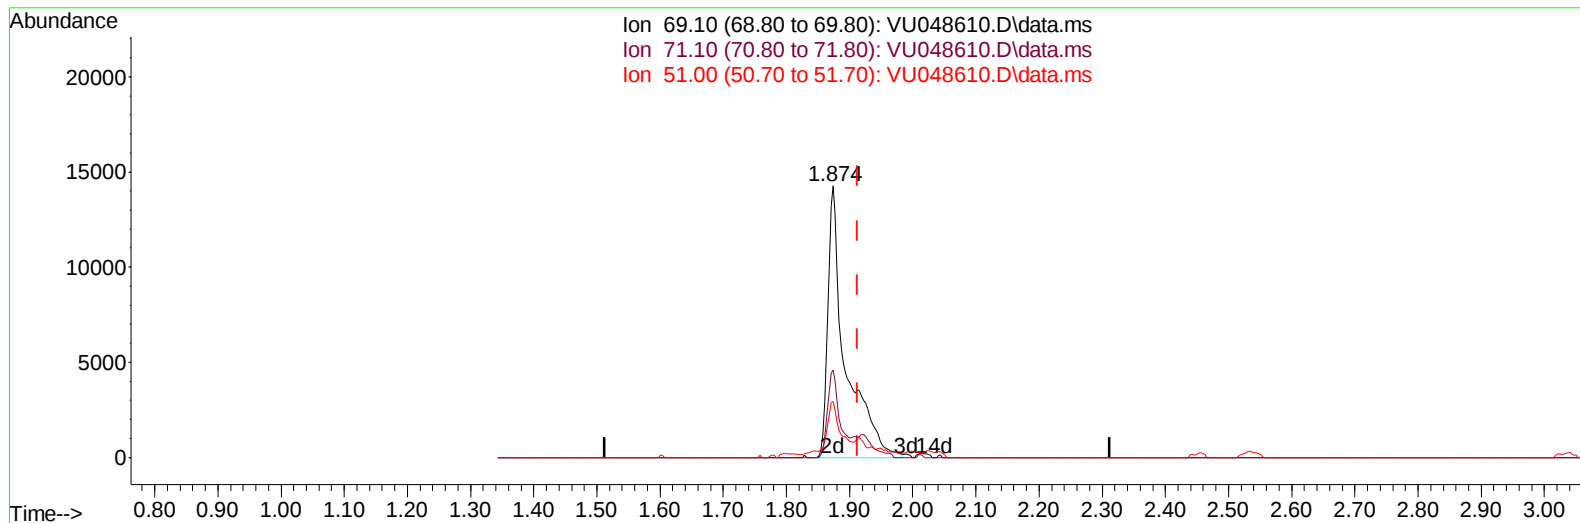

TIC: VU048610.D\data.ms

(7) Chloroethane-d5 (S)

1.874min (-0.039) 32.68 ug/L m

response 27773

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.70	0.26#
51.00	26.90	0.31#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
 Data File : VU048610.D
 Acq On : 18 May 2022 13:48
 Operator : SY/MD
 Sample : N2843-22ME
 Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW4K2ME

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/19/2022
 Supervised By :Mahesh Dadoda 05/24/2022

Quant Time: May 19 06:03:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 19 06:01:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	185177	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	190593	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152	115395	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	29709	26.194	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery =	52.380%#		
7) Chloroethane-d5	1.874	69	27773m	32.685	ug/L	-0.04
Spiked Amount 50.000	Range 70	- 130	Recovery =	65.360%#		
11) 1,1-Dichloroethene-d2	2.533	63	51107	19.924	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery =	39.840%#		
21) 2-Butanone-d5	4.629	46	125088	115.894	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery =	115.890%		
24) Chloroform-d	5.060	84	117458	40.982	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	81.960%		
26) 1,2-Dichloroethane-d4	5.700	65	86455	42.757	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	85.520%		
32) Benzene-d6	5.723	84	178400	33.633	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery =	67.260%#		
36) 1,2-Dichloropropane-d6	6.690	67	60632	38.937	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery =	77.880%		
41) Toluene-d8	7.899	98	152988	30.663	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	61.320%#		
43) trans-1,3-Dichloroprop...	8.185	79	35581	35.733	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery =	71.460%		
47) 2-Hexanone-d5	8.655	63	96021	112.439	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery =	112.440%		
56) 1,1,2,2-Tetrachloroeth...	10.764	84	132802	51.539	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery =	103.080%		
66) 1,2-Dichlorobenzene-d4	12.198	152	100503	42.604	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery =	85.200%		
Target Compounds						
22) 2-Butanone	4.713	43	14579	13.094	ug/L	Qvalue 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
Data File : VU048610.D
Acq On : 18 May 2022 13:48
Operator : SY/MD
Sample : N2843-22ME
Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW4K2ME

Manual IntegrationsAPPROVED

Quant Time: May 19 06:03:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 19 06:01:59 2022
Response via : Initial Calibration

Reviewed By : John Carlone 05/19/2022
Supervised By : Mahesh Dadoda 05/24/2022

