

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
 Data File : VU048619.D
 Acq On : 18 May 2022 17:18
 Operator : SY/MD
 Sample : N2849-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	80817	87952	10.34%	1.222%
2	1.912	169	178	196	rVB	64304	83464	9.81%	1.160%
3	2.208	263	270	275	rBV3	1882	2500	0.29%	0.035%
4	2.568	368	382	395	rBV	171743	282468	33.21%	3.925%
5	2.674	412	415	419	rBV2	281	222	0.03%	0.003%
6	2.713	423	427	430	rBV2	239	194	0.02%	0.003%
7	2.758	436	441	442	rBV	263	209	0.02%	0.003%
8	2.806	448	456	460	rBB3	446	569	0.07%	0.008%
9	2.954	500	502	508	rBB2	333	316	0.04%	0.004%
10	3.047	526	531	535	rBV4	674	725	0.09%	0.010%
11	3.141	556	560	564	rBV2	307	318	0.04%	0.004%
12	3.163	564	567	568	rBV	526	298	0.04%	0.004%
13	3.562	689	691	694	rBB2	278	199	0.02%	0.003%
14	3.594	699	701	703	rBV	424	236	0.03%	0.003%
15	3.681	726	728	733	rBV	184	198	0.02%	0.003%
16	4.449	959	967	969	rBV3	1709	2009	0.24%	0.028%
17	4.620	1006	1020	1045	rBV	89165	210173	24.71%	2.920%
18	4.822	1081	1083	1086	rVB2	421	190	0.02%	0.003%
19	4.928	1115	1116	1121	rVV2	343	218	0.03%	0.003%
20	4.996	1132	1137	1139	rBB	257	172	0.02%	0.002%
21	5.063	1142	1158	1181	rBV2	173219	429242	50.46%	5.964%
22	5.292	1225	1229	1231	rBV2	475	451	0.05%	0.006%
23	5.359	1247	1250	1252	rBB2	332	196	0.02%	0.003%
24	5.726	1341	1364	1389	rBV2	309039	850596	100.00%	11.819%
25	5.874	1408	1410	1412	rVB2	388	184	0.02%	0.003%
26	5.944	1429	1432	1435	rBB2	248	177	0.02%	0.002%
27	6.112	1479	1484	1486	rVV	216	224	0.03%	0.003%
28	6.250	1512	1527	1547	rBV	287699	542062	63.73%	7.532%
29	6.372	1562	1565	1568	rVB2	694	404	0.05%	0.006%
30	6.488	1599	1601	1605	rVB	254	185	0.02%	0.003%
31	6.530	1605	1614	1623	rBV3	3248	5836	0.69%	0.081%
32	6.690	1649	1664	1688	rVV	193275	370658	43.58%	5.150%
33	6.880	1716	1723	1735	rVB6	3445	6482	0.76%	0.090%
34	7.047	1771	1775	1779	rVB2	365	389	0.05%	0.005%
35	7.070	1779	1782	1783	rBV	336	177	0.02%	0.002%
36	7.108	1783	1794	1809	rVB3	17039	30519	3.59%	0.424%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
 Data File : VU048619.D
 Acq On : 18 May 2022 17:18
 Operator : SY/MD
 Sample : N2849-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	7.186	1810	1818	1828	rBV5	1758	2833	0.33%	0.039%
38	7.491	1909	1913	1916	rBV	155	178	0.02%	0.002%
39	7.565	1924	1936	1950	rBV2	114249	197637	23.24%	2.746%
40	7.690	1970	1975	1984	rVB5	1119	1650	0.19%	0.023%
41	7.780	2001	2003	2004	rBV	311	169	0.02%	0.002%
42	7.899	2025	2040	2056	rBV	398035	684254	80.44%	9.508%
43	8.076	2093	2095	2102	rVB4	700	795	0.09%	0.011%
44	8.140	2111	2115	2116	rBV	310	215	0.03%	0.003%
45	8.179	2116	2127	2145	rBV	83910	142099	16.71%	1.975%
46	8.356	2180	2182	2186	rVB	401	220	0.03%	0.003%
47	8.382	2186	2190	2193	rBV2	233	203	0.02%	0.003%
48	8.414	2196	2200	2203	rBV	222	175	0.02%	0.002%
49	8.468	2209	2217	2218	rBV2	1235	996	0.12%	0.014%
50	8.555	2240	2244	2248	rBB2	332	251	0.03%	0.003%
51	8.581	2249	2252	2255	rBV	177	173	0.02%	0.002%
52	8.632	2255	2268	2296	rBV	271850	486655	57.21%	6.762%
53	8.787	2306	2316	2337	rVB5	41084	82685	9.72%	1.149%
54	8.883	2344	2346	2351	rVV	414	223	0.03%	0.003%
55	8.989	2375	2379	2385	rBB2	334	356	0.04%	0.005%
56	9.128	2419	2422	2425	rBB	281	177	0.02%	0.002%
57	9.160	2425	2432	2435	rBV2	282	346	0.04%	0.005%
58	9.324	2478	2483	2486	rBV	309	278	0.03%	0.004%
59	9.417	2499	2512	2531	rBV	404011	677844	79.69%	9.419%
60	9.578	2559	2562	2566	rVB2	364	286	0.03%	0.004%
61	9.697	2593	2599	2606	rBB3	843	1328	0.16%	0.018%
62	9.812	2632	2635	2639	rBV	214	228	0.03%	0.003%
63	9.976	2682	2686	2692	rVB2	314	346	0.04%	0.005%
64	10.031	2699	2703	2705	rBV	313	250	0.03%	0.003%
65	10.089	2717	2721	2725	rBV2	453	450	0.05%	0.006%
66	10.240	2766	2768	2772	rVB	289	185	0.02%	0.003%
67	10.275	2775	2779	2780	rBV	296	194	0.02%	0.003%
68	10.298	2780	2786	2789	rVB2	365	342	0.04%	0.005%
69	10.346	2796	2801	2808	rVB4	1475	1906	0.22%	0.026%
70	10.565	2865	2869	2871	rBV	278	176	0.02%	0.002%
71	10.758	2916	2929	2948	rBV	296531	477422	56.13%	6.634%
72	10.896	2961	2972	2978	rBV2	2834	3979	0.47%	0.055%
73	11.462	3138	3148	3156	rBV7	1235	2520	0.30%	0.035%
74	11.626	3196	3199	3203	rVB	242	168	0.02%	0.002%
75	11.693	3214	3220	3229	rVB5	1392	1636	0.19%	0.023%
76	11.812	3243	3257	3277	rBV	489381	768005	90.29%	10.672%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
 Data File : VU048619.D
 Acq On : 18 May 2022 17:18
 Operator : SY/MD
 Sample : N2849-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	12.076	3330	3339	3346	rBV7	2608	4185	0.49%	0.058%
78	12.192	3363	3375	3390	rBV	449466	726746	85.44%	10.098%
79	12.330	3412	3418	3420	rBV4	745	708	0.08%	0.010%
80	12.385	3428	3435	3436	rBV3	542	408	0.05%	0.006%
81	12.436	3448	3451	3453	rBV2	564	325	0.04%	0.005%
82	12.722	3538	3540	3546	rBV2	344	296	0.03%	0.004%
83	12.770	3548	3555	3556	rBV	819	1001	0.12%	0.014%
84	12.864	3582	3584	3586	rBV	639	320	0.04%	0.004%
85	12.893	3586	3593	3601	rVV7	2602	4701	0.55%	0.065%
86	13.044	3637	3640	3642	rBV	361	220	0.03%	0.003%
87	13.121	3662	3664	3666	rBV2	390	219	0.03%	0.003%
88	13.134	3666	3668	3671	rVB2	357	180	0.02%	0.003%
89	13.298	3714	3719	3721	rBV3	516	464	0.05%	0.006%
90	13.349	3733	3735	3738	rBV	410	240	0.03%	0.003%
91	13.513	3784	3786	3790	rBV2	473	362	0.04%	0.005%
92	13.639	3822	3825	3829	rBV2	587	509	0.06%	0.007%
93	13.722	3849	3851	3855	rBV	454	255	0.03%	0.004%
94	13.844	3887	3889	3891	rBV2	527	262	0.03%	0.004%
95	13.944	3916	3920	3921	rBV	346	237	0.03%	0.003%
96	13.986	3931	3933	3936	rBV2	512	260	0.03%	0.004%
97	14.172	3989	3991	3993	rBV	860	478	0.06%	0.007%
98	14.288	4025	4027	4030	rBV2	564	319	0.04%	0.004%
99	14.449	4073	4077	4083	rVB5	2989	3182	0.37%	0.044%
100	14.886	4210	4213	4216	rVB3	809	553	0.07%	0.008%




Sum of corrected areas: 7196675

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
Data File : VU048619.D
Acq On : 18 May 2022 17:18
Operator : SY/MD
Sample : N2849-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

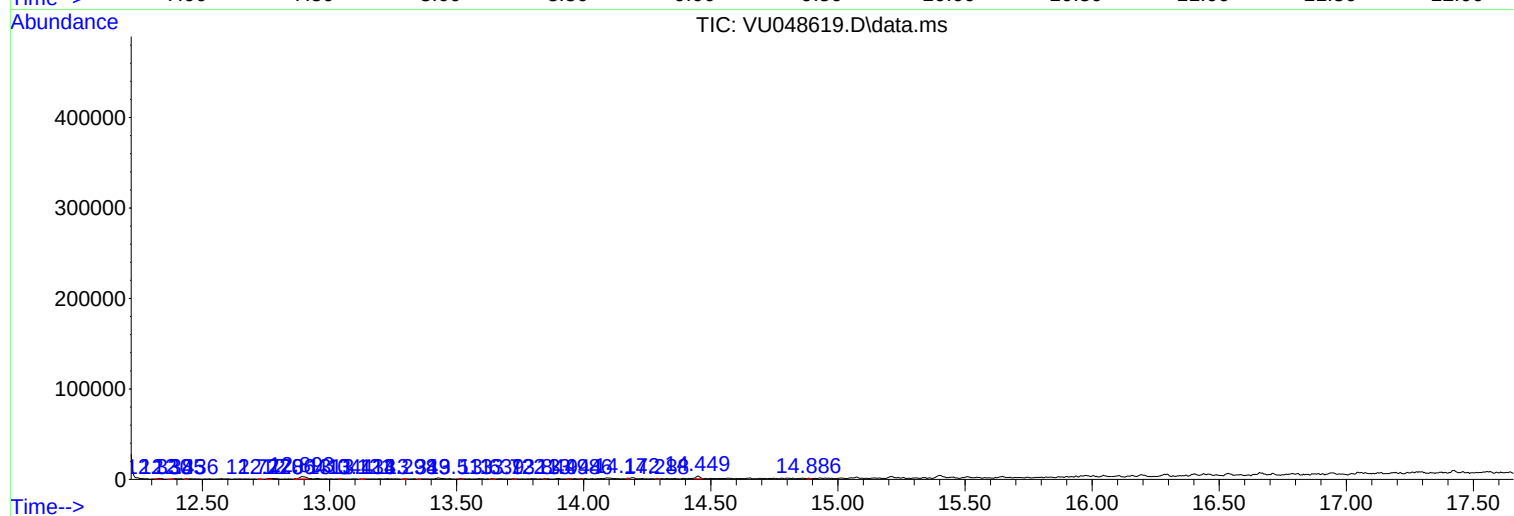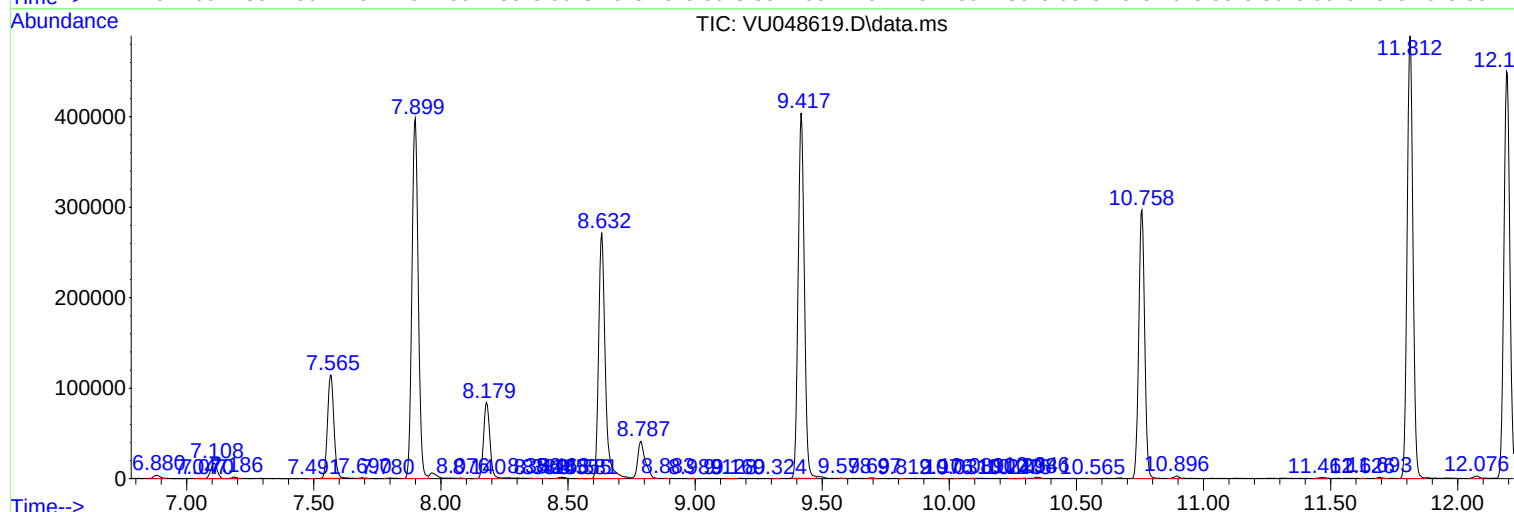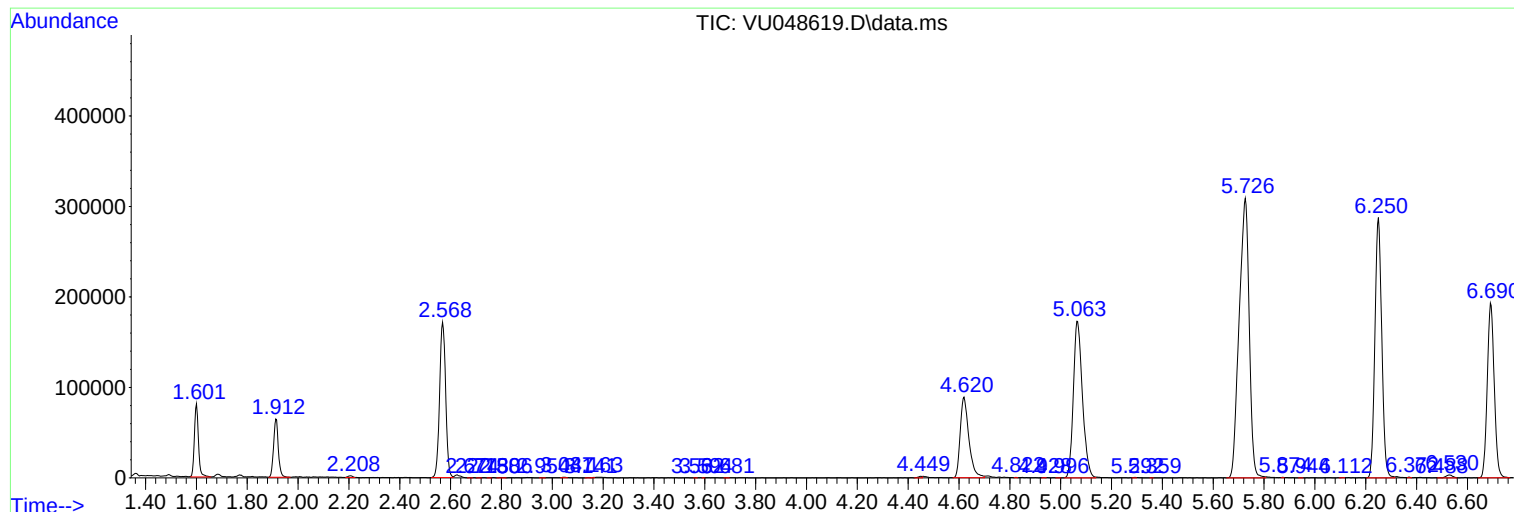

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
Data File : VU048619.D
Acq On : 18 May 2022 17:18
Operator : SY/MD
Sample : N2849-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
Data File : VU048619.D
Acq On : 18 May 2022 17:18
Operator : SY/MD
Sample : N2849-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc