


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051822\
 Data File : VU048605.D
 Acq On : 18 May 2022 08:52
 Operator : SY/MD
 Sample : BFB089
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB089

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis
 Last Update : Tue May 24 02:53:22 2022

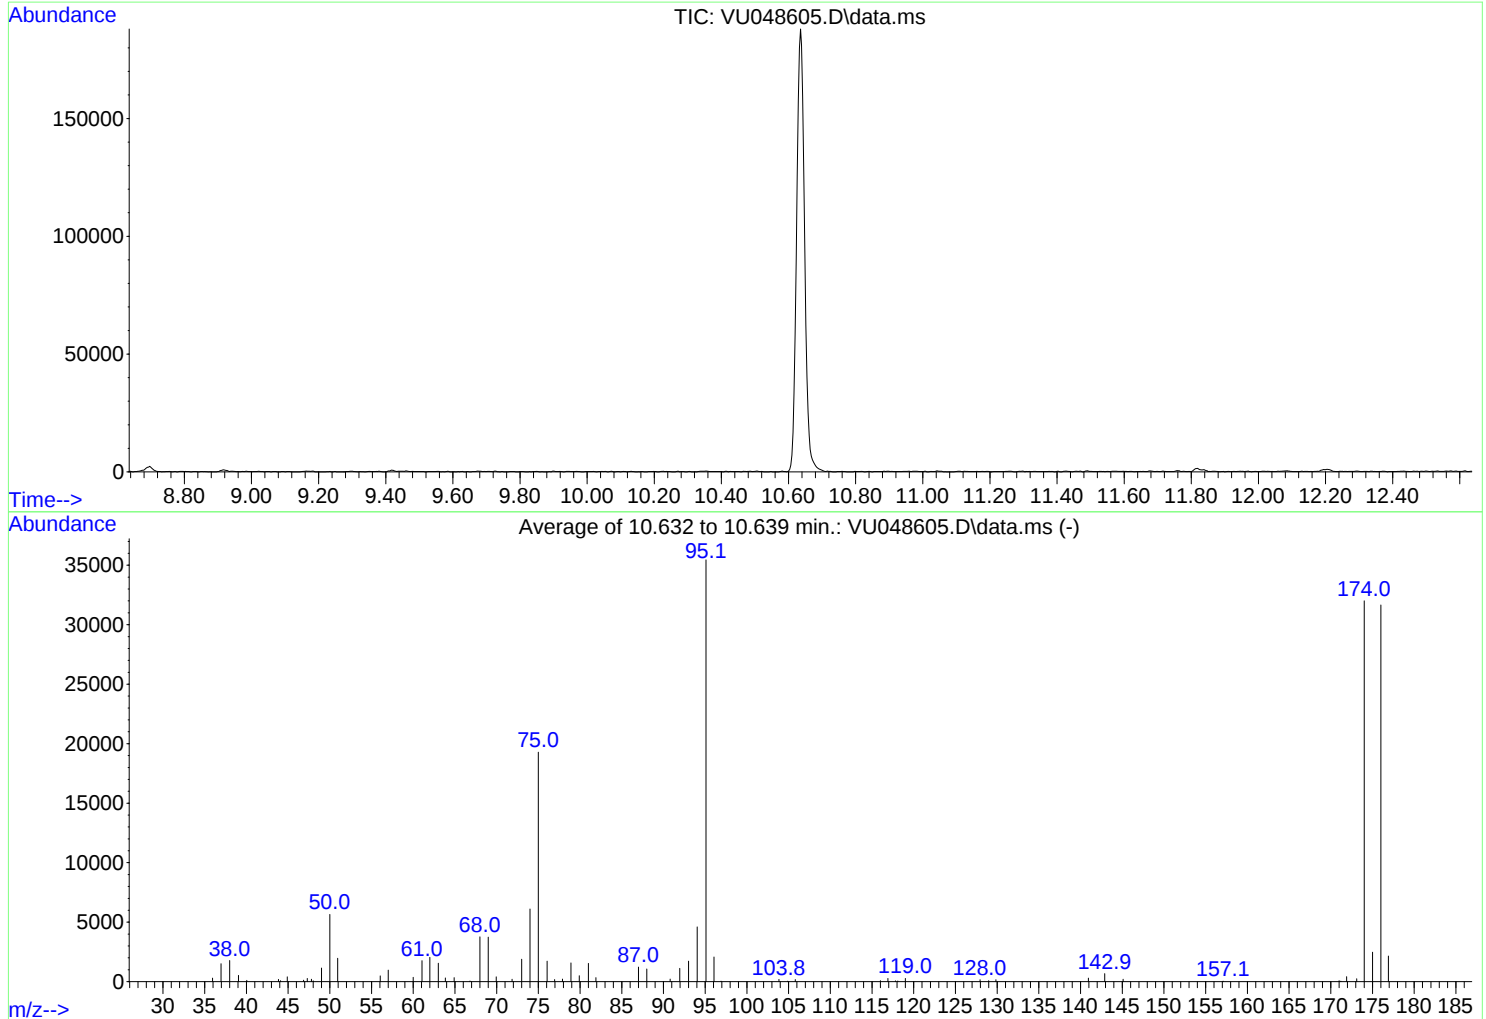

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	5651	PASS
75	95	30	80	54.4	19291	PASS
95	95	100	100	100.0	35451	PASS
96	95	5	9	5.8	2070	PASS
173	174	0.00	2	0.7	240	PASS
174	95	50	120	90.3	32003	PASS
175	174	5	9	7.7	2474	PASS
176	174	95	101	98.9	31661	PASS
177	176	5	9	6.8	2154	PASS

Scan 2878 (10.594 min): VU048605.D\data.ms
BFB089

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB089

m/z	Abundance
35.90	276.0
36.90	1511.0
38.00	1809.0
39.00	583.0
40.00	115.0
43.80	304.0
44.90	434.0
46.80	128.0
47.30	258.0
47.80	352.0
49.00	1273.0
50.00	5574.0
50.90	2000.0
56.00	389.0
57.00	888.0
60.00	347.0
61.00	1641.0
62.00	2021.0
63.00	1475.0
63.80	280.0
64.80	306.0
68.00	3795.0
69.00	3805.0
69.90	448.0
71.80	187.0
73.00	1982.0
74.00	6131.0
75.00	19248.0
76.00	1665.0
76.90	195.0
77.90	226.0
78.90	1567.0
79.90	518.0
81.00	1482.0
81.90	345.0
87.00	1129.0
88.00	946.0
90.80	240.0
92.00	1141.0
93.00	1670.0
94.00	4640.0
95.10	35064.0
96.10	2069.0
103.90	199.0
105.70	189.0
116.00	133.0
116.80	285.0
117.80	115.0
119.00	267.0
127.90	177.0
129.80	171.0
140.90	321.0
142.90	590.0
145.10	194.0
171.00	140.0
171.90	397.0
174.00	31416.0
175.00	2524.0
176.00	30048.0
176.90	2268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB089

m/z	Abundance
35.90	315.0
36.90	1502.0
38.00	1833.0
39.00	540.0
40.00	122.0
43.90	250.0
44.90	418.0
46.80	109.0
47.30	305.0
47.80	271.0
49.00	1127.0
50.00	5857.0
51.00	2007.0
56.10	500.0
57.00	1013.0
60.00	375.0
61.10	1835.0
62.00	2083.0
63.00	1575.0
63.90	314.0
64.90	324.0
68.00	3878.0
69.00	3838.0
70.00	440.0
71.80	221.0
73.00	1934.0
74.00	6203.0
75.00	19840.0
76.00	1785.0
76.90	161.0
77.90	243.0
78.90	1661.0
79.90	514.0
81.00	1565.0
81.90	338.0
87.00	1247.0
88.00	1120.0
90.80	237.0
92.00	1110.0
93.00	1757.0
94.10	4684.0
95.10	36640.0
96.00	2148.0
103.80	205.0
104.90	123.0
105.80	156.0
116.00	129.0
116.90	251.0
117.80	100.0
119.00	283.0
127.90	166.0
129.00	127.0
129.90	168.0
141.00	303.0
142.90	669.0
145.10	206.0
171.00	121.0
171.90	418.0
174.00	32816.0
175.00	2552.0
176.00	32664.0
176.90	2259.0

Instrument :
MSVOA_U
ClientSampleId :
BFB089

m/z	Abundance
36.00	290.0
37.00	1519.0
38.00	1671.0
39.10	448.0
40.10	104.0
44.10	241.0
44.90	341.0
46.90	145.0
47.30	254.0
48.00	222.0
49.00	1034.0
50.00	5521.0
51.00	1887.0
56.10	585.0
57.00	993.0
60.00	384.0
61.10	1811.0
62.00	2046.0
63.00	1597.0
63.90	317.0
65.00	360.0
66.80	173.0
68.00	3614.0
69.00	3572.0
70.00	344.0
71.90	190.0
73.00	1746.0
74.00	5981.0
75.00	18784.0
76.10	1716.0
77.00	170.0
77.90	196.0
78.90	1514.0
79.90	463.0
81.00	1552.0
81.90	334.0
87.00	1285.0
88.00	1115.0
90.80	188.0
91.90	1110.0
93.00	1743.0
94.10	4482.0
95.10	34648.0
96.00	1993.0
96.90	107.0
103.90	161.0
105.90	174.0
117.00	256.0
118.10	146.0
119.00	268.0
128.00	150.0
129.00	116.0
129.90	137.0
141.00	279.0
142.90	751.0
145.10	217.0
157.10	123.0
171.20	108.0
171.90	428.0
173.10	721.0
174.00	31776.0
175.00	2347.0
176.00	32272.0
176.90	1934.0

Instrument :
MSVOA_U
ClientSampleId :
BFB089