

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051823\
 Data File : VU054178.D
 Acq On : 18 May 2023 20:29
 Operator : JC/MD
 Sample : 02844-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBX06

Quant Time: May 19 02:10:25 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri May 19 02:02:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	179876	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	170307	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	85283	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	44409	4.579	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.600%
7) Chloroethane-d5	1.912	69	33604	4.632	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.600%
11) 1,1-Dichloroethene-d2	2.562	65	19773	4.515	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.200%
20) 2-Butanone-d5	4.633	46	83796	48.453	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.900%
24) Chloroform-d	5.057	84	79041	4.335	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
26) 1,2-Dichloroethane-d4	5.697	65	39579	4.719	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.400%
32) Benzene-d6	5.723	84	159913	4.611	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.200%
36) 1,2-Dichloropropane-d6	6.684	67	48993	4.887	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.800%
41) Toluene-d8	7.893	98	142698	4.357	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	8.176	79	18873	4.661	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.200%
46) 2-Hexanone-d5	8.629	63	59592	49.432	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.860%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	34107	4.747	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.000%
66) 1,2-Dichlorobenzene-d4	12.188	152	52793	5.073	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.400%
Target Compounds					Qvalue	
13) Acetone	2.645	43	25578	10.872	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051823\
Data File : VU054178.D
Acq On : 18 May 2023 20:29
Operator : JC/MD
Sample : 02844-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBX06

Quant Time: May 19 02:10:25 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri May 19 02:02:28 2023
Response via : Initial Calibration

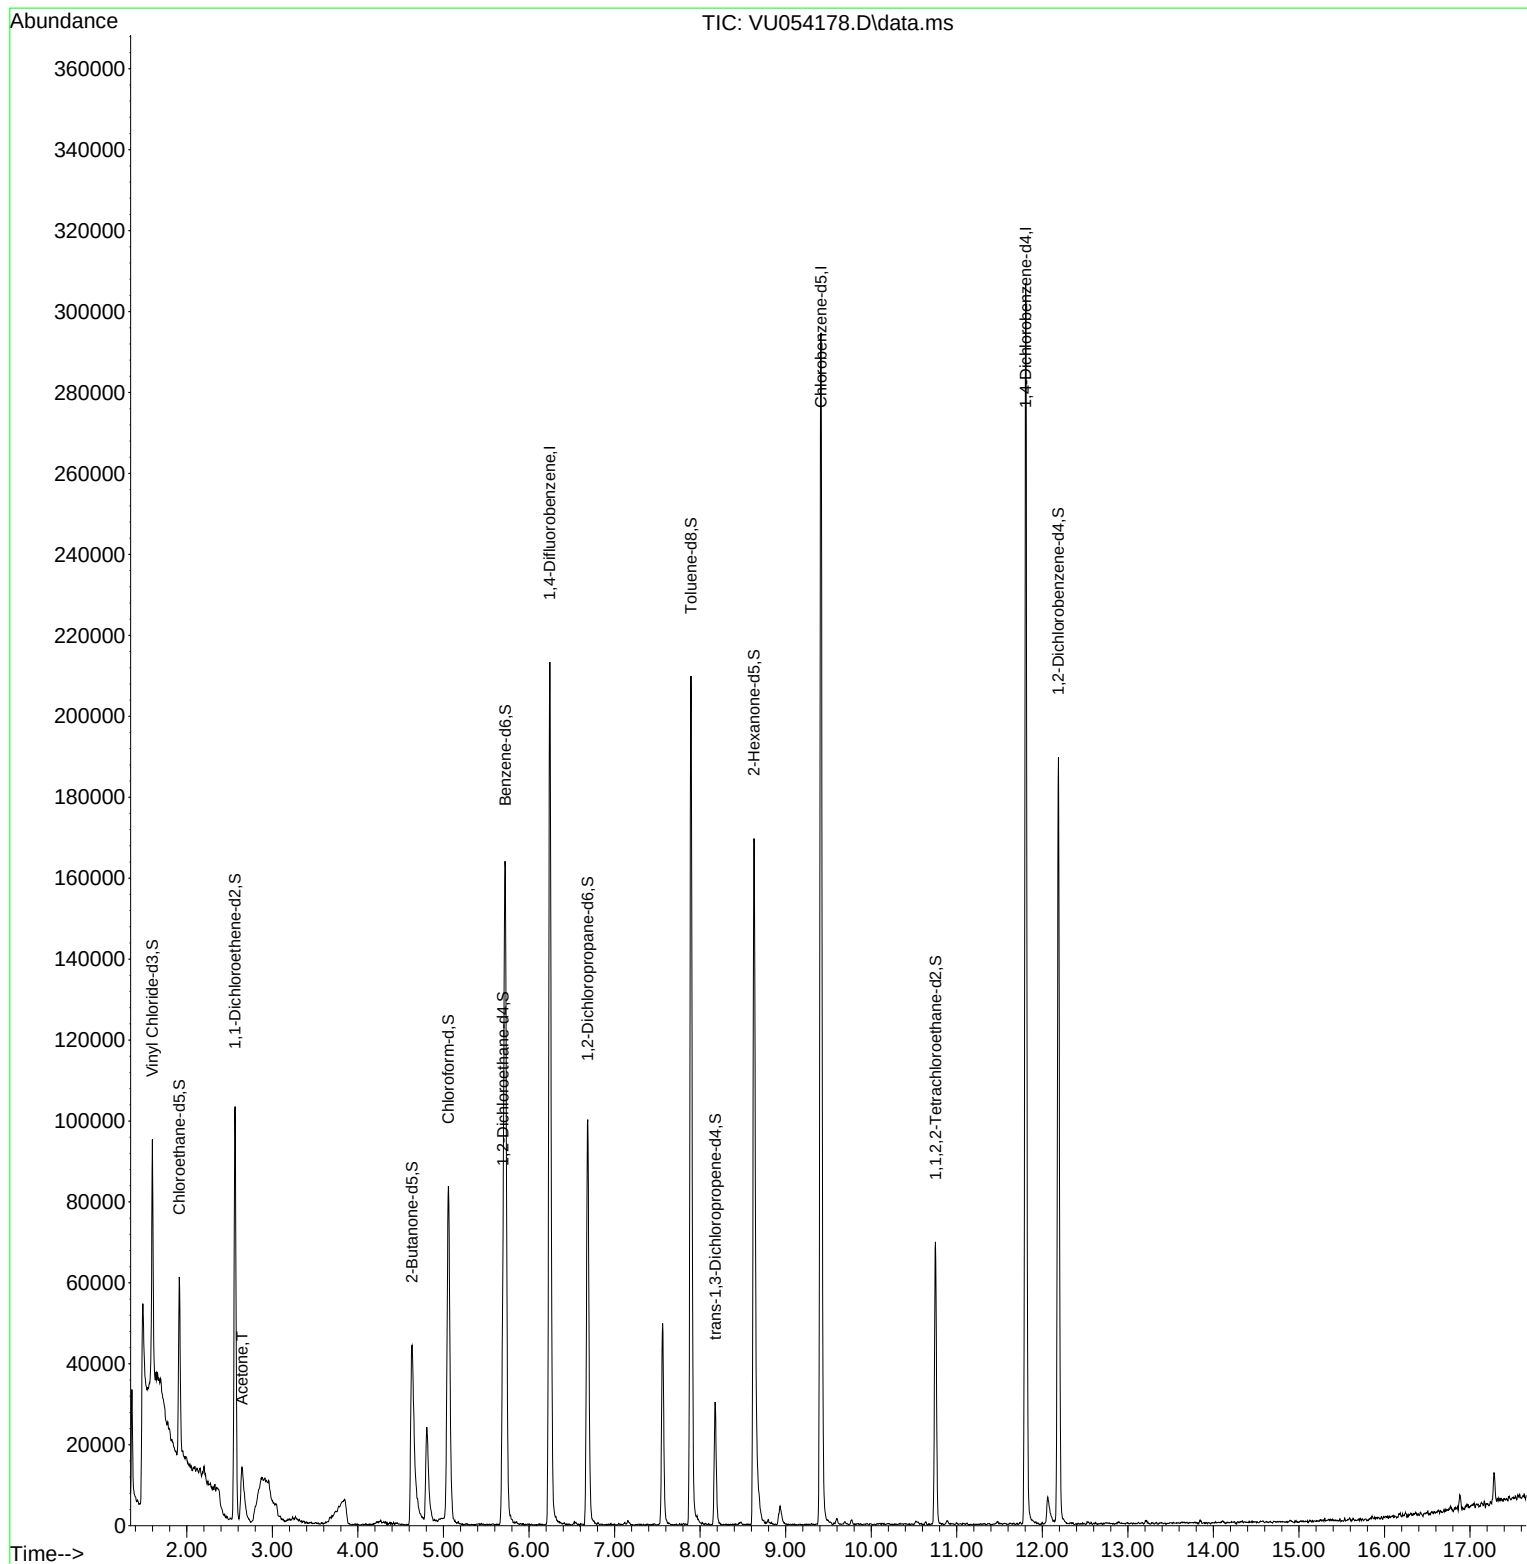

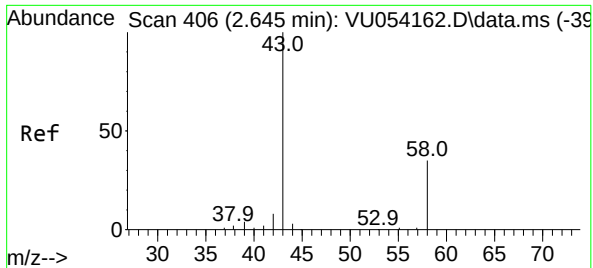

#13
 Acetone
 Concen: 10.872 ug/L
 RT: 2.645 min Scan# 406
 Delta R.T. 0.000 min
 Lab File: VU054178.D
 Acq: 18 May 2023 20:29

Instrument :
 MSVOA_U
 ClientSampleId :
 GBX06

Tgt Ion: 43 Resp: 25578
 Ion Ratio Lower Upper
 43 100
 58 34.9 0.0 73.2

