


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051823\
Data File : VU054155.D
Acq On : 18 May 2023 08:59
Operator : JC/MD
Sample : BFB011
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB011

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri May 19 04:28:00 2023

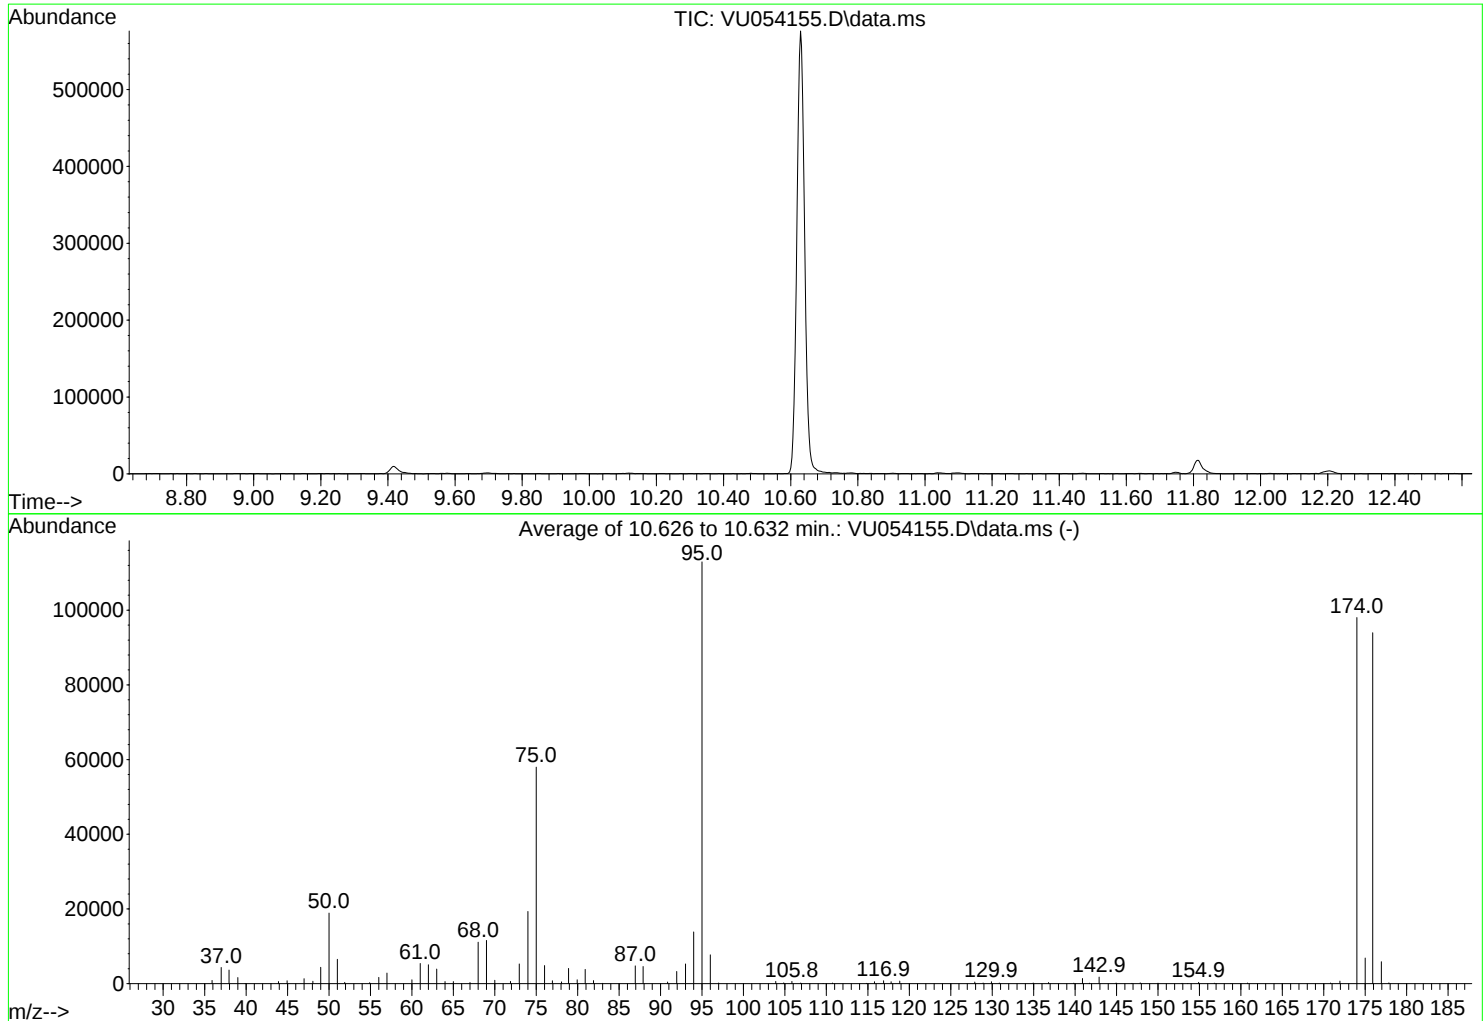

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	18907	PASS
75	95	30	80	51.3	57955	PASS
95	95	100	100	100.0	112939	PASS
96	95	5	9	6.8	7725	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	98005	PASS
175	174	5	9	7.0	6860	PASS
176	174	95	101	95.8	93936	PASS
177	176	5	9	6.2	5868	PASS

Scan 2875 (10.584 min): VU054155.D\data.ms
BFB011

m/z	Abundance
39.90	176.0
44.10	217.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	880.0
37.00	4343.0
38.00	3504.0
39.00	1543.0
39.90	261.0
43.00	108.0
43.90	700.0
45.00	783.0
47.00	1332.0
48.10	598.0
49.00	4555.0
50.00	18520.0
51.00	6634.0
51.90	341.0
54.90	302.0
56.00	1741.0
57.00	2646.0
60.00	975.0
61.00	5313.0
62.00	5205.0
63.00	3885.0
64.00	568.0
65.00	454.0
67.00	261.0
68.00	10635.0
69.00	11658.0
70.00	913.0
71.90	549.0
72.90	4909.0
74.00	18792.0
75.00	57608.0
76.00	4958.0
77.00	871.0
78.10	541.0
78.90	4003.0
79.90	998.0
80.90	3706.0
81.90	839.0
83.00	114.0
87.00	4451.0
87.90	4403.0
90.90	439.0
92.00	3306.0
93.00	5045.0
94.00	13350.0
95.00	109880.0
96.00	7732.0
97.00	179.0
103.90	637.0
104.90	203.0
105.80	635.0
106.90	147.0
109.60	109.0
110.70	140.0
114.90	104.0
115.80	514.0
116.90	744.0
117.80	448.0
118.90	636.0
127.90	432.0
128.90	174.0
129.90	401.0
130.80	168.0
134.90	190.0
136.80	254.0
139.80	112.0
140.90	1374.0
141.80	137.0
142.90	1681.0
145.00	193.0
146.90	127.0
147.90	225.0
150.00	155.0
153.60	106.0
154.90	395.0
156.80	185.0
160.80	164.0
170.80	154.0
172.00	670.0
174.00	93560.0
175.00	6674.0
175.90	89176.0
176.90	5744.0
177.90	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	893.0
37.00	4437.0
37.90	3736.0
39.00	1704.0
39.90	215.0
43.90	774.0
45.00	795.0
47.00	1383.0
48.10	693.0
49.00	4525.0
50.00	19416.0
51.00	6822.0
51.90	338.0
54.90	247.0
56.00	1705.0
57.00	2885.0
60.00	1076.0
61.00	5645.0
62.00	5129.0
63.00	4043.0
64.00	563.0
65.00	568.0
67.00	280.0
68.00	11456.0
69.00	11838.0
70.00	928.0
71.90	617.0
73.00	5444.0
74.00	19952.0
75.00	59696.0
76.00	4982.0
77.00	784.0
78.10	502.0
78.90	4224.0
79.90	1080.0
80.90	3937.0
81.90	823.0
83.00	111.0
86.90	4928.0
87.90	4725.0
90.90	467.0
92.00	3397.0
93.00	5471.0
94.00	14382.0
95.00	116416.0
96.00	8059.0
97.00	184.0
103.90	637.0
104.90	207.0
105.80	615.0
106.90	165.0
110.80	187.0
115.80	564.0
116.90	745.0
117.80	502.0
118.80	689.0
127.90	469.0
128.90	187.0
129.90	527.0
130.90	164.0
134.90	183.0
136.80	322.0
139.90	142.0
140.90	1426.0
141.70	121.0
142.90	1840.0
145.00	187.0
146.80	114.0
147.90	224.0
150.00	145.0
152.90	113.0
154.90	364.0
157.00	201.0
160.80	201.0
170.80	175.0
171.90	721.0
174.00	101104.0
175.00	7032.0
175.90	97272.0
176.90	6040.0
177.90	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011

m/z	Abundance
35.90	766.0
37.00	4191.0
37.90	3735.0
39.00	1605.0
40.00	154.0
43.90	814.0
44.90	754.0
47.00	1297.0
48.00	621.0
49.00	4098.0
50.00	18784.0
51.00	6049.0
51.90	309.0
54.90	206.0
56.00	1514.0
57.00	2992.0
60.00	1038.0
61.00	5274.0
62.00	4841.0
63.00	3748.0
64.00	572.0
65.00	603.0
67.00	302.0
68.00	11150.0
69.00	11220.0
70.00	840.0
71.90	592.0
73.00	5476.0
74.00	19296.0
75.00	56560.0
76.00	4642.0
76.90	676.0
77.90	378.0
78.90	4006.0
80.00	1021.0
80.90	3771.0
81.90	765.0
86.90	4837.0
87.90	4620.0
90.80	428.0
91.90	3084.0
93.00	5326.0
94.00	13746.0
95.00	112520.0
96.00	7384.0
97.00	206.0
103.90	509.0
104.80	195.0
105.90	543.0
106.90	152.0
110.80	205.0
114.80	112.0
115.80	507.0
116.90	775.0
117.80	570.0
118.80	695.0
127.90	400.0
128.90	203.0
129.90	624.0
130.90	166.0
135.00	188.0
136.80	328.0
139.90	141.0
140.90	1293.0
141.80	118.0
142.90	1721.0
144.80	179.0
147.80	233.0
150.00	129.0
152.90	139.0
154.90	307.0
156.80	227.0
158.80	122.0
160.80	220.0
170.80	147.0
171.90	686.0
174.00	99352.0
175.00	6874.0
175.90	95360.0
177.00	5821.0
177.80	166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB011