
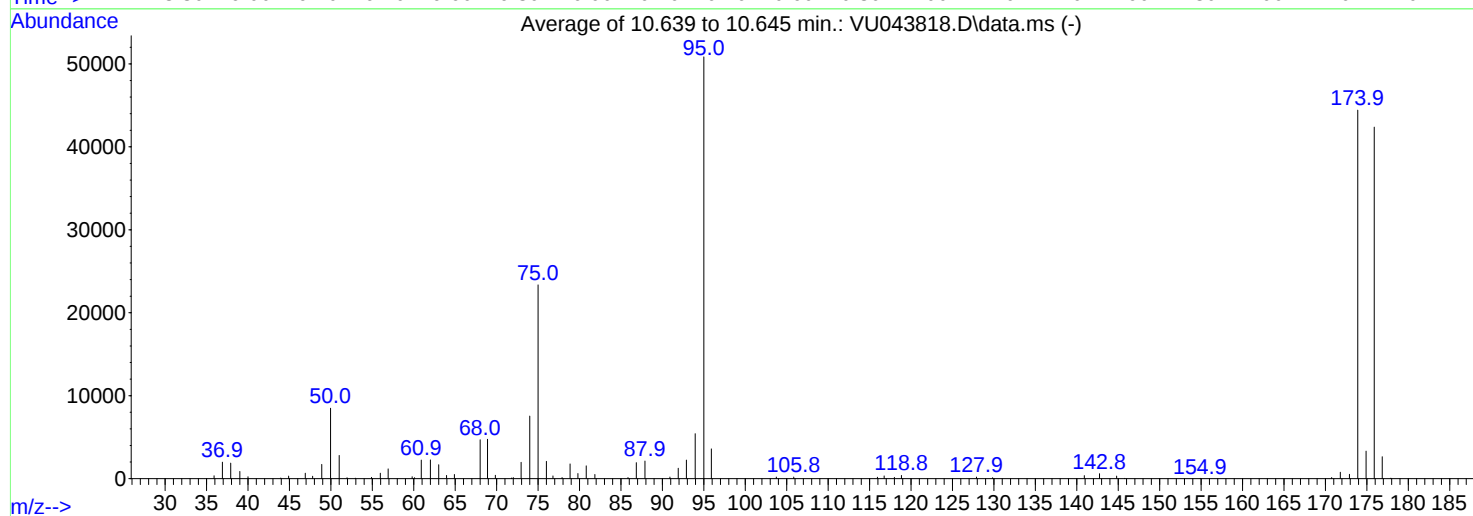


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051921\
 Data File : VU043818.D
 Acq On : 19 May 2021 08:55
 Operator : SY/MD
 Sample : BFB47
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB147

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051421WMA.M
 Title : VOC Analysis
 Last Update : Thu May 20 03:28:54 2021

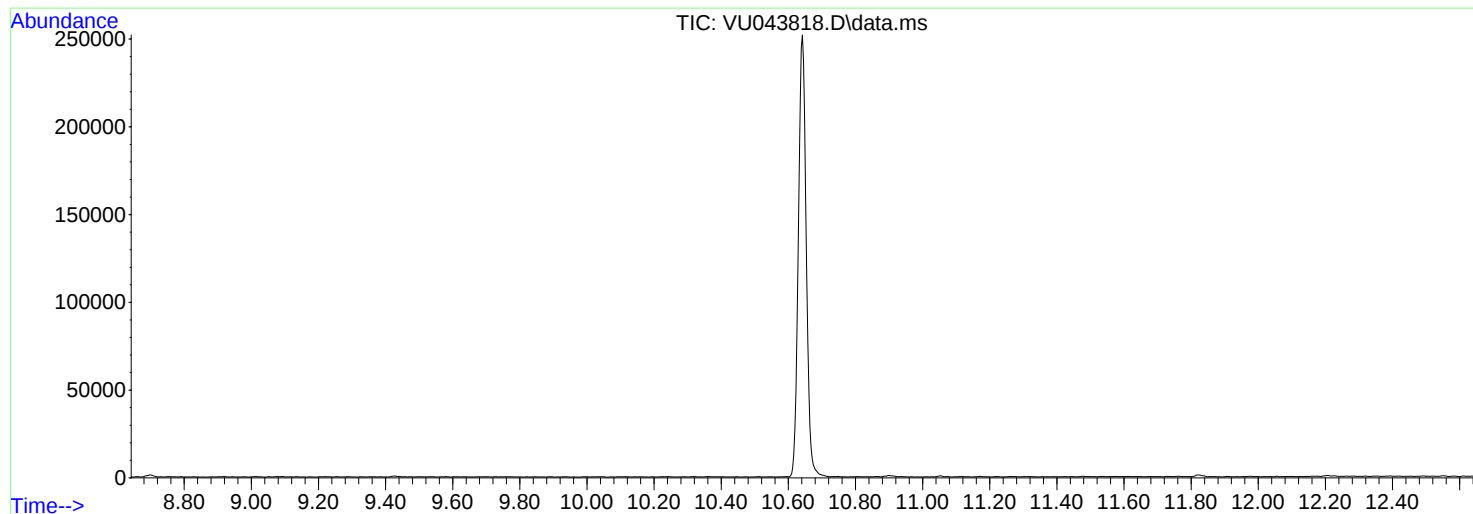

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	8480	PASS
75	95	30	80	45.9	23365	PASS
95	95	100	100	100.0	50851	PASS
96	95	5	9	7.1	3588	PASS
173	174	0.00	2	1.2	529	PASS
174	95	50	120	87.4	44419	PASS
175	174	5	9	7.5	3313	PASS
176	174	95	101	95.4	42384	PASS
177	176	5	9	6.2	2648	PASS

Scan 2880 (10.600 min): VU043818.D\data.ms
BFB47

m/z	Abundance
39.80	124.0
43.90	518.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	363.0
36.90	2012.0
37.90	2002.0
39.00	925.0
39.90	260.0
44.00	557.0
44.90	308.0
46.90	764.0
47.70	324.0
48.90	1760.0
49.90	8703.0
51.00	2756.0
51.90	118.0
52.90	105.0
54.90	147.0
55.90	704.0
56.90	1191.0
59.80	334.0
60.90	2269.0
62.00	2226.0
63.00	1606.0
64.00	430.0
64.90	544.0
68.00	4628.0
68.90	4812.0
69.90	434.0
71.80	210.0
73.00	1999.0
74.00	7747.0
75.00	23680.0
76.00	2143.0
76.80	382.0
78.00	231.0
78.90	1726.0
79.80	567.0
80.80	1553.0
81.80	501.0
85.80	144.0
86.90	2038.0
87.90	2105.0
90.90	211.0
91.90	1293.0
92.90	2252.0
93.90	5425.0
95.00	50272.0
95.90	3709.0
103.80	207.0
105.90	192.0
115.90	173.0
116.70	320.0
118.00	130.0
118.80	381.0
127.90	206.0
129.90	121.0
140.90	333.0
142.70	595.0
144.80	329.0
170.80	152.0
171.80	770.0
172.90	472.0
173.90	43968.0
174.90	3288.0
175.90	42000.0
176.80	2754.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	353.0
36.90	2020.0
37.90	1929.0
39.00	906.0
40.00	228.0
44.00	607.0
44.90	319.0
46.90	674.0
47.80	294.0
48.90	1757.0
50.00	8808.0
51.00	2889.0
51.90	133.0
53.00	101.0
54.90	147.0
55.90	665.0
56.90	1211.0
59.80	341.0
60.90	2287.0
62.00	2295.0
63.00	1733.0
64.00	390.0
64.90	513.0
68.00	4897.0
68.90	4883.0
69.90	422.0
72.00	199.0
72.90	2030.0
74.00	7689.0
75.00	24152.0
76.00	2181.0
76.80	334.0
78.90	1846.0
79.80	632.0
80.80	1567.0
81.80	510.0
85.90	150.0
86.90	1968.0
87.90	2175.0
90.90	210.0
91.90	1275.0
92.90	2305.0
93.90	5563.0
95.00	52552.0
95.90	3738.0
103.70	188.0
105.90	183.0
115.90	185.0
116.70	318.0
118.00	170.0
118.90	386.0
127.90	214.0
129.90	118.0
140.90	397.0
142.70	619.0
144.80	310.0
145.80	101.0
170.80	146.0
171.80	780.0
172.90	546.0
173.90	45912.0
174.90	3414.0
175.90	43600.0
176.90	2703.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
35.90	344.0
36.90	1936.0
37.90	1708.0
39.00	778.0
39.70	202.0
40.10	212.0
44.00	648.0
44.90	313.0
46.90	562.0
47.90	258.0
48.90	1627.0
50.00	7930.0
51.00	2733.0
52.00	124.0
54.90	165.0
56.00	608.0
56.90	1121.0
60.10	346.0
60.90	2135.0
62.00	2224.0
63.00	1703.0
63.90	334.0
64.90	435.0
68.00	4563.0
68.90	4552.0
69.80	367.0
72.00	183.0
72.90	1875.0
74.00	7175.0
75.00	22264.0
76.00	1938.0
76.80	290.0
77.80	159.0
78.80	1775.0
79.80	632.0
80.80	1517.0
81.90	483.0
85.90	131.0
86.80	1762.0
87.90	2092.0
90.90	169.0
91.90	1184.0
92.90	2136.0
94.00	5289.0
95.00	49728.0
95.90	3318.0
103.70	160.0
105.80	193.0
116.00	180.0
116.80	342.0
118.00	158.0
118.90	392.0
127.90	183.0
129.80	122.0
140.90	400.0
142.80	604.0
144.80	279.0
154.90	117.0
170.70	115.0
171.80	775.0
172.90	569.0
173.90	43376.0
174.90	3236.0
175.90	41552.0
176.90	2486.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147