

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048624.D
 Acq On : 19 May 2022 10:40
 Operator : SY/MD
 Sample : VU0519MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK132

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB	75212	87447	10.17%	1.260%
2	1.912	169	178	193	rVB	64040	83291	9.69%	1.200%
3	2.276	288	291	292	rBV	265	139	0.02%	0.002%
4	2.475	350	353	358	rBV	240	174	0.02%	0.003%
5	2.568	370	382	398	rBV	175081	286929	33.37%	4.133%
6	2.752	436	439	442	rBB	216	158	0.02%	0.002%
7	2.803	444	455	461	rBV2	893	1838	0.21%	0.026%
8	3.054	525	533	537	rBV4	926	1220	0.14%	0.018%
9	3.192	565	576	587	rBV2	2564	5148	0.60%	0.074%
10	3.356	620	627	636	rBB3	760	1036	0.12%	0.015%
11	3.414	641	645	647	rBV	158	158	0.02%	0.002%
12	4.147	870	873	878	rBB	216	246	0.03%	0.004%
13	4.475	972	975	981	rBB	210	208	0.02%	0.003%
14	4.571	1002	1005	1008	rBV	226	210	0.02%	0.003%
15	4.623	1008	1021	1045	rBV	89378	220994	25.70%	3.184%
16	4.848	1087	1091	1097	rVB3	579	439	0.05%	0.006%
17	4.932	1113	1117	1120	rBB	281	148	0.02%	0.002%
18	4.951	1121	1123	1125	rBB	305	139	0.02%	0.002%
19	4.967	1125	1128	1130	rBB	250	138	0.02%	0.002%
20	5.063	1142	1158	1183	rBV	168703	371750	43.23%	5.355%
21	5.176	1190	1193	1195	rBV2	323	177	0.02%	0.003%
22	5.215	1202	1205	1210	rBV2	280	267	0.03%	0.004%
23	5.282	1222	1226	1229	rBV	657	450	0.05%	0.006%
24	5.385	1256	1258	1261	rBB	279	168	0.02%	0.002%
25	5.504	1291	1295	1298	rBB	161	153	0.02%	0.002%
26	5.520	1298	1300	1303	rBV	230	179	0.02%	0.003%
27	5.726	1342	1364	1387	rBV2	310509	859916	100.00%	12.387%
28	5.893	1413	1416	1419	rVB	386	298	0.03%	0.004%
29	5.938	1426	1430	1433	rBB2	351	261	0.03%	0.004%
30	5.989	1444	1446	1448	rBV	348	153	0.02%	0.002%
31	6.034	1458	1460	1462	rBV2	391	210	0.02%	0.003%
32	6.051	1463	1465	1469	rVB2	252	179	0.02%	0.003%
33	6.250	1512	1527	1545	rBV	267608	499919	58.14%	7.202%
34	6.501	1601	1605	1606	rBV2	247	163	0.02%	0.002%
35	6.530	1606	1614	1624	rVV5	4887	8451	0.98%	0.122%
36	6.694	1651	1665	1683	rBV	192648	374562	43.56%	5.396%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048624.D
 Acq On : 19 May 2022 10:40
 Operator : SY/MD
 Sample : VU0519MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK132

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.793	1694	1696	1698	rBV	297	176	0.02%	0.003%
38	6.809	1698	1701	1703	rBV2	546	305	0.04%	0.004%
39	6.858	1712	1716	1719	rBB2	227	178	0.02%	0.003%
40	6.960	1743	1748	1753	rBV	200	294	0.03%	0.004%
41	7.186	1810	1818	1826	rBV5	1699	2499	0.29%	0.036%
42	7.337	1862	1865	1868	rBB2	262	209	0.02%	0.003%
43	7.362	1871	1873	1878	rBV	264	229	0.03%	0.003%
44	7.565	1924	1936	1949	rBV	117694	205982	23.95%	2.967%
45	7.642	1958	1960	1964	rBV2	252	174	0.02%	0.003%
46	7.694	1970	1976	1979	rVB3	805	775	0.09%	0.011%
47	7.742	1987	1991	1994	rBB	202	157	0.02%	0.002%
48	7.803	2000	2010	2016	rVV5	842	1327	0.15%	0.019%
49	7.899	2024	2040	2058	rBV	403941	690153	80.26%	9.942%
50	8.073	2090	2094	2098	rBV3	464	486	0.06%	0.007%
51	8.124	2107	2110	2113	rBV2	267	212	0.02%	0.003%
52	8.179	2115	2127	2143	rBV	86035	147982	17.21%	2.132%
53	8.407	2196	2198	2202	rBV2	352	265	0.03%	0.004%
54	8.462	2212	2215	2219	rBV2	257	198	0.02%	0.003%
55	8.546	2237	2241	2242	rBV	903	500	0.06%	0.007%
56	8.632	2254	2268	2307	rBV	273349	495864	57.66%	7.143%
57	8.809	2321	2323	2329	rVB3	519	401	0.05%	0.006%
58	8.877	2342	2344	2347	rVB	278	162	0.02%	0.002%
59	8.912	2348	2355	2356	rBV2	1668	1802	0.21%	0.026%
60	9.021	2386	2389	2391	rBB	269	142	0.02%	0.002%
61	9.041	2392	2395	2400	rBV	211	259	0.03%	0.004%
62	9.240	2455	2457	2460	rVB	303	172	0.02%	0.002%
63	9.346	2487	2490	2493	rBV	171	167	0.02%	0.002%
64	9.417	2499	2512	2534	rBV	377631	634419	73.78%	9.139%
65	9.571	2553	2560	2567	rBV3	1271	1706	0.20%	0.025%
66	9.623	2574	2576	2580	rVB	303	195	0.02%	0.003%
67	9.655	2580	2586	2588	rBV	301	280	0.03%	0.004%
68	9.697	2592	2599	2606	rVV2	1208	1937	0.23%	0.028%
69	9.899	2659	2662	2668	rBV2	303	239	0.03%	0.003%
70	10.012	2694	2697	2700	rBB	203	167	0.02%	0.002%
71	10.037	2700	2705	2707	rBV	194	203	0.02%	0.003%
72	10.095	2718	2723	2724	rBV2	682	537	0.06%	0.008%
73	10.285	2776	2782	2785	rBV2	367	413	0.05%	0.006%
74	10.484	2839	2844	2850	rVV2	669	915	0.11%	0.013%
75	10.639	2884	2892	2897	rBV4	1474	2042	0.24%	0.029%
76	10.664	2897	2900	2901	rBV	534	318	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048624.D
 Acq On : 19 May 2022 10:40
 Operator : SY/MD
 Sample : VU0519MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK132

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.758	2917	2929	2947	rBV	295770	477567	55.54%	6.880%
78	10.928	2977	2982	2984	rBV	198	226	0.03%	0.003%
79	11.063	3019	3024	3026	rBV	204	221	0.03%	0.003%
80	11.092	3026	3033	3039	rVB3	443	633	0.07%	0.009%
81	11.153	3046	3052	3053	rBV	262	215	0.03%	0.003%
82	11.256	3081	3084	3086	rBV	218	169	0.02%	0.002%
83	11.417	3131	3134	3141	rVB	257	197	0.02%	0.003%
84	11.465	3141	3149	3151	rBV3	1631	1606	0.19%	0.023%
85	11.748	3230	3237	3245	rBV4	2532	3395	0.39%	0.049%
86	11.812	3245	3257	3273	rBV	431836	695863	80.92%	10.024%
87	12.108	3343	3349	3350	rBV	213	228	0.03%	0.003%
88	12.195	3362	3376	3397	rBV	449225	731569	85.07%	10.539%
89	12.449	3452	3455	3458	rVB	326	160	0.02%	0.002%
90	12.533	3477	3481	3484	rVB2	285	254	0.03%	0.004%
91	13.037	3636	3638	3643	rVB	224	165	0.02%	0.002%
92	13.118	3660	3663	3670	rVB2	276	290	0.03%	0.004%
93	13.224	3689	3696	3700	rBV5	2368	2640	0.31%	0.038%
94	13.282	3710	3714	3715	rBV	378	178	0.02%	0.003%
95	13.410	3751	3754	3756	rBV2	224	162	0.02%	0.002%
96	13.623	3817	3820	3825	rBV2	329	372	0.04%	0.005%
97	13.848	3883	3890	3901	rVB4	3346	4905	0.57%	0.071%
98	14.089	3957	3965	3979	rBV3	9116	14635	1.70%	0.211%
99	14.288	4024	4027	4028	rBV	260	165	0.02%	0.002%
100	14.333	4035	4041	4050	rVB4	2988	4258	0.50%	0.061%




Sum of corrected areas: 6941830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048624.D
Acq On : 19 May 2022 10:40
Operator : SY/MD
Sample : VU0519MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

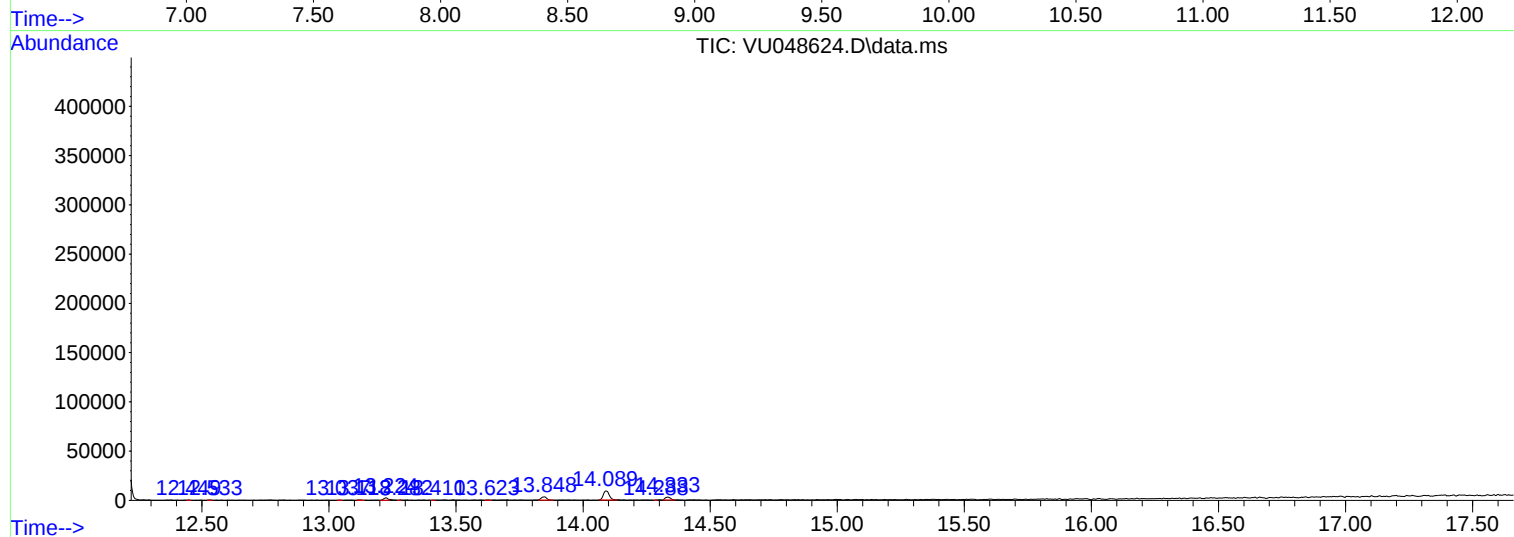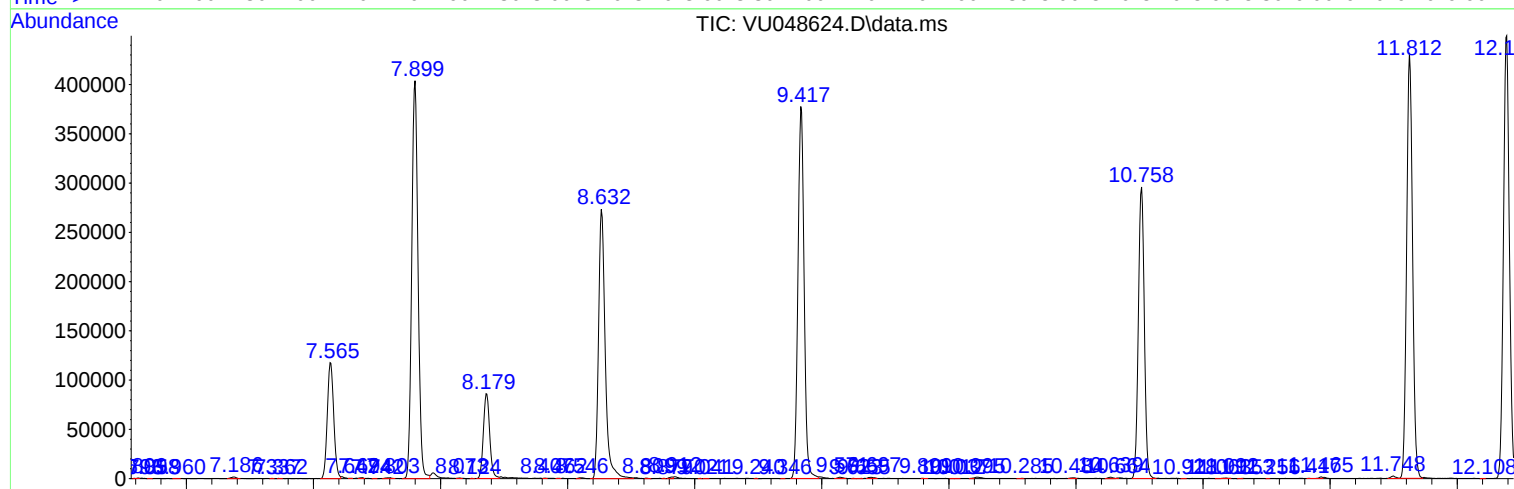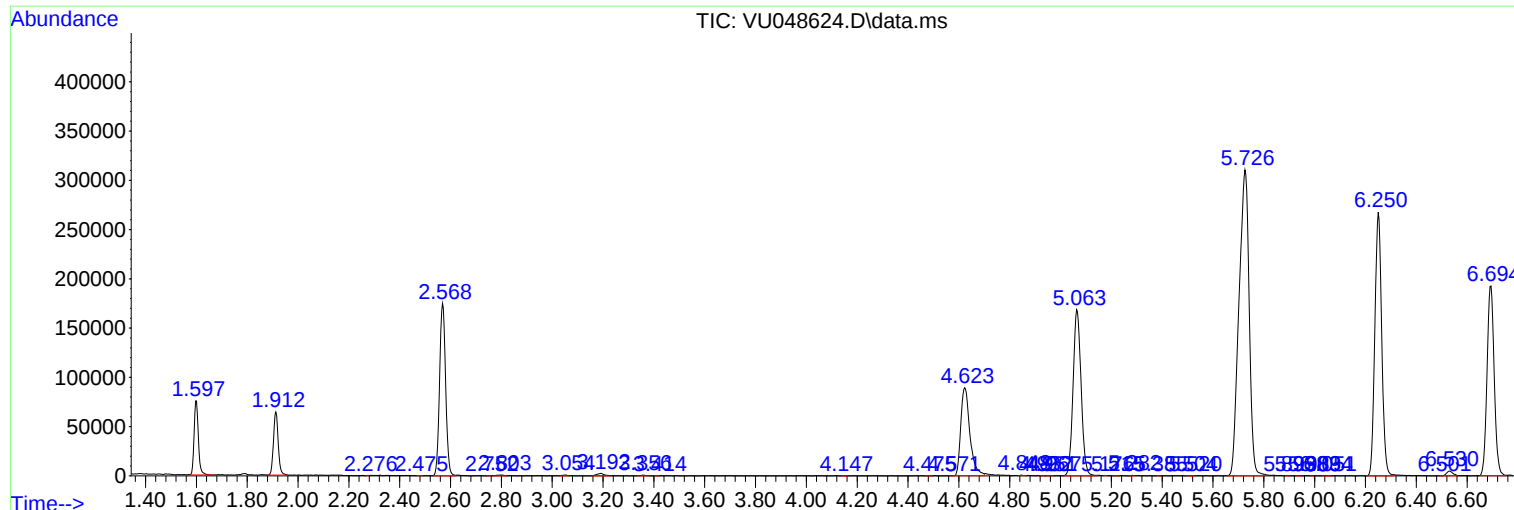

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048624.D
Acq On : 19 May 2022 10:40
Operator : SY/MD
Sample : VU0519MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048624.D
Acq On : 19 May 2022 10:40
Operator : SY/MD
Sample : VU0519MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK132

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc