

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048626.D
 Acq On : 19 May 2022 11:32
 Operator : SY/MD
 Sample : N2848-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	98	rVB	70951	80510	9.92%	1.225%
2	1.912	170	178	198	rVB	58987	77257	9.52%	1.176%
3	2.247	279	282	285	rBV2	259	211	0.03%	0.003%
4	2.488	350	357	362	rBV	249	403	0.05%	0.006%
5	2.568	370	382	405	rBV	160204	262848	32.40%	4.000%
6	2.662	408	411	418	rVB	257	301	0.04%	0.005%
7	2.729	429	432	438	rBB	168	215	0.03%	0.003%
8	2.861	470	473	481	rBV	292	329	0.04%	0.005%
9	2.954	499	502	506	rBB2	241	150	0.02%	0.002%
10	3.051	526	532	537	rBB2	666	751	0.09%	0.011%
11	3.076	538	540	543	rBV	182	141	0.02%	0.002%
12	3.183	563	573	574	rBV2	1858	1898	0.23%	0.029%
13	3.289	603	606	610	rBV	159	181	0.02%	0.003%
14	3.449	653	656	658	rBB	269	150	0.02%	0.002%
15	3.469	659	662	667	rBB	166	161	0.02%	0.002%
16	3.520	671	678	680	rBB	255	191	0.02%	0.003%
17	3.539	681	684	686	rBB	232	135	0.02%	0.002%
18	3.581	694	697	701	rBV	343	247	0.03%	0.004%
19	4.125	862	866	869	rBB	298	218	0.03%	0.003%
20	4.215	889	894	897	rBV	178	216	0.03%	0.003%
21	4.626	1008	1022	1044	rBV2	83907	215352	26.54%	3.277%
22	4.883	1094	1102	1106	rBV	432	393	0.05%	0.006%
23	4.967	1123	1128	1131	rBV2	344	294	0.04%	0.004%
24	5.067	1143	1159	1179	rBV	159922	350543	43.20%	5.335%
25	5.224	1204	1208	1210	rBV	149	131	0.02%	0.002%
26	5.292	1226	1229	1233	rVB2	315	157	0.02%	0.002%
27	5.346	1244	1246	1250	rVB2	229	153	0.02%	0.002%
28	5.424	1267	1270	1272	rBV	227	130	0.02%	0.002%
29	5.726	1342	1364	1382	rBV2	292990	811364	100.00%	12.348%
30	5.883	1410	1413	1415	rVB2	258	142	0.02%	0.002%
31	6.038	1458	1461	1463	rBV	230	178	0.02%	0.003%
32	6.112	1479	1484	1486	rBV	235	248	0.03%	0.004%
33	6.250	1513	1527	1552	rBV	247856	469901	57.91%	7.151%
34	6.395	1570	1572	1575	rVB2	336	167	0.02%	0.003%
35	6.417	1575	1579	1581	rVB2	426	244	0.03%	0.004%
36	6.430	1581	1583	1585	rVB	354	155	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048626.D
 Acq On : 19 May 2022 11:32
 Operator : SY/MD
 Sample : N2848-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.472	1593	1596	1599	rVB2	343	241	0.03%	0.004%
38	6.533	1603	1615	1624	rBB6	4216	7446	0.92%	0.113%
39	6.694	1651	1665	1689	rBV	180722	356159	43.90%	5.420%
40	6.800	1693	1698	1705	rVV3	479	582	0.07%	0.009%
41	6.877	1720	1722	1725	rBV	207	155	0.02%	0.002%
42	7.186	1806	1818	1821	rBV3	1413	1657	0.20%	0.025%
43	7.472	1904	1907	1911	rBB	186	176	0.02%	0.003%
44	7.565	1924	1936	1954	rBV	108070	195899	24.14%	2.981%
45	7.645	1956	1961	1964	rVB3	608	606	0.07%	0.009%
46	7.735	1988	1989	1993	rBV	211	156	0.02%	0.002%
47	7.796	2004	2008	2014	rBB2	665	642	0.08%	0.010%
48	7.851	2021	2025	2027	rBV	179	159	0.02%	0.002%
49	7.899	2027	2040	2056	rBV	374649	639187	78.78%	9.728%
50	8.182	2116	2128	2148	rBV	82286	142760	17.60%	2.173%
51	8.366	2183	2185	2186	rBV	287	132	0.02%	0.002%
52	8.433	2200	2206	2207	rBV2	444	360	0.04%	0.005%
53	8.468	2213	2217	2218	rBV2	297	224	0.03%	0.003%
54	8.497	2224	2226	2229	rBV	422	204	0.03%	0.003%
55	8.555	2237	2244	2247	rBV2	513	498	0.06%	0.008%
56	8.636	2256	2269	2302	rBV3	263125	488013	60.15%	7.427%
57	8.848	2332	2335	2338	rBB	319	183	0.02%	0.003%
58	8.874	2340	2343	2347	rVB	289	219	0.03%	0.003%
59	8.906	2347	2353	2354	rBV2	1111	826	0.10%	0.013%
60	8.976	2372	2375	2377	rBV	172	140	0.02%	0.002%
61	9.182	2435	2439	2442	rVB	284	234	0.03%	0.004%
62	9.218	2446	2450	2451	rBV	221	146	0.02%	0.002%
63	9.308	2476	2478	2482	rBV2	229	183	0.02%	0.003%
64	9.417	2500	2512	2531	rBV	355792	601563	74.14%	9.155%
65	9.530	2545	2547	2549	rBV2	290	157	0.02%	0.002%
66	9.562	2554	2557	2560	rBV2	380	292	0.04%	0.004%
67	9.620	2573	2575	2578	rVB	211	137	0.02%	0.002%
68	9.687	2594	2596	2604	rVB3	680	650	0.08%	0.010%
69	9.742	2610	2613	2616	rBB	249	186	0.02%	0.003%
70	9.922	2666	2669	2674	rBB2	247	208	0.03%	0.003%
71	9.957	2675	2680	2684	rBV	325	331	0.04%	0.005%
72	10.099	2721	2724	2726	rBV2	336	194	0.02%	0.003%
73	10.404	2814	2819	2822	rBV2	253	215	0.03%	0.003%
74	10.616	2882	2885	2886	rBV2	267	162	0.02%	0.002%
75	10.658	2895	2898	2900	rBV	383	260	0.03%	0.004%
76	10.758	2916	2929	2950	rVB	293725	471292	58.09%	7.173%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048626.D
 Acq On : 19 May 2022 11:32
 Operator : SY/MD
 Sample : N2848-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	11.034	3009	3015	3022	rBB2	372	519	0.06%	0.008%
78	11.394	3122	3127	3130	rBV	224	267	0.03%	0.004%
79	11.420	3132	3135	3138	rBV	206	171	0.02%	0.003%
80	11.456	3140	3146	3147	rBV	436	328	0.04%	0.005%
81	11.565	3178	3180	3182	rBV	261	150	0.02%	0.002%
82	11.607	3191	3193	3196	rBV	192	146	0.02%	0.002%
83	11.738	3231	3234	3236	rVV2	652	388	0.05%	0.006%
84	11.812	3245	3257	3276	rBV	417993	669130	82.47%	10.183%
85	12.192	3362	3375	3392	rBV	423989	703787	86.74%	10.711%
86	12.317	3411	3414	3416	rVB	305	160	0.02%	0.002%
87	12.523	3477	3478	3483	rBV2	248	169	0.02%	0.003%
88	12.777	3554	3557	3561	rBV	281	207	0.03%	0.003%
89	13.082	3649	3652	3655	rBV2	309	219	0.03%	0.003%
90	13.217	3692	3694	3696	rBV2	664	415	0.05%	0.006%
91	13.279	3711	3713	3717	rVB	262	147	0.02%	0.002%
92	13.520	3783	3788	3793	rBV	457	362	0.04%	0.006%
93	13.687	3836	3840	3842	rBV	308	240	0.03%	0.004%
94	13.719	3847	3850	3854	rBV	519	362	0.04%	0.006%
95	13.848	3884	3890	3895	rBV4	784	1099	0.14%	0.017%
96	13.928	3912	3915	3919	rBV2	384	298	0.04%	0.005%
97	14.089	3962	3965	3975	rVB4	1655	2167	0.27%	0.033%
98	14.166	3987	3989	3995	rBV2	398	257	0.03%	0.004%
99	14.385	4056	4057	4060	rBV	223	153	0.02%	0.002%
100	15.291	4335	4339	4343	rBV3	665	708	0.09%	0.011%




Sum of corrected areas: 6570748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048626.D
Acq On : 19 May 2022 11:32
Operator : SY/MD
Sample : N2848-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

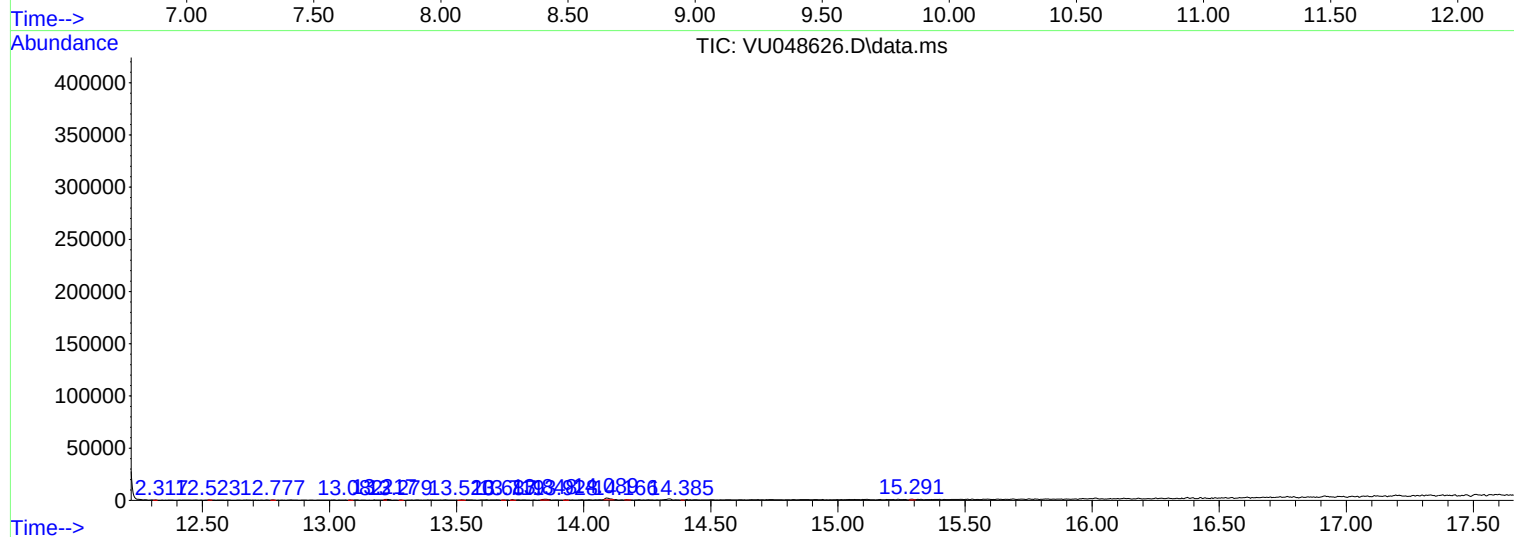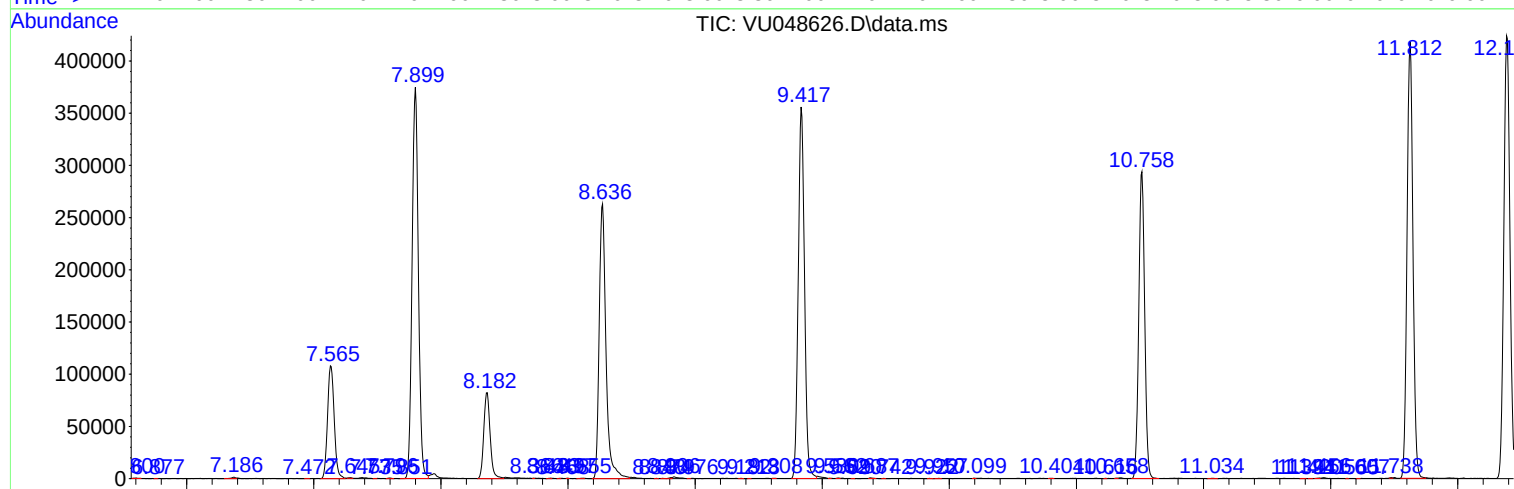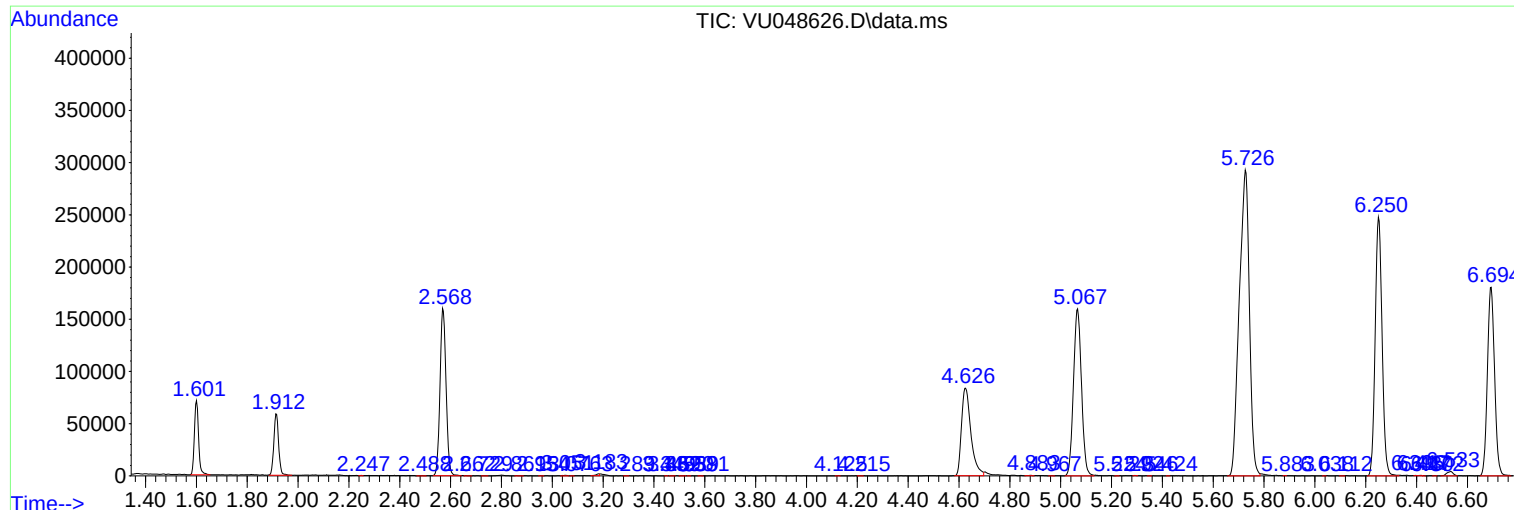

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048626.D
Acq On : 19 May 2022 11:32
Operator : SY/MD
Sample : N2848-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048626.D
Acq On : 19 May 2022 11:32
Operator : SY/MD
Sample : N2848-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc