

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048627.D
 Acq On : 19 May 2022 12:17
 Operator : SY/MD
 Sample : N2849-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	99	rVB	72179	80892	9.68%	1.105%
2	1.687	103	108	116	rVB3	3601	4535	0.54%	0.062%
3	1.912	170	178	193	rVB	59562	77618	9.29%	1.060%
4	2.205	263	269	277	rBV3	1645	2196	0.26%	0.030%
5	2.388	323	326	327	rBV3	289	171	0.02%	0.002%
6	2.568	366	382	397	rBV	164582	278479	33.33%	3.804%
7	2.784	445	449	450	rBV	441	252	0.03%	0.003%
8	2.906	484	487	490	rBV2	334	290	0.03%	0.004%
9	3.044	527	530	532	rBV	505	401	0.05%	0.005%
10	3.176	563	571	573	rBV3	610	659	0.08%	0.009%
11	3.314	610	614	619	rBB	168	214	0.03%	0.003%
12	3.388	634	637	642	rBB	184	206	0.02%	0.003%
13	3.587	695	699	702	rVV3	720	628	0.08%	0.009%
14	3.604	702	704	708	rVB	432	264	0.03%	0.004%
15	4.452	957	968	987	rBV5	9408	22674	2.71%	0.310%
16	4.520	987	989	994	rVB3	450	350	0.04%	0.005%
17	4.565	1000	1003	1005	rBV	321	239	0.03%	0.003%
18	4.626	1006	1022	1043	rBV	76384	190999	22.86%	2.609%
19	4.944	1117	1121	1125	rBB2	342	269	0.03%	0.004%
20	5.067	1143	1159	1183	rBV3	175758	437623	52.38%	5.978%
21	5.481	1285	1288	1290	rBB2	268	164	0.02%	0.002%
22	5.597	1320	1324	1327	rBB	160	163	0.02%	0.002%
23	5.645	1336	1339	1341	rBV2	263	187	0.02%	0.003%
24	5.726	1342	1364	1389	rBV2	296981	835490	100.00%	11.412%
25	5.906	1416	1420	1422	rVB2	407	301	0.04%	0.004%
26	5.973	1434	1441	1449	rVB5	1029	1655	0.20%	0.023%
27	6.137	1490	1492	1493	rVV5	380	164	0.02%	0.002%
28	6.147	1493	1495	1497	rVB	366	162	0.02%	0.002%
29	6.250	1513	1527	1549	rBV	279854	528172	63.22%	7.214%
30	6.539	1604	1617	1626	rBB7	3662	7054	0.84%	0.096%
31	6.636	1644	1647	1650	rBV	192	169	0.02%	0.002%
32	6.693	1650	1665	1682	rBV2	183708	366129	43.82%	5.001%
33	6.883	1713	1724	1739	rBV3	9745	19319	2.31%	0.264%
34	7.108	1783	1794	1806	rBB3	12873	22858	2.74%	0.312%
35	7.179	1812	1816	1817	rBV	999	625	0.07%	0.009%
36	7.285	1847	1849	1856	rBB	188	213	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048627.D
 Acq On : 19 May 2022 12:17
 Operator : SY/MD
 Sample : N2849-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	7.568	1925	1937	1953	rBV	114272	201889	24.16%	2.758%
38	7.693	1968	1976	1980	rBV4	869	1171	0.14%	0.016%
39	7.803	2001	2010	2022	rBB5	1268	2250	0.27%	0.031%
40	7.899	2027	2040	2055	rBV	394298	680492	81.45%	9.295%
41	8.102	2098	2103	2109	rVB2	167	162	0.02%	0.002%
42	8.182	2117	2128	2145	rBV	86050	148384	17.76%	2.027%
43	8.404	2195	2197	2201	rVB2	412	267	0.03%	0.004%
44	8.452	2209	2212	2213	rBV	649	311	0.04%	0.004%
45	8.558	2239	2245	2248	rVV4	815	935	0.11%	0.013%
46	8.636	2253	2269	2305	rBV	251303	462767	55.39%	6.321%
47	8.787	2305	2316	2337	rBV2	142011	249259	29.83%	3.405%
48	8.918	2355	2357	2361	rVB2	544	255	0.03%	0.003%
49	8.983	2373	2377	2379	rBV	330	234	0.03%	0.003%
50	9.144	2424	2427	2431	rBV	237	245	0.03%	0.003%
51	9.163	2431	2433	2436	rVV	267	223	0.03%	0.003%
52	9.211	2446	2448	2453	rBB	215	192	0.02%	0.003%
53	9.343	2485	2489	2494	rBB	309	311	0.04%	0.004%
54	9.420	2495	2513	2530	rBV	404946	670003	80.19%	9.152%
55	9.571	2553	2560	2571	rVB2	1126	1851	0.22%	0.025%
56	9.697	2589	2599	2606	rBV3	1716	2671	0.32%	0.036%
57	9.780	2623	2625	2630	rBB	285	227	0.03%	0.003%
58	9.812	2631	2635	2640	rBB	187	199	0.02%	0.003%
59	9.934	2669	2673	2675	rBB	425	275	0.03%	0.004%
60	9.970	2681	2684	2686	rBB	350	221	0.03%	0.003%
61	10.044	2705	2707	2711	rBV2	274	187	0.02%	0.003%
62	10.098	2720	2724	2725	rBV3	657	409	0.05%	0.006%
63	10.214	2755	2760	2763	rBV	239	296	0.04%	0.004%
64	10.298	2783	2786	2789	rVV2	465	311	0.04%	0.004%
65	10.349	2792	2802	2809	rVV5	3588	4693	0.56%	0.064%
66	10.443	2827	2831	2834	rBB	197	194	0.02%	0.003%
67	10.481	2839	2843	2850	rVV2	402	521	0.06%	0.007%
68	10.632	2885	2890	2893	rBB	253	237	0.03%	0.003%
69	10.674	2894	2903	2909	rBV3	969	1398	0.17%	0.019%
70	10.758	2916	2929	2948	rVB	299617	477536	57.16%	6.523%
71	10.844	2952	2956	2958	rBV	198	190	0.02%	0.003%
72	10.896	2962	2972	2982	rBB3	3403	5596	0.67%	0.076%
73	11.082	3026	3030	3033	rBV2	210	191	0.02%	0.003%
74	11.156	3049	3053	3055	rBV	231	224	0.03%	0.003%
75	11.237	3075	3078	3080	rBV	238	205	0.02%	0.003%
76	11.304	3093	3099	3110	rVB5	1812	2704	0.32%	0.037%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048627.D
 Acq On : 19 May 2022 12:17
 Operator : SY/MD
 Sample : N2849-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXXX6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	11.465	3145	3149	3152	rBV3	1090	1074	0.13%	0.015%
78	11.523	3163	3167	3169	rBV2	221	176	0.02%	0.002%
79	11.584	3183	3186	3189	rBV2	471	284	0.03%	0.004%
80	11.690	3213	3219	3229	rBV6	4635	6453	0.77%	0.088%
81	11.748	3233	3237	3245	rVB4	784	773	0.09%	0.011%
82	11.812	3245	3257	3276	rBV	468193	751084	89.90%	10.259%
83	11.934	3292	3295	3300	rBV3	394	415	0.05%	0.006%
84	12.018	3318	3321	3326	rVB	338	223	0.03%	0.003%
85	12.066	3330	3336	3346	rVB5	2537	3967	0.47%	0.054%
86	12.195	3362	3376	3392	rBV	461349	740987	88.69%	10.121%
87	12.561	3481	3490	3496	rBV6	1009	1578	0.19%	0.022%
88	12.844	3575	3578	3584	rVB3	416	336	0.04%	0.005%
89	12.893	3585	3593	3602	rVV4	6460	8707	1.04%	0.119%
90	13.015	3627	3631	3635	rBV	214	199	0.02%	0.003%
91	13.095	3653	3656	3657	rBV	320	195	0.02%	0.003%
92	13.172	3675	3680	3683	rBV	198	192	0.02%	0.003%
93	13.227	3690	3697	3701	rVB2	716	899	0.11%	0.012%
94	13.561	3798	3801	3802	rBV	308	192	0.02%	0.003%
95	13.629	3819	3822	3825	rBV2	320	258	0.03%	0.004%
96	13.844	3886	3889	3891	rBV3	990	785	0.09%	0.011%
97	13.938	3915	3918	3922	rBV2	216	176	0.02%	0.002%
98	14.169	3987	3990	3993	rBV2	360	210	0.03%	0.003%
99	14.262	4016	4019	4021	rBV2	384	235	0.03%	0.003%
100	15.056	4264	4266	4270	rBV	514	258	0.03%	0.004%




Sum of corrected areas: 7321126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048627.D
Acq On : 19 May 2022 12:17
Operator : SY/MD
Sample : N2849-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

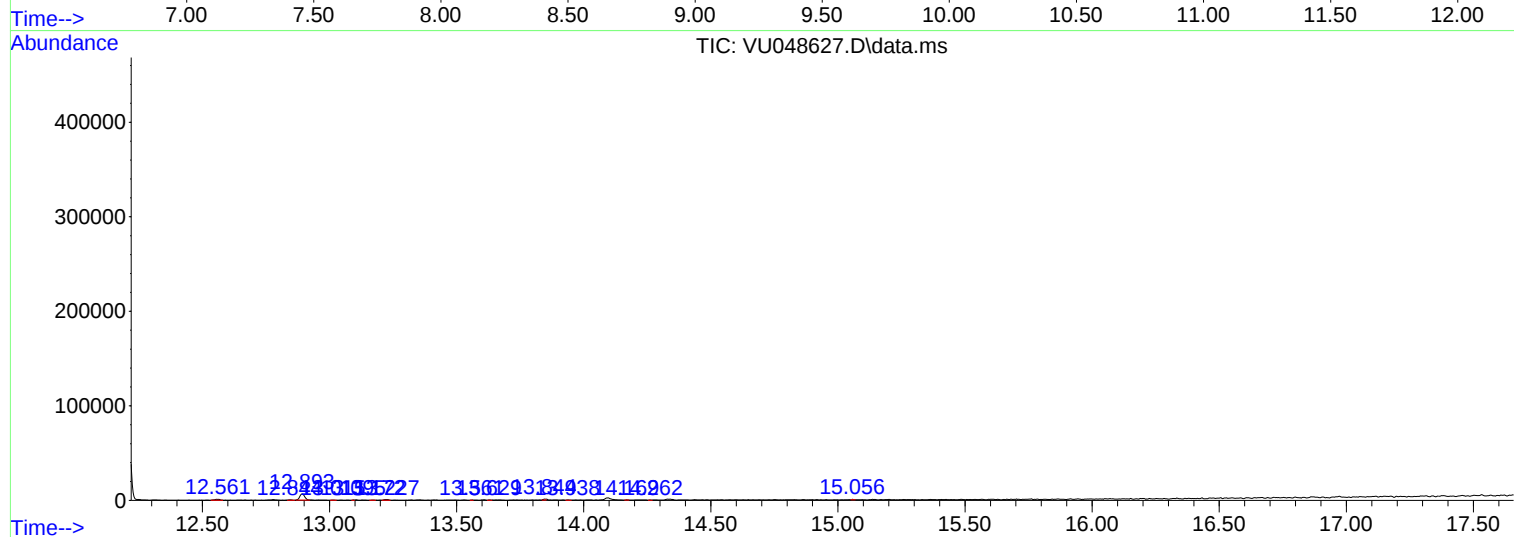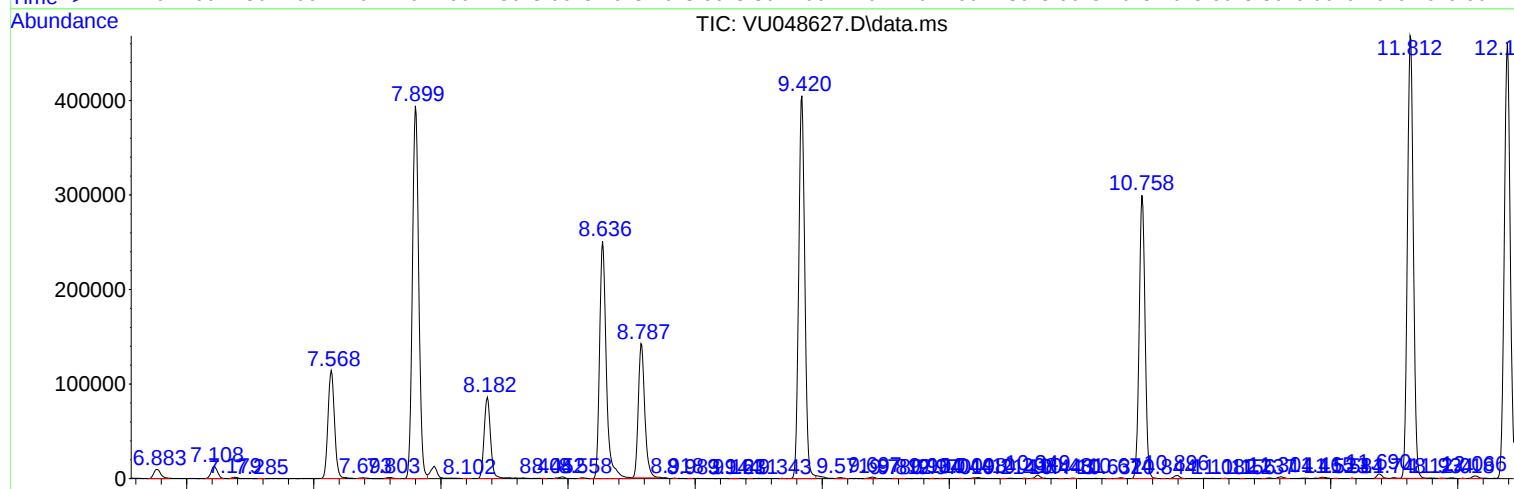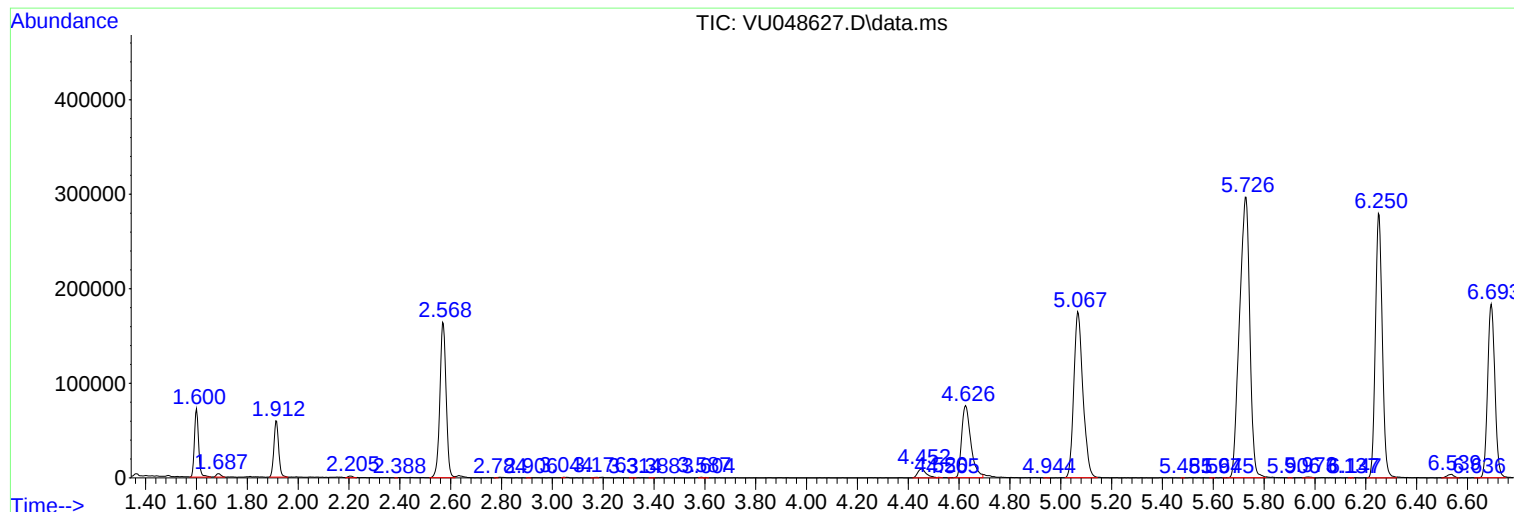

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048627.D
Acq On : 19 May 2022 12:17
Operator : SY/MD
Sample : N2849-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048627.D
Acq On : 19 May 2022 12:17
Operator : SY/MD
Sample : N2849-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXXX6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------