

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048633.D
 Acq On : 19 May 2022 16:30
 Operator : SY/MD
 Sample : N2860-04ME
 Misc : 6.69g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOATOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	86	rBV	56185	71805	7.25%	0.889%
2	1.890	166	171	181	rBV	50698	67527	6.82%	0.836%
3	2.543	362	374	386	rBV	190792	309920	31.29%	3.836%
4	2.668	411	413	417	rVB2	547	301	0.03%	0.004%
5	2.720	421	429	432	rBV3	560	800	0.08%	0.010%
6	2.745	434	437	439	rBV3	399	309	0.03%	0.004%
7	2.826	459	462	464	rBV2	417	283	0.03%	0.004%
8	2.919	488	491	493	rBB2	397	218	0.02%	0.003%
9	3.179	558	572	589	rBV	9504	22955	2.32%	0.284%
10	3.588	696	699	702	rVB	347	220	0.02%	0.003%
11	3.729	737	743	746	rBV	193	243	0.02%	0.003%
12	3.745	746	748	751	rVB	244	154	0.02%	0.002%
13	3.787	758	761	765	rBV	160	180	0.02%	0.002%
14	4.285	913	916	919	rBB	242	162	0.02%	0.002%
15	4.398	948	951	955	rBB2	237	188	0.02%	0.002%
16	4.478	973	976	980	rVB	413	227	0.02%	0.003%
17	4.636	1011	1025	1061	rBV	71160	249781	25.22%	3.091%
18	5.060	1139	1157	1182	rBV	184736	420126	42.42%	5.199%
19	5.285	1225	1227	1230	rBV	358	278	0.03%	0.003%
20	5.347	1236	1246	1247	rBV2	841	944	0.10%	0.012%
21	5.420	1266	1269	1274	rVB2	266	218	0.02%	0.003%
22	5.498	1290	1293	1296	rBB	242	165	0.02%	0.002%
23	5.720	1340	1362	1386	rBV2	375719	990332	100.00%	12.256%
24	5.967	1436	1439	1447	rBV3	601	804	0.08%	0.010%
25	6.080	1471	1474	1478	rBB	179	185	0.02%	0.002%
26	6.125	1483	1488	1490	rBB2	370	243	0.02%	0.003%
27	6.247	1510	1526	1547	rVV	261211	503785	50.87%	6.235%
28	6.408	1575	1576	1582	rBB	208	170	0.02%	0.002%
29	6.437	1582	1585	1590	rBB	321	313	0.03%	0.004%
30	6.462	1590	1593	1594	rBV	232	149	0.02%	0.002%
31	6.527	1604	1613	1623	rVB5	5024	8868	0.90%	0.110%
32	6.581	1627	1630	1631	rBV	274	148	0.01%	0.002%
33	6.601	1631	1636	1638	rVV2	383	315	0.03%	0.004%
34	6.610	1638	1639	1642	rVB	629	274	0.03%	0.003%
35	6.691	1649	1664	1687	rBV	215330	433859	43.81%	5.369%
36	6.806	1696	1700	1704	rBV3	630	594	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048633.D
 Acq On : 19 May 2022 16:30
 Operator : SY/MD
 Sample : N2860-04ME
 Misc : 6.69g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOATOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.858	1712	1716	1718	rVB	264	168	0.02%	0.002%
38	7.115	1792	1796	1797	rBV	221	154	0.02%	0.002%
39	7.202	1810	1823	1834	rBV4	5104	13103	1.32%	0.162%
40	7.305	1852	1855	1858	rVB2	332	279	0.03%	0.003%
41	7.334	1859	1864	1865	rBV	284	230	0.02%	0.003%
42	7.382	1875	1879	1880	rBV	240	179	0.02%	0.002%
43	7.443	1894	1898	1904	rBB2	393	410	0.04%	0.005%
44	7.565	1924	1936	1958	rBV3	124289	240349	24.27%	2.975%
45	7.691	1972	1975	1982	rVB5	773	808	0.08%	0.010%
46	7.790	1997	2006	2016	rBV4	4849	8564	0.86%	0.106%
47	7.896	2026	2039	2057	rBV	448451	795371	80.31%	9.843%
48	8.044	2083	2085	2094	rVB2	345	336	0.03%	0.004%
49	8.086	2094	2098	2101	rVB2	489	377	0.04%	0.005%
50	8.108	2102	2105	2108	rBB2	315	189	0.02%	0.002%
51	8.182	2116	2128	2153	rVB2	85887	171808	17.35%	2.126%
52	8.272	2153	2156	2159	rVB3	439	229	0.02%	0.003%
53	8.292	2160	2162	2166	rBV2	317	276	0.03%	0.003%
54	8.362	2181	2184	2189	rVB2	349	306	0.03%	0.004%
55	8.440	2204	2208	2210	rBV2	398	310	0.03%	0.004%
56	8.478	2212	2220	2231	rVB3	4255	7444	0.75%	0.092%
57	8.658	2258	2276	2303	rBV	264203	579866	58.55%	7.176%
58	8.825	2326	2328	2333	rVB	371	283	0.03%	0.004%
59	8.864	2336	2340	2341	rBV	275	232	0.02%	0.003%
60	8.938	2352	2363	2368	rBV3	1273	2706	0.27%	0.033%
61	9.141	2422	2426	2430	rBV	265	271	0.03%	0.003%
62	9.170	2430	2435	2437	rVV	287	210	0.02%	0.003%
63	9.256	2457	2462	2465	rBV2	229	266	0.03%	0.003%
64	9.420	2498	2513	2533	rBV	335831	637510	64.37%	7.890%
65	9.571	2557	2560	2563	rBV	391	330	0.03%	0.004%
66	9.604	2568	2570	2575	rBV2	437	310	0.03%	0.004%
67	9.658	2586	2587	2590	rBV	271	157	0.02%	0.002%
68	9.803	2630	2632	2636	rBV	175	164	0.02%	0.002%
69	9.957	2677	2680	2682	rBV	289	212	0.02%	0.003%
70	10.118	2726	2730	2734	rBV2	336	335	0.03%	0.004%
71	10.163	2740	2744	2745	rBV	280	206	0.02%	0.003%
72	10.218	2758	2761	2767	rVB	453	363	0.04%	0.004%
73	10.260	2768	2774	2776	rBV	228	311	0.03%	0.004%
74	10.623	2884	2887	2888	rBV	230	150	0.02%	0.002%
75	10.633	2888	2890	2893	rVV	262	179	0.02%	0.002%
76	10.764	2918	2931	2949	rBV	364959	596224	60.20%	7.379%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048633.D
 Acq On : 19 May 2022 16:30
 Operator : SY/MD
 Sample : N2860-04ME
 Misc : 6.69g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOATOME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M

Title : VOC Analysis

77	10.893	2958	2971	2992	rVB	160828	268552	27.12%	3.324%
78	11.096	3029	3034	3035	rBV	292	177	0.02%	0.002%
79	11.256	3081	3084	3087	rBB	211	153	0.02%	0.002%
80	11.276	3087	3090	3093	rBV2	326	261	0.03%	0.003%
81	11.305	3097	3099	3106	rVB	356	315	0.03%	0.004%
82	11.356	3109	3115	3117	rBV2	208	217	0.02%	0.003%
83	11.456	3140	3146	3160	rVB6	2298	4021	0.41%	0.050%
84	11.748	3233	3237	3246	rBV2	714	653	0.07%	0.008%
85	11.816	3246	3258	3275	rBV	453213	722635	72.97%	8.943%
86	11.967	3304	3305	3308	rBV2	597	336	0.03%	0.004%
87	12.070	3334	3337	3340	rBV	200	160	0.02%	0.002%
88	12.195	3361	3376	3398	rVV	548482	878712	88.73%	10.875%
89	12.314	3410	3413	3417	rVB	282	185	0.02%	0.002%
90	12.472	3459	3462	3466	rBB2	305	210	0.02%	0.003%
91	12.774	3545	3556	3566	rBV	28016	43996	4.44%	0.544%
92	13.169	3676	3679	3683	rBB3	466	314	0.03%	0.004%
93	13.275	3710	3712	3719	rVB	334	242	0.02%	0.003%
94	13.475	3772	3774	3777	rBV	237	151	0.02%	0.002%
95	13.636	3821	3824	3826	rBV	403	270	0.03%	0.003%
96	13.848	3885	3890	3895	rBV3	765	997	0.10%	0.012%
97	13.928	3912	3915	3918	rBV	409	290	0.03%	0.004%
98	14.076	3959	3961	3963	rBV2	449	203	0.02%	0.003%
99	14.578	4110	4117	4128	rVB2	5595	8858	0.89%	0.110%
100	14.655	4139	4141	4144	rBV	382	159	0.02%	0.002%




Sum of corrected areas: 8080285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048633.D
Acq On : 19 May 2022 16:30
Operator : SY/MD
Sample : N2860-04ME
Misc : 6.69g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
HOATOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

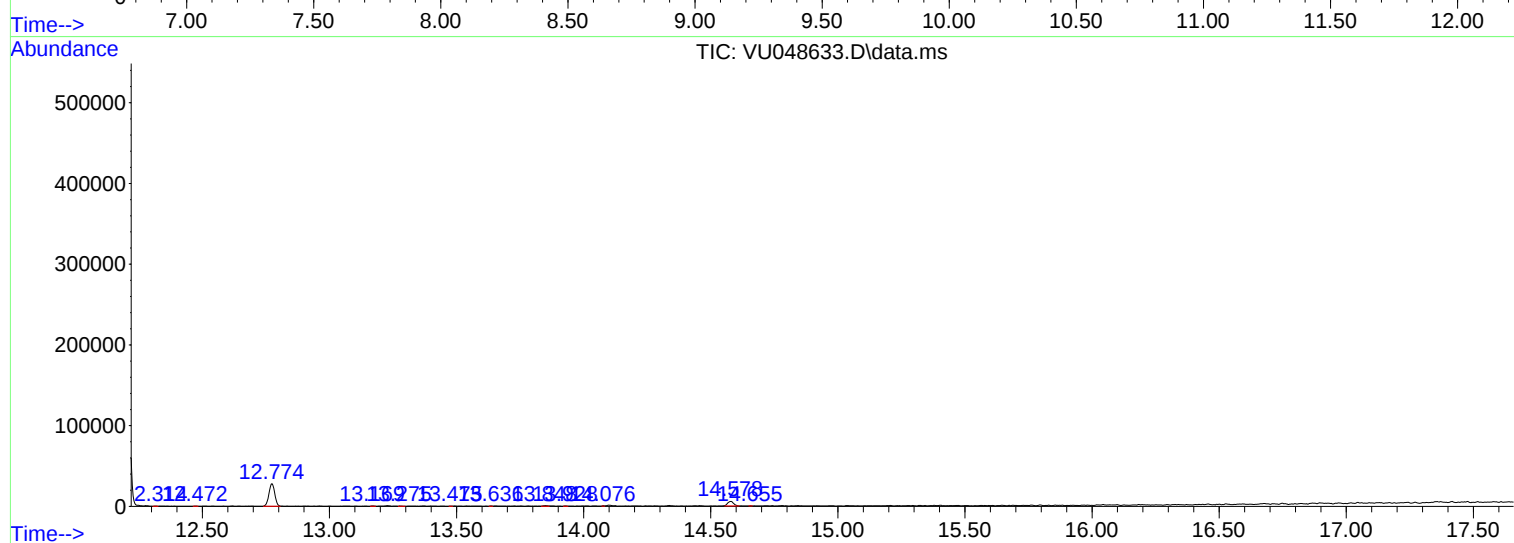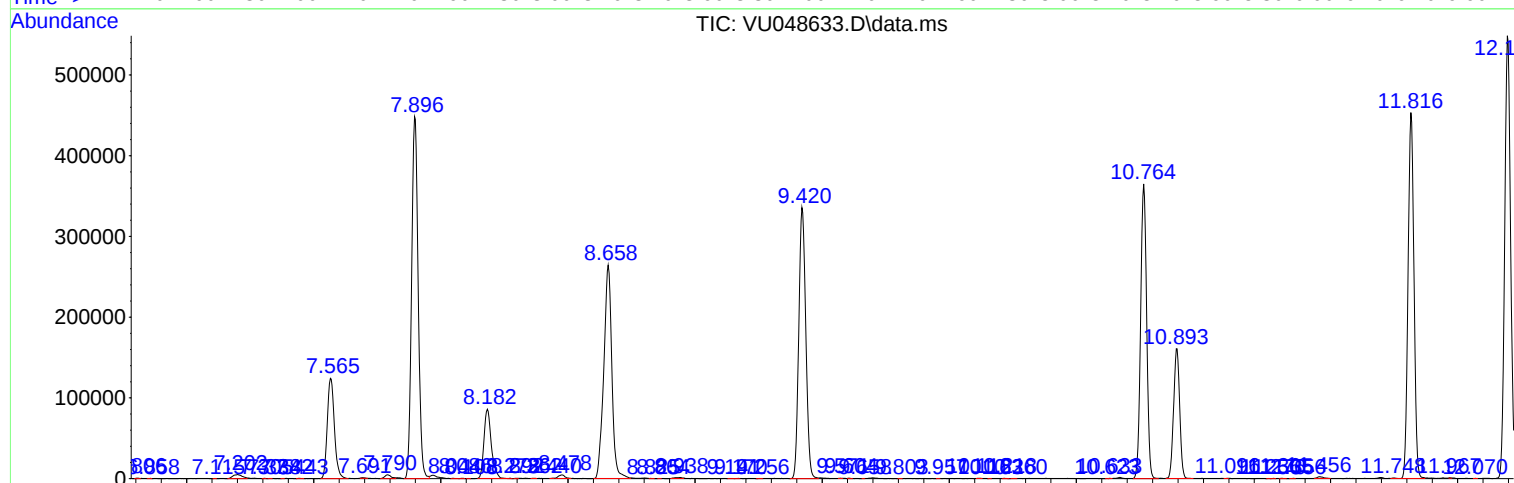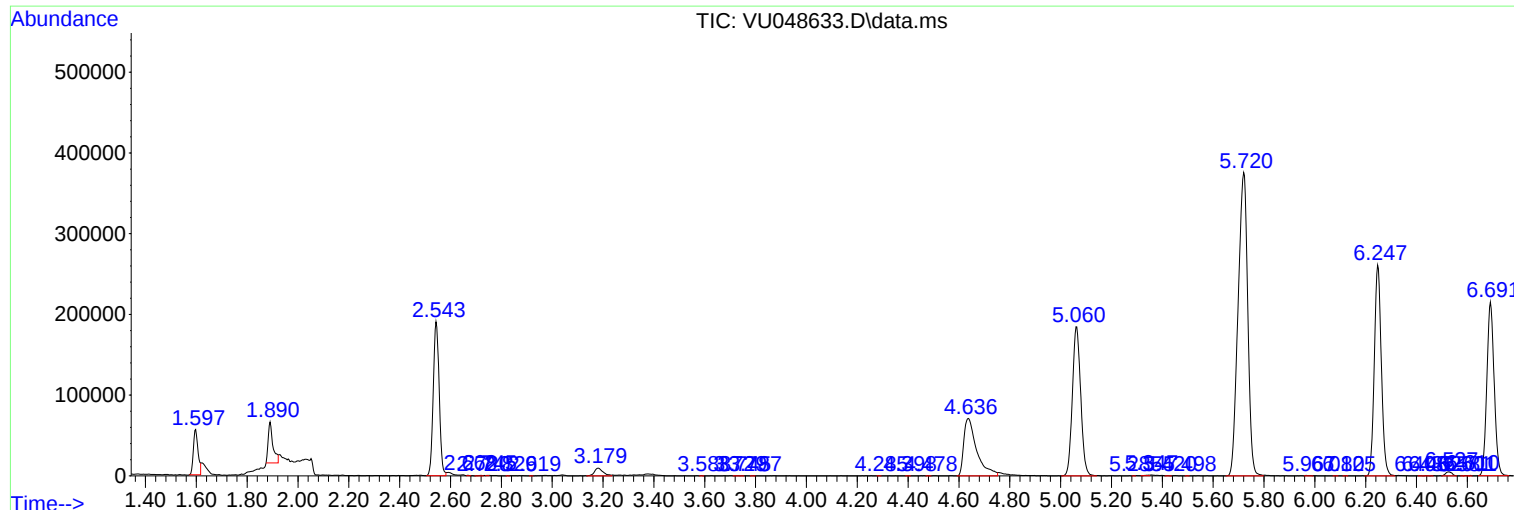

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048633.D
Acq On : 19 May 2022 16:30
Operator : SY/MD
Sample : N2860-04ME
Misc : 6.69g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0ATOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
Data File : VU048633.D
Acq On : 19 May 2022 16:30
Operator : SY/MD
Sample : N2860-04ME
Misc : 6.69g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0ATOME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc