


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051922\
 Data File : VU048622.D
 Acq On : 19 May 2022 09:13
 Operator : SY/MD
 Sample : BFB090
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB090

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis
 Last Update : Tue May 24 02:53:22 2022

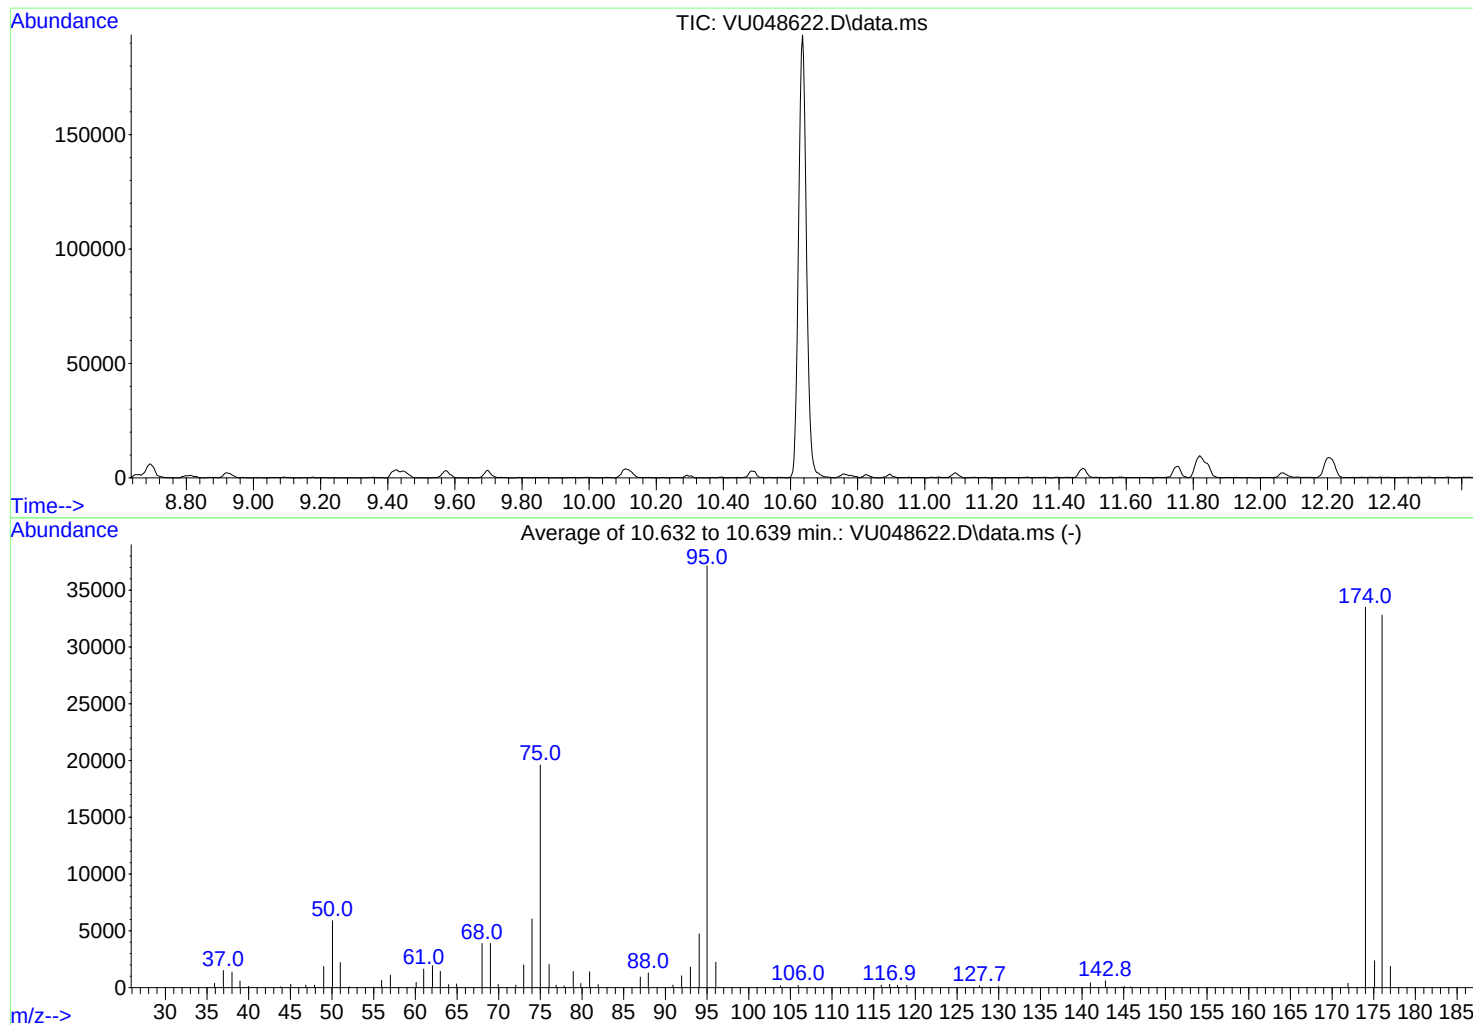

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	5886	PASS
75	95	30	80	52.8	19619	PASS
95	95	100	100	100.0	37144	PASS
96	95	5	9	6.0	2236	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.2	33491	PASS
175	174	5	9	7.1	2375	PASS
176	174	95	101	98.0	32805	PASS
177	176	5	9	5.7	1880	PASS

m/z	Abundance
43.90	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	372.0
37.00	1544.0
38.00	1465.0
38.90	550.0
43.80	256.0
45.00	286.0
46.90	247.0
47.90	221.0
49.00	1870.0
50.00	5911.0
51.00	2135.0
52.10	111.0
55.90	677.0
57.00	978.0
57.80	101.0
60.10	505.0
61.00	1667.0
62.00	1938.0
63.00	1440.0
64.00	259.0
64.90	343.0
68.00	3990.0
69.00	3963.0
69.90	332.0
72.20	205.0
73.00	1892.0
74.00	6002.0
75.00	19480.0
76.10	1874.0
76.90	215.0
77.90	134.0
79.00	1350.0
79.90	368.0
80.90	1428.0
81.90	265.0
87.00	836.0
88.00	1095.0
90.90	231.0
92.00	1120.0
93.00	1735.0
94.00	4831.0
95.00	37184.0
96.00	2273.0
103.80	118.0
106.00	234.0
115.90	182.0
116.80	257.0
117.80	186.0
119.00	224.0
127.70	135.0
128.90	107.0
129.90	199.0
141.00	468.0
142.80	619.0
144.80	182.0
171.90	462.0
174.00	32720.0
175.10	2312.0
176.00	32280.0
177.00	1943.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	387.0
37.00	1552.0
38.00	1398.0
39.00	548.0
40.00	155.0
43.80	225.0
45.10	317.0
46.80	233.0
47.90	237.0
49.00	1961.0
50.10	5993.0
51.00	2348.0
52.10	102.0
55.90	650.0
57.00	1147.0
60.10	480.0
61.00	1661.0
62.00	1967.0
63.00	1467.0
64.00	280.0
65.00	303.0
68.00	4046.0
69.00	3954.0
70.00	289.0
72.00	229.0
73.00	2084.0
74.00	6119.0
75.00	20160.0
76.00	2061.0
76.90	231.0
77.90	157.0
78.90	1480.0
79.90	379.0
80.90	1449.0
82.00	271.0
87.00	936.0
87.90	1321.0
90.90	239.0
92.00	1075.0
93.00	1854.0
94.10	4888.0
95.00	38304.0
96.10	2282.0
103.80	178.0
105.90	202.0
115.90	244.0
116.90	286.0
117.90	234.0
119.00	228.0
127.70	183.0
130.00	146.0
141.00	418.0
142.80	613.0
145.10	155.0
145.80	102.0
171.90	406.0
174.00	34472.0
175.10	2438.0
176.00	34080.0
177.00	1946.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090

m/z	Abundance
35.90	362.0
36.90	1413.0
38.00	1237.0
39.00	620.0
40.00	198.0
43.90	222.0
45.00	291.0
46.90	195.0
47.90	225.0
49.00	1742.0
50.00	5754.0
51.00	2141.0
55.00	117.0
56.00	573.0
57.00	1179.0
60.10	399.0
61.00	1570.0
62.10	1881.0
63.00	1407.0
64.00	264.0
65.00	315.0
68.00	3615.0
69.00	3773.0
70.00	209.0
72.00	231.0
73.00	2013.0
74.00	5992.0
75.00	19216.0
76.00	2184.0
76.90	247.0
77.80	172.0
78.90	1456.0
79.80	342.0
80.90	1301.0
82.00	277.0
87.00	1040.0
87.90	1475.0
90.90	228.0
91.90	945.0
93.00	1840.0
94.00	4486.0
95.00	35944.0
96.10	2152.0
103.80	214.0
105.90	161.0
115.90	270.0
117.00	296.0
117.80	215.0
118.90	192.0
127.70	202.0
141.00	368.0
142.80	574.0
145.10	138.0
145.80	112.0
172.00	275.0
174.00	33280.0
175.10	2376.0
176.00	32056.0
177.00	1751.0

Instrument :
MSVOA_U
ClientSampleId :
BFB090