

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
 Data File : VU054224.D
 Acq On : 19 May 2023 17:05
 Operator : JC/MD
 Sample : 02843-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBWX7

Quant Time: May 20 02:10:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 20 02:06:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	189510	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	179928	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	84836	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	43805	4.287	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.800%
7) Chloroethane-d5	1.912	69	34492	4.513	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.562	65	20010	4.336	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.800%
20) 2-Butanone-d5	4.632	46	89394	49.062	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.120%
24) Chloroform-d	5.057	84	84120	4.379	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.697	65	40105	4.538	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
32) Benzene-d6	5.722	84	166814	4.553	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
36) 1,2-Dichloropropane-d6	6.687	67	51851	4.896	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.000%
41) Toluene-d8	7.893	98	144651	4.181	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
43) trans-1,3-Dichloroprop...	8.176	79	18477	4.319	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.400%
46) 2-Hexanone-d5	8.629	63	63276	49.681	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.360%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	37563	4.948	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.000%
66) 1,2-Dichlorobenzene-d4	12.188	152	55525	5.364	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.200%
Target Compounds					Qvalue	
13) Acetone	2.645	43	14860	5.995	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
Data File : VU054224.D
Acq On : 19 May 2023 17:05
Operator : JC/MD
Sample : 02843-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBWX7

Quant Time: May 20 02:10:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 20 02:06:23 2023
Response via : Initial Calibration

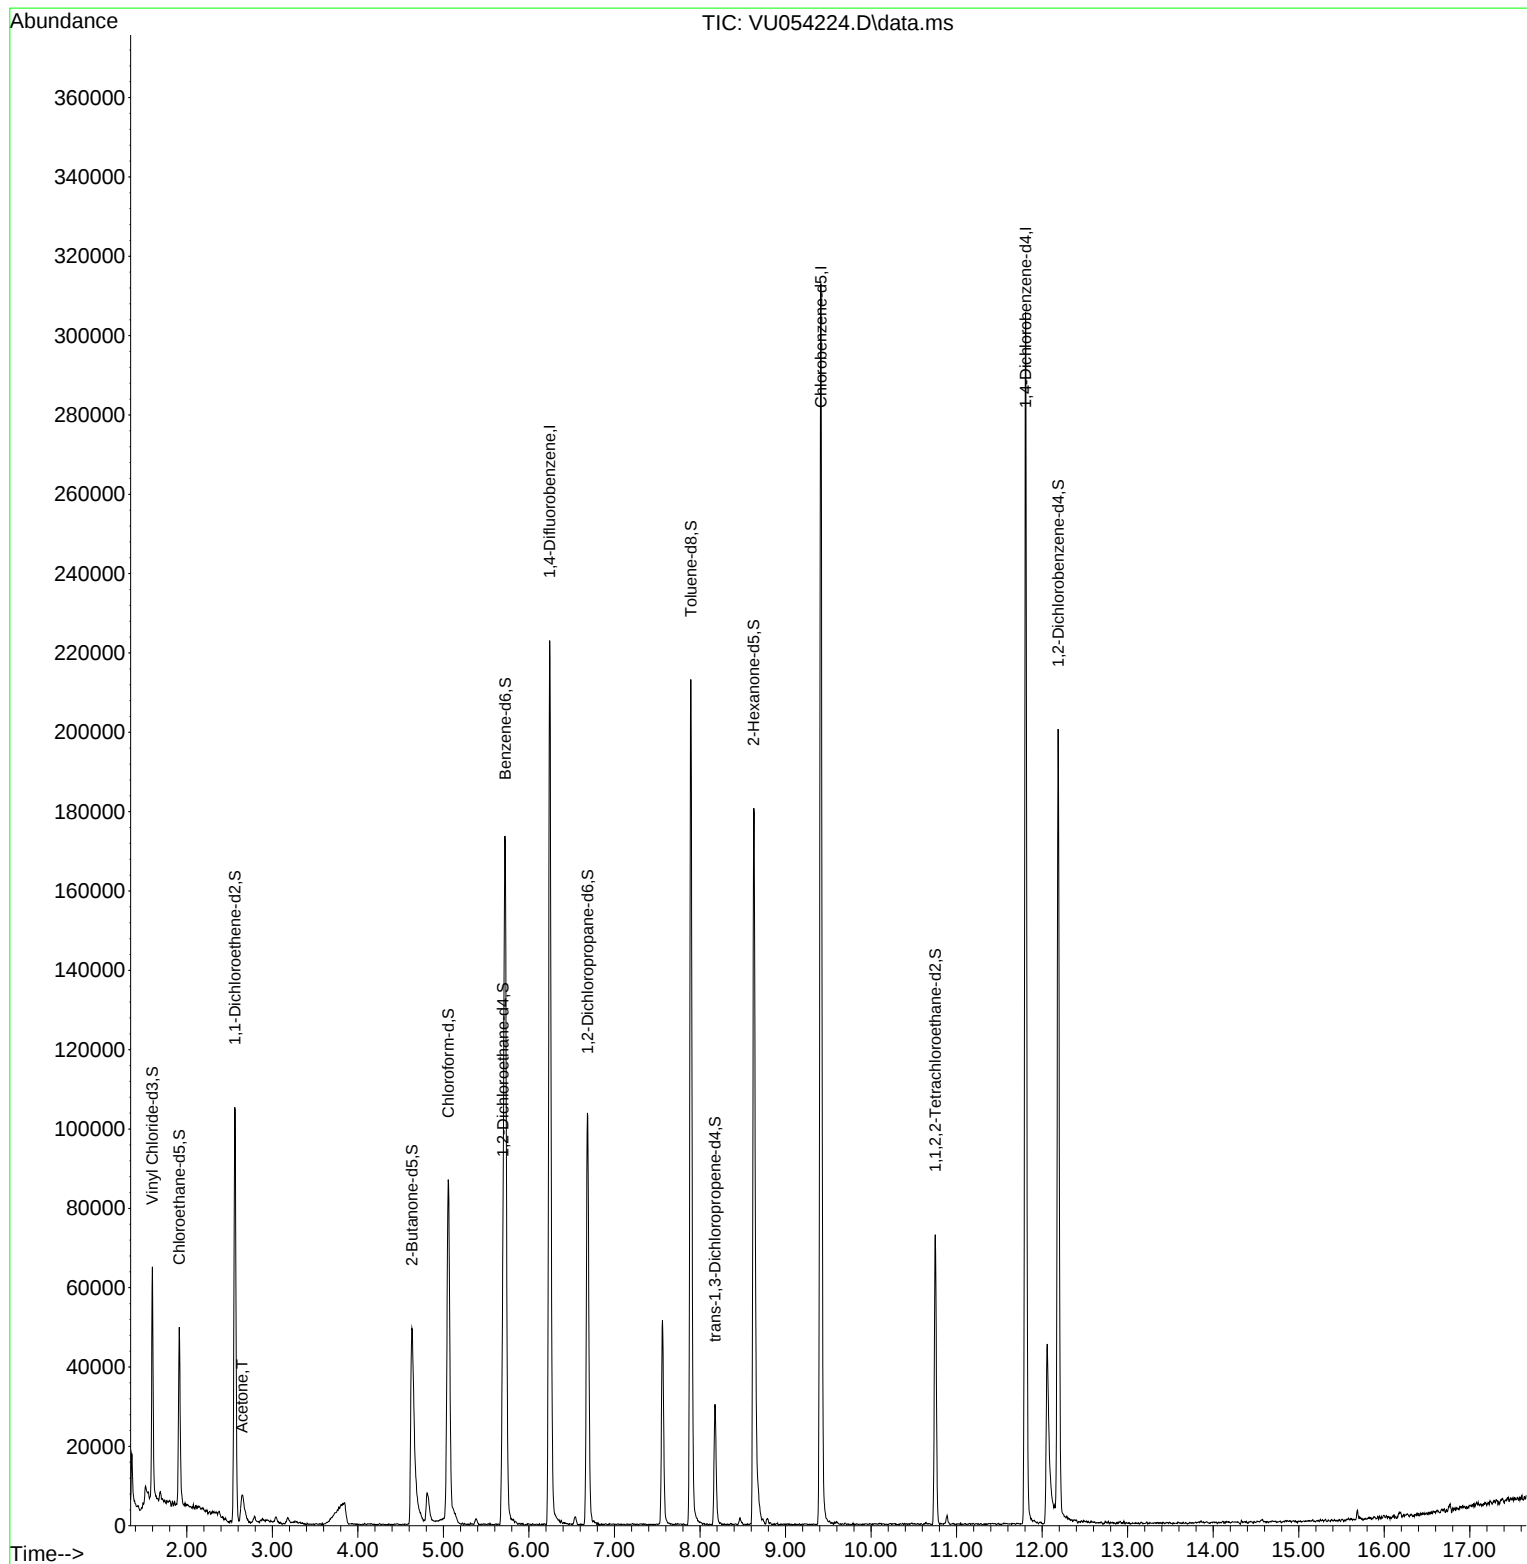

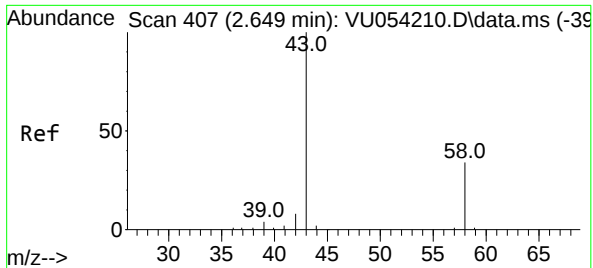

#13
 Acetone
 Concen: 5.995 ug/L
 RT: 2.645 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: VU054224.D
 Acq: 19 May 2023 17:05

Instrument :
 MSVOA_U
 ClientSampleId :
 GBWX7

Tgt Ion: 43 Resp: 14860
 Ion Ratio Lower Upper
 43 100
 58 33.9 0.0 73.2

