

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
 Data File : VU054225.D
 Acq On : 19 May 2023 17:29
 Operator : JC/MD
 Sample : 02843-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBWX8

Quant Time: May 20 02:10:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 20 02:06:23 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	182033	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	175441	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	83912	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	43764	4.459	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.200%
7) Chloroethane-d5	1.912	69	33468	4.559	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	2.562	65	20096	4.534	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.600%
20) 2-Butanone-d5	4.629	46	85390	48.790	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.580%
24) Chloroform-d	5.057	84	81034	4.392	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.800%
26) 1,2-Dichloroethane-d4	5.697	65	38764	4.567	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
32) Benzene-d6	5.722	84	162720	4.554	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.000%
36) 1,2-Dichloropropane-d6	6.684	67	50369	4.878	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.893	98	139392	4.132	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	8.176	79	18203	4.364	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.200%
46) 2-Hexanone-d5	8.629	63	60885	49.026	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.060%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	34974	4.725	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.400%
66) 1,2-Dichlorobenzene-d4	12.188	152	52519	5.129	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds					Qvalue	
13) Acetone	2.645	43	19507	8.193	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
Data File : VU054225.D
Acq On : 19 May 2023 17:29
Operator : JC/MD
Sample : 02843-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBWX8

Quant Time: May 20 02:10:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 20 02:06:23 2023
Response via : Initial Calibration

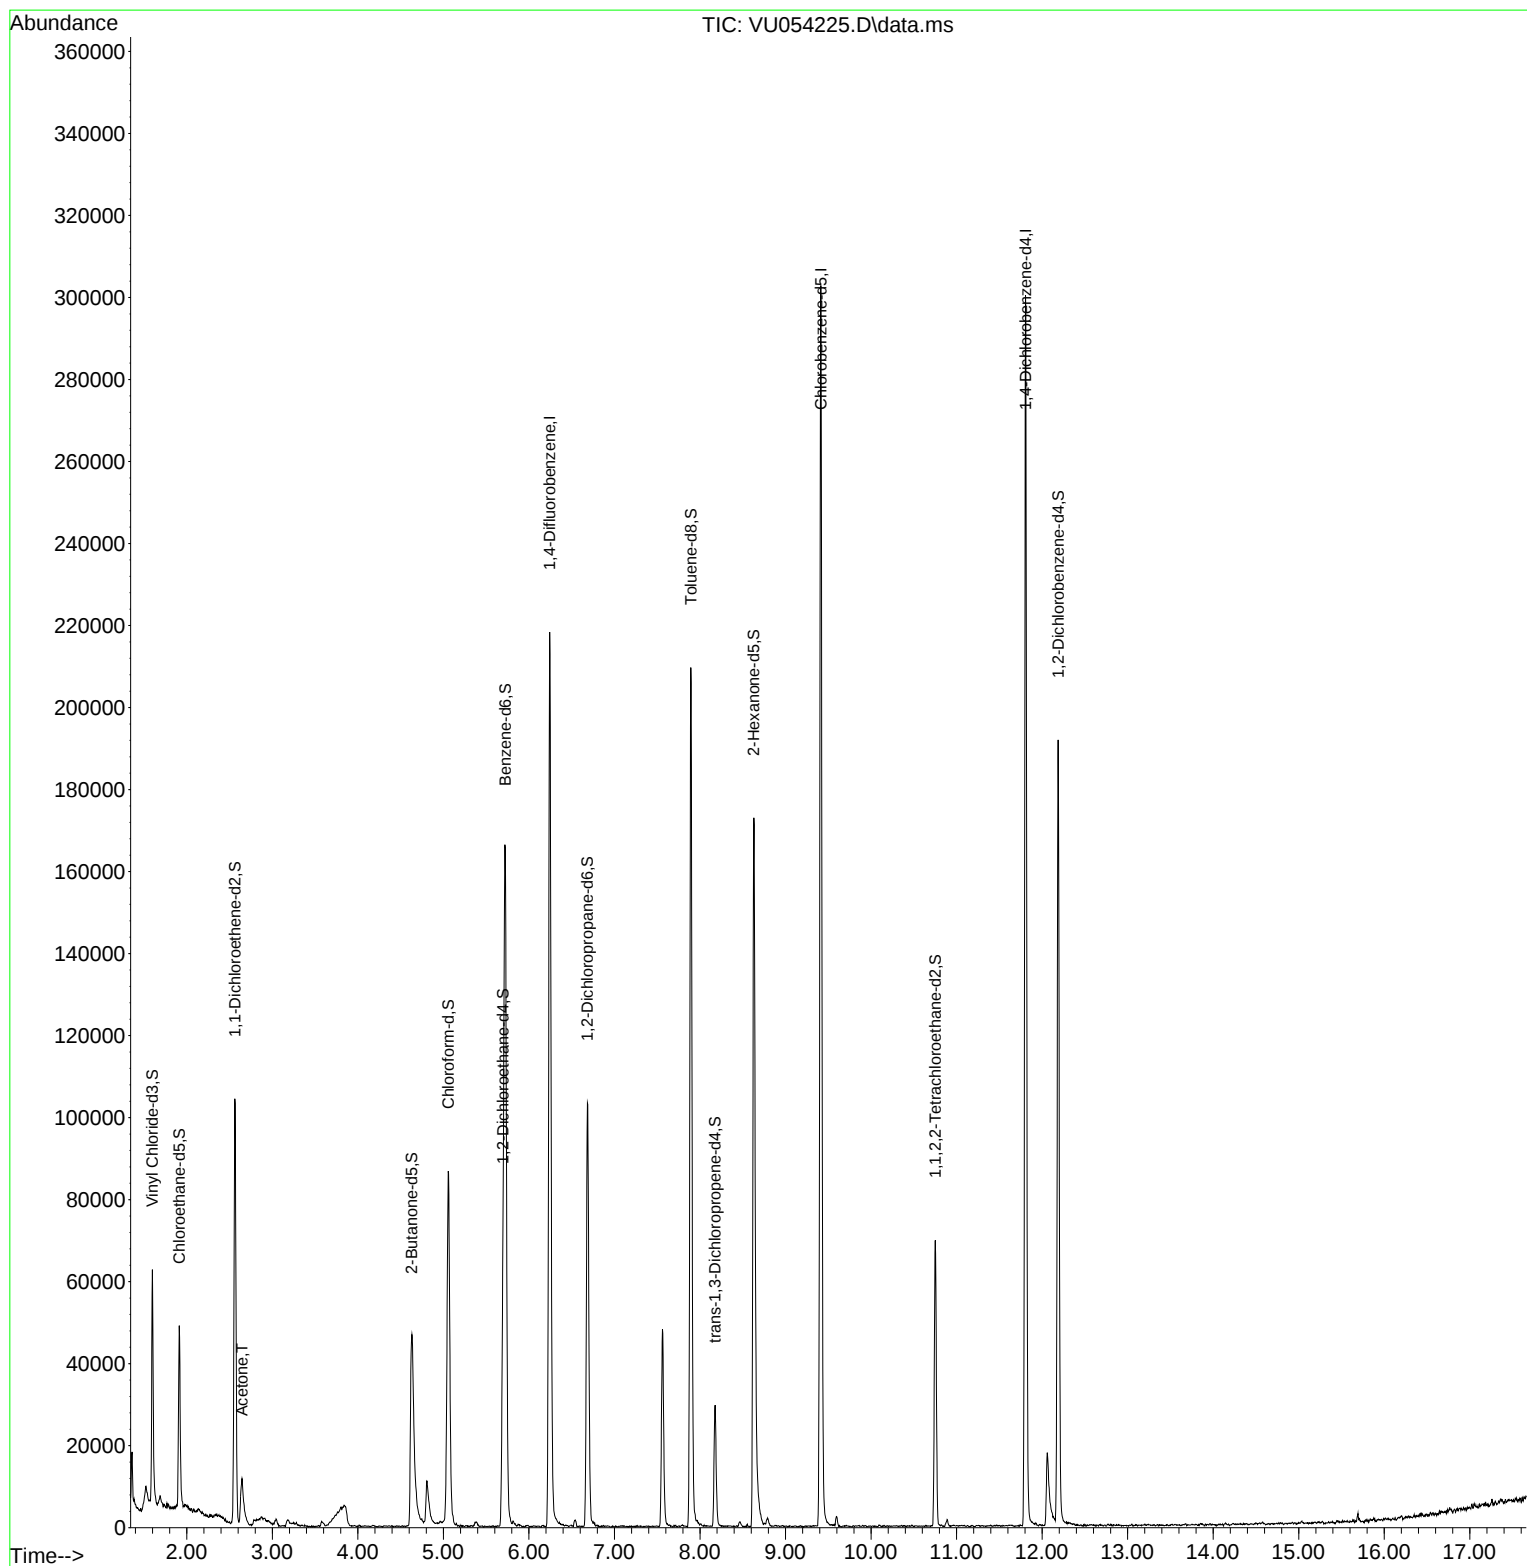

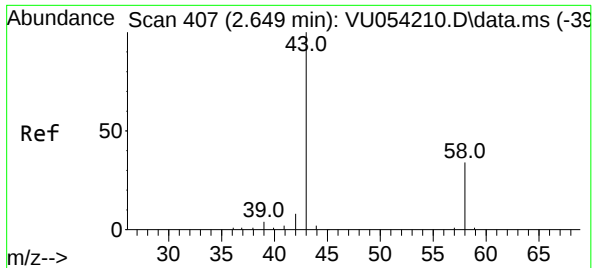

#13
 Acetone
 Concen: 8.193 ug/L
 RT: 2.645 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: VU054225.D
 Acq: 19 May 2023 17:29

Instrument :
 MSVOA_U
 ClientSampleId :
 GBWX8

Tgt Ion: 43 Resp: 19507
 Ion Ratio Lower Upper
 43 100
 58 35.7 0.0 73.2

