

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
 Data File : VU054217.D
 Acq On : 19 May 2023 14:16
 Operator : JC/MD
 Sample : 02844-07DL 4X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBX01DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	13	rVB2	12888	11795	2.04%	0.266%
2	1.597	72	80	92	rBV	53925	64617	11.15%	1.459%
3	1.912	170	178	194	rVB	42046	57418	9.91%	1.296%
4	2.562	367	380	396	rVB	99811	163421	28.20%	3.689%
5	2.646	396	406	423	rBV2	2903	6746	1.16%	0.152%
6	3.041	520	529	543	rVB3	4665	8911	1.54%	0.201%
7	4.633	1011	1024	1050	rBV	46172	137265	23.69%	3.099%
8	4.809	1069	1079	1097	rBV3	10582	24858	4.29%	0.561%
9	5.057	1139	1156	1185	rVB	80978	188321	32.50%	4.252%
10	5.719	1343	1362	1387	rBV2	163664	415577	71.71%	9.382%
11	6.243	1512	1525	1549	rBV	207380	401043	69.20%	9.054%
12	6.536	1602	1616	1648	rBV	302458	579524	100.00%	13.083%
13	6.684	1650	1662	1685	rVB2	96025	192968	33.30%	4.356%
14	7.562	1923	1935	1951	rBV	47720	84550	14.59%	1.909%
15	7.893	2025	2038	2059	rBV	200789	352753	60.87%	7.964%
16	8.176	2114	2126	2142	rBV2	29381	49260	8.50%	1.112%
17	8.629	2254	2267	2306	rBV2	169559	333962	57.63%	7.540%
18	9.411	2497	2510	2542	rBV	282076	479293	82.70%	10.821%
19	10.751	2913	2927	2940	rBV2	68410	110504	19.07%	2.495%
20	11.806	3244	3255	3275	rBV	292519	471547	81.37%	10.646%
21	12.189	3359	3374	3393	rBV	179173	295152	50.93%	6.663%




Sum of corrected areas: 4429485

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
Data File : VU054217.D
Acq On : 19 May 2023 14:16
Operator : JC/MD
Sample : 02844-07DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBX01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

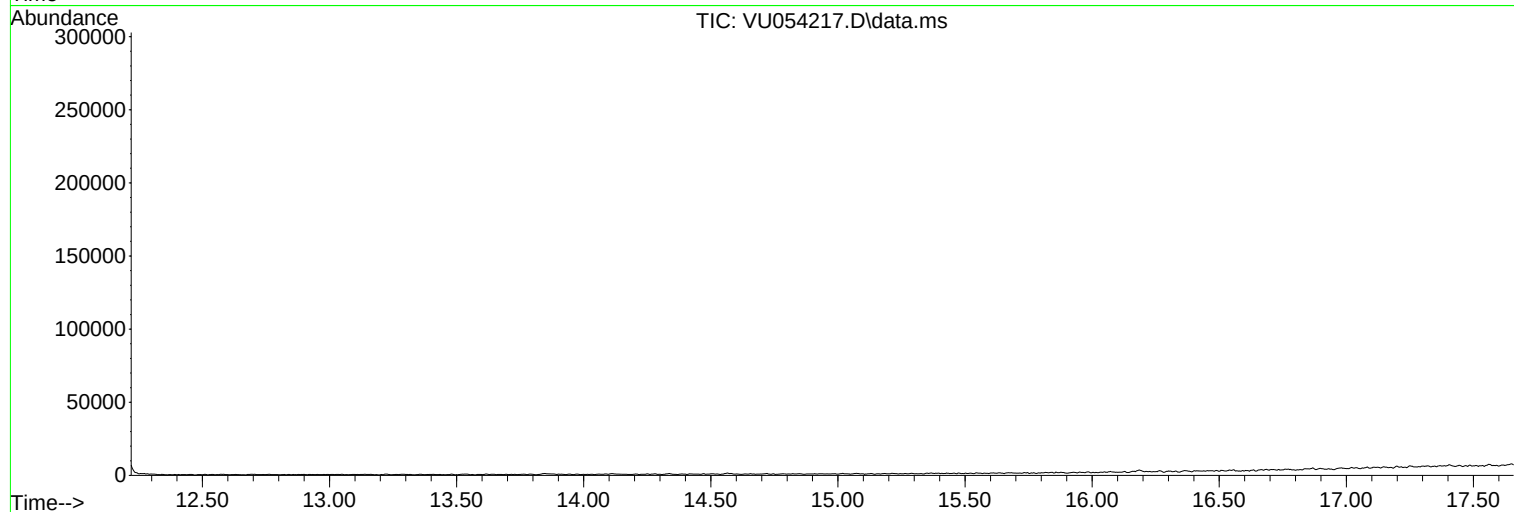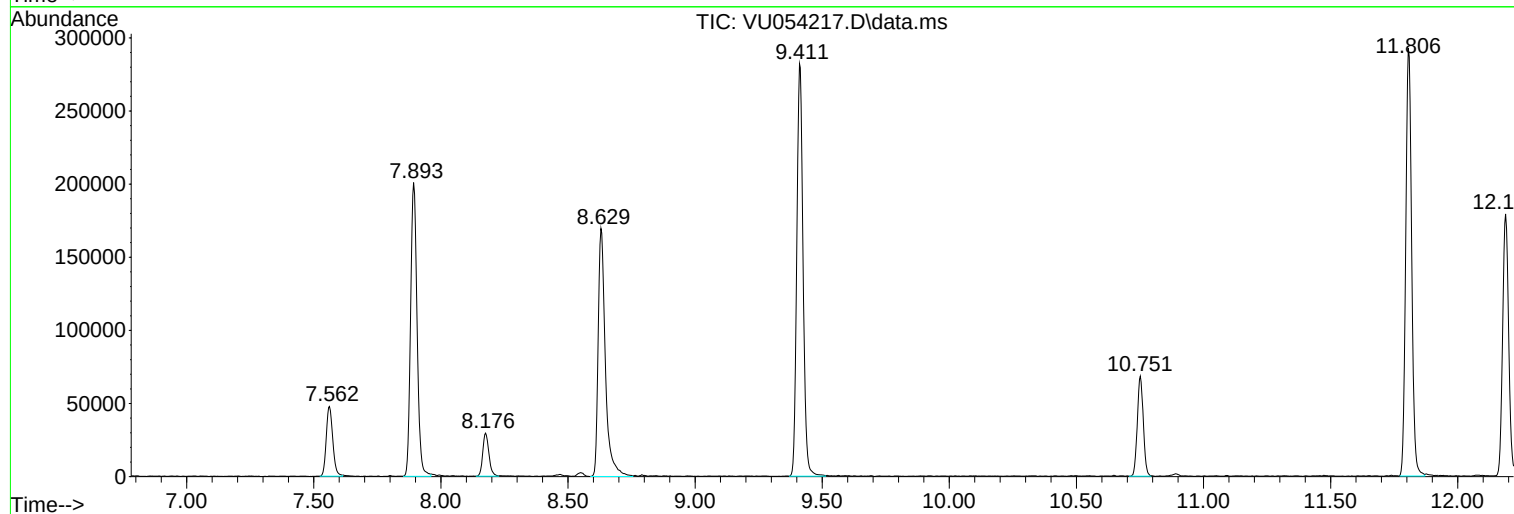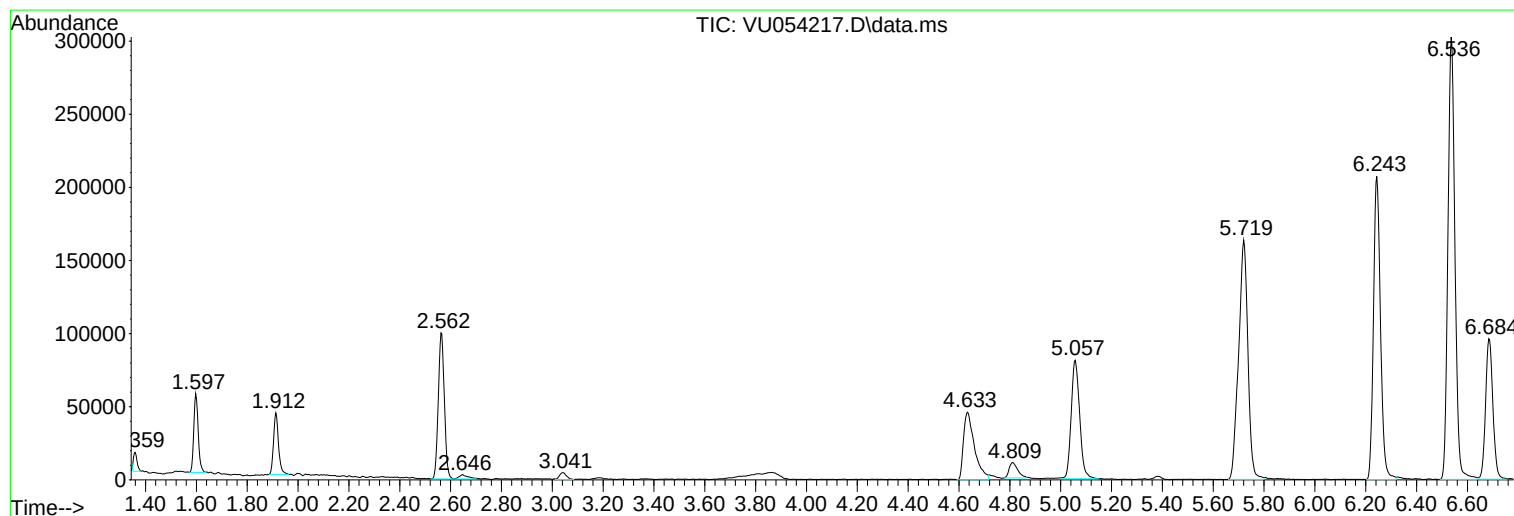

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
Data File : VU054217.D
Acq On : 19 May 2023 14:16
Operator : JC/MD
Sample : 02844-07DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBX01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
Data File : VU054217.D
Acq On : 19 May 2023 14:16
Operator : JC/MD
Sample : 02844-07DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBX01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc