
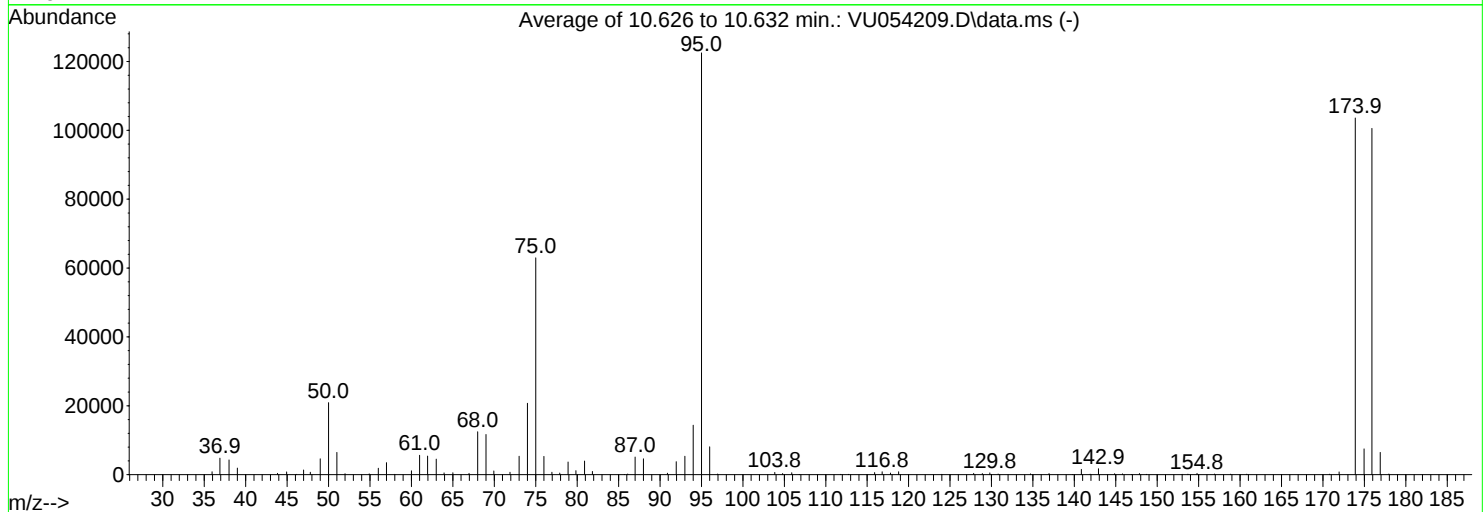


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051923\
Data File : VU054209.D
Acq On : 19 May 2023 10:26
Operator : JC/MD
Sample : BFB012
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB012

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat May 20 02:06:23 2023

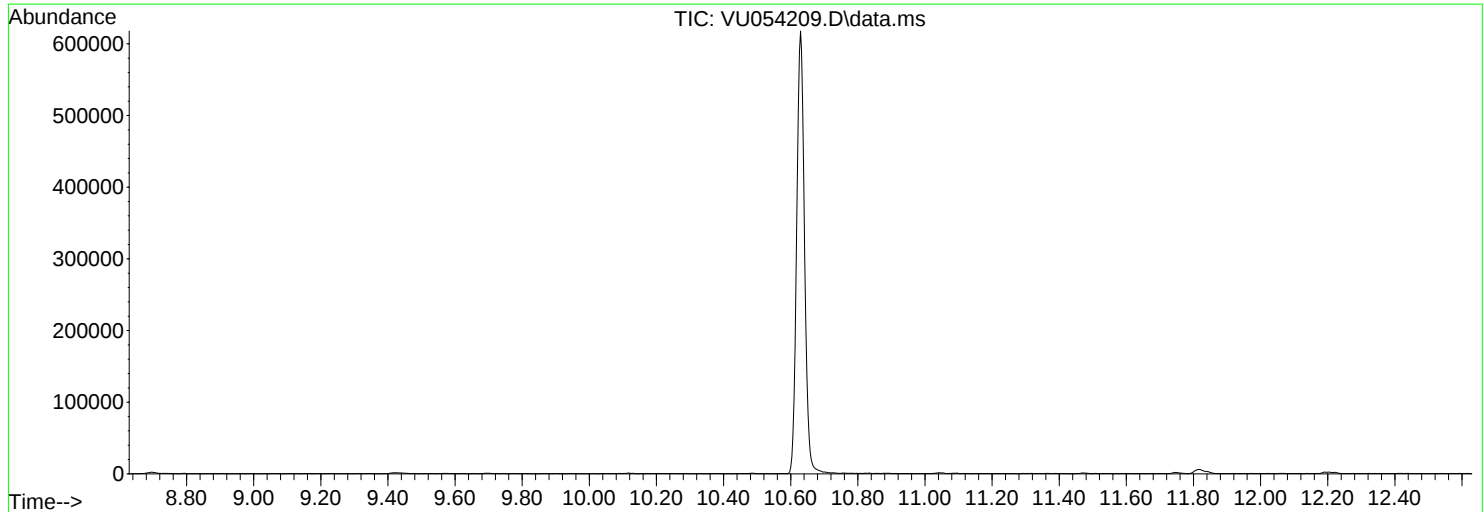

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	20933	PASS
75	95	30	80	51.4	62965	PASS
95	95	100	100	100.0	122501	PASS
96	95	5	9	6.6	8085	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.6	103595	PASS
175	174	5	9	7.2	7469	PASS
176	174	95	101	97.1	100549	PASS
177	176	5	9	6.4	6460	PASS

m/z	Abundance
39.80	167.0
43.80	347.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	879.0
36.90	4708.0
38.00	4273.0
39.00	1845.0
39.90	172.0
43.90	747.0
44.90	849.0
46.10	128.0
47.00	1180.0
47.80	671.0
49.00	4568.0
50.00	21112.0
51.00	6442.0
52.10	310.0
54.90	236.0
56.00	1749.0
57.00	3494.0
60.00	1015.0
61.00	5697.0
62.00	5476.0
63.00	4617.0
63.90	458.0
65.00	581.0
66.90	327.0
68.00	12419.0
69.00	11467.0
69.90	1045.0
71.90	868.0
73.00	5325.0
74.00	20872.0
75.00	62584.0
76.00	5578.0
76.90	746.0
77.90	490.0
78.90	3693.0
79.90	1083.0
80.90	3809.0
81.90	908.0
85.70	116.0
86.10	138.0
87.00	4951.0
88.00	4560.0
90.80	383.0
92.00	3608.0
93.00	5114.0
94.00	14153.0
95.00	120648.0
96.00	8221.0
96.90	208.0
103.90	605.0
104.80	331.0
105.90	516.0
112.70	136.0
115.90	559.0
116.80	871.0
117.80	458.0
118.80	781.0
127.80	383.0
128.90	335.0
129.80	543.0
130.80	173.0
134.80	266.0
136.90	307.0
139.80	108.0
140.80	1384.0
141.90	132.0
142.90	1650.0
144.80	242.0
145.80	222.0
146.90	106.0
147.90	365.0
153.00	143.0
153.70	158.0
154.80	319.0
156.90	196.0
158.90	130.0
160.80	135.0
170.80	129.0
171.90	802.0
173.90	100280.0
174.90	7539.0
175.90	96576.0
176.90	6553.0
177.90	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
35.90	851.0
36.90	4998.0
38.00	4450.0
39.00	1945.0
39.90	156.0
43.90	724.0
44.90	806.0
46.10	109.0
47.00	1367.0
47.80	719.0
49.00	4755.0
50.00	21616.0
51.00	6632.0
52.00	274.0
54.90	266.0
56.00	1944.0
57.00	3618.0
58.00	104.0
60.00	1182.0
61.00	5830.0
61.90	5554.0
63.00	4597.0
64.00	513.0
65.00	613.0
67.00	370.0
68.00	12907.0
69.00	11981.0
70.00	1130.0
71.90	720.0
73.00	5554.0
74.00	21336.0
75.00	64808.0
76.00	5368.0
76.90	720.0
77.90	488.0
78.90	3761.0
79.80	1221.0
80.90	4125.0
81.90	1029.0
86.10	194.0
87.00	5400.0
88.00	4804.0
90.90	438.0
92.00	3900.0
93.00	5599.0
94.00	14775.0
95.00	126288.0
96.00	8348.0
97.00	179.0
103.80	690.0
104.80	369.0
105.90	601.0
111.80	108.0
112.80	112.0
115.90	638.0
116.80	841.0
117.80	501.0
118.80	858.0
124.00	115.0
127.90	371.0
128.90	364.0
129.80	555.0
130.80	169.0
134.70	246.0
137.00	362.0
140.80	1598.0
141.90	126.0
142.90	1776.0
144.80	290.0
145.80	256.0
147.90	346.0
148.70	107.0
153.00	119.0
153.70	132.0
154.80	377.0
156.90	207.0
158.80	128.0
160.80	139.0
170.80	162.0
172.00	854.0
173.90	107024.0
175.00	7703.0
175.90	103768.0
176.90	6629.0
177.90	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012

m/z	Abundance
36.00	725.0
36.90	4699.0
38.00	4155.0
39.00	1863.0
39.90	143.0
43.90	655.0
45.00	766.0
47.00	1438.0
47.80	677.0
49.00	4423.0
50.00	20072.0
51.00	6261.0
51.90	269.0
54.90	264.0
56.00	1893.0
57.00	3345.0
58.00	117.0
60.00	1208.0
61.00	5413.0
62.00	5140.0
63.00	4267.0
64.00	509.0
65.00	547.0
67.00	387.0
68.00	12030.0
69.00	11522.0
70.00	1079.0
72.00	515.0
73.00	5218.0
74.00	20000.0
75.00	61504.0
76.00	4914.0
77.00	585.0
77.90	464.0
78.90	3619.0
79.80	1204.0
80.90	3983.0
81.80	913.0
86.10	178.0
87.00	4999.0
88.00	4462.0
91.00	456.0
91.90	3838.0
93.00	5383.0
94.00	14189.0
95.00	120568.0
96.00	7686.0
97.00	180.0
103.80	710.0
104.80	298.0
105.90	629.0
106.80	100.0
111.80	121.0
115.00	114.0
115.90	586.0
116.80	745.0
117.80	498.0
118.80	816.0
124.00	103.0
127.90	353.0
128.90	305.0
129.80	466.0
130.80	184.0
134.60	229.0
137.00	358.0
140.90	1678.0
141.90	143.0
142.90	1721.0
144.90	290.0
145.80	235.0
147.80	310.0
148.70	115.0
153.70	128.0
154.80	383.0
156.90	216.0
158.80	139.0
160.80	157.0
170.80	153.0
172.00	782.0
173.90	103480.0
175.00	7166.0
175.90	101304.0
176.90	6197.0
178.00	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB012