

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU052019\
Quantitation Report (QT Reviewed)


Data File : VU032155.D
Acq On : 20 May 2019 15:17
Operator : JC/SP
Sample : K2860-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9W38

Manual Integrations
APPROVED

MMDadoda
5/21/2019 11:11:07 AM

Quant Time: May 21 08:25:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 21 06:39:31 2019
Response via : Initial Calibration

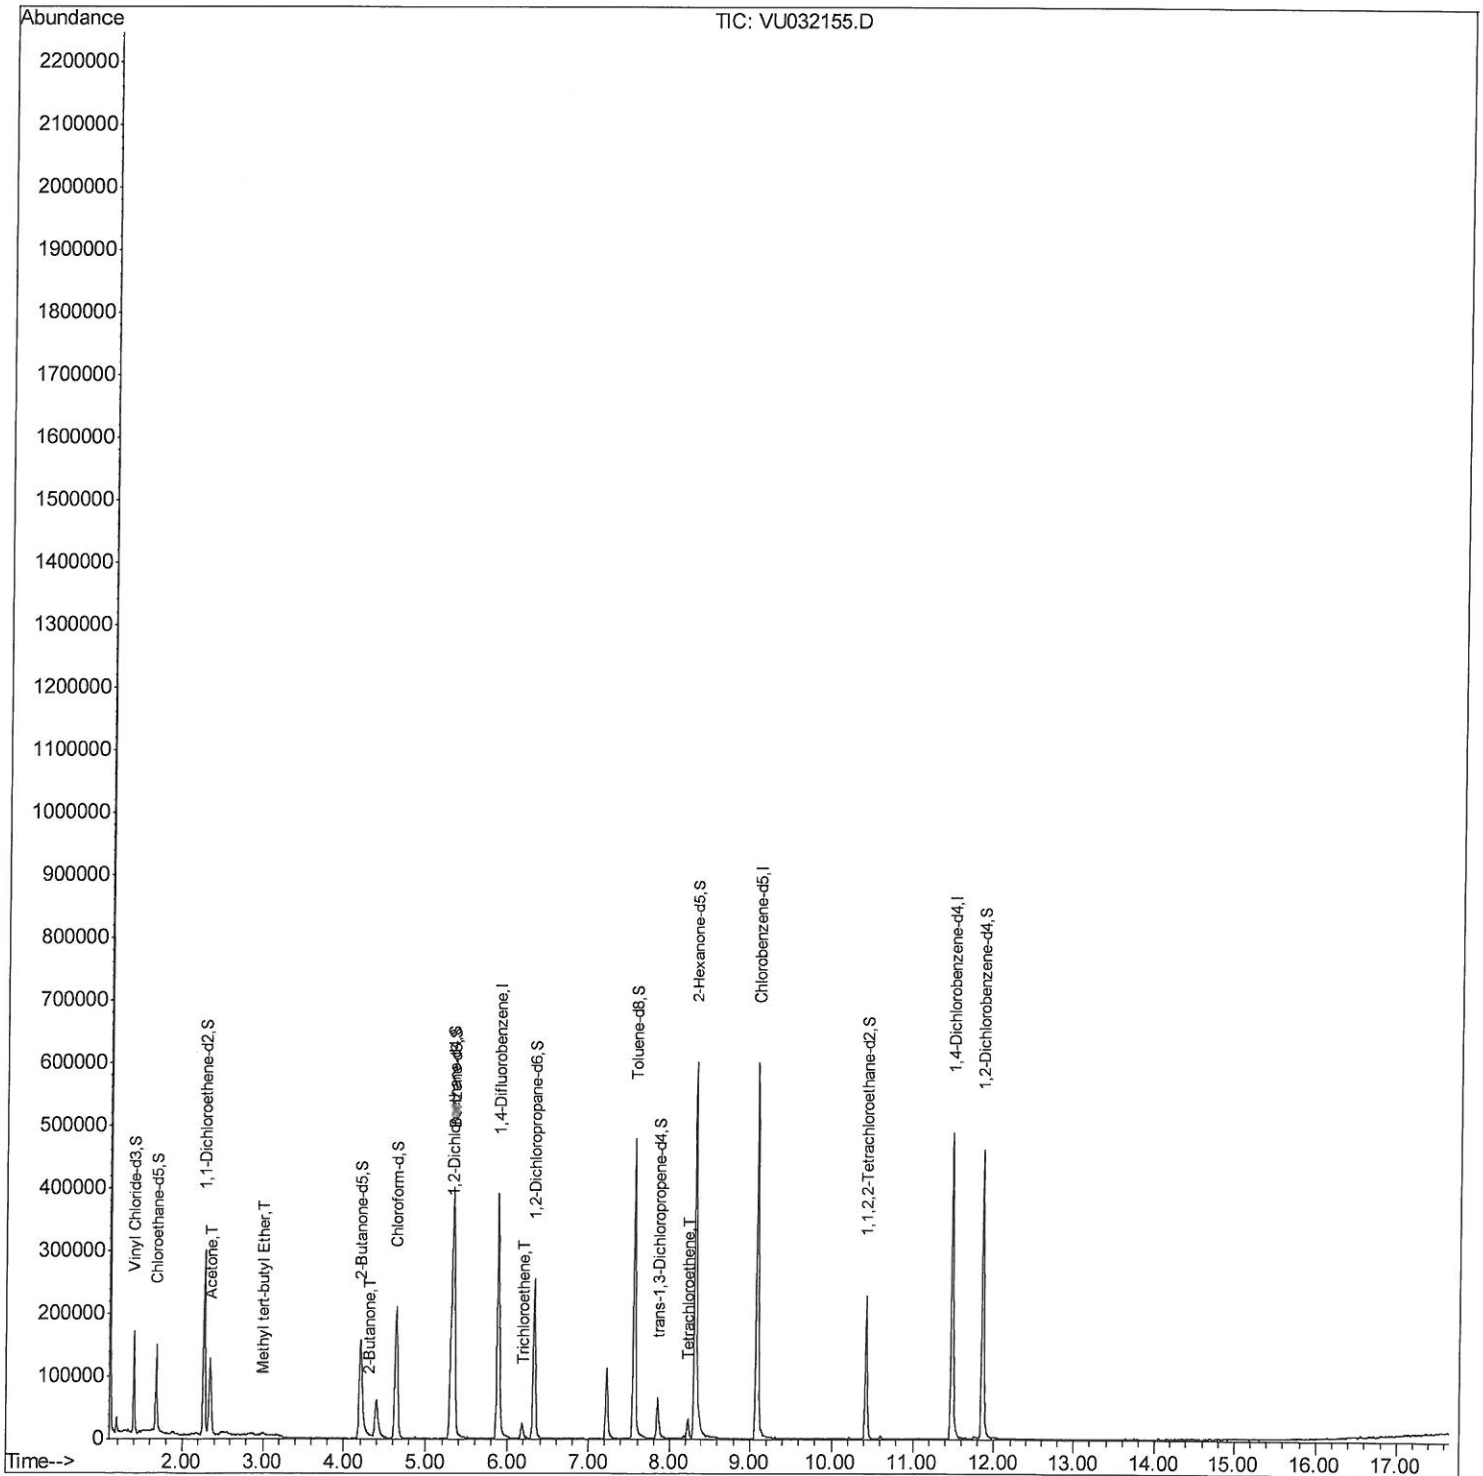

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU052019\
Quantitation Report (Qedit)




Data File : VU032155.D
Acq On : 20 May 2019 15:17
Operator : JC/SP
Sample : K2860-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9W38

Manual Integrations
APPROVED

MMDadoda
5/21/2019 11:11:07 AM

Quant Time: May 21 06:43:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 21 06:39:31 2019
Response via : Initial Calibration

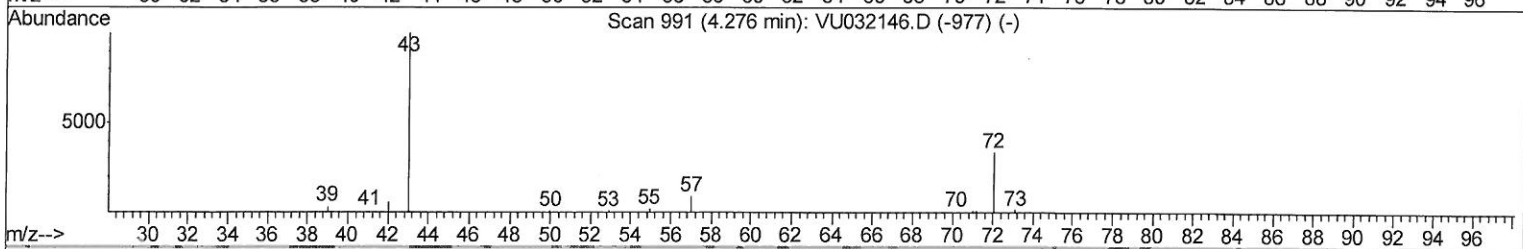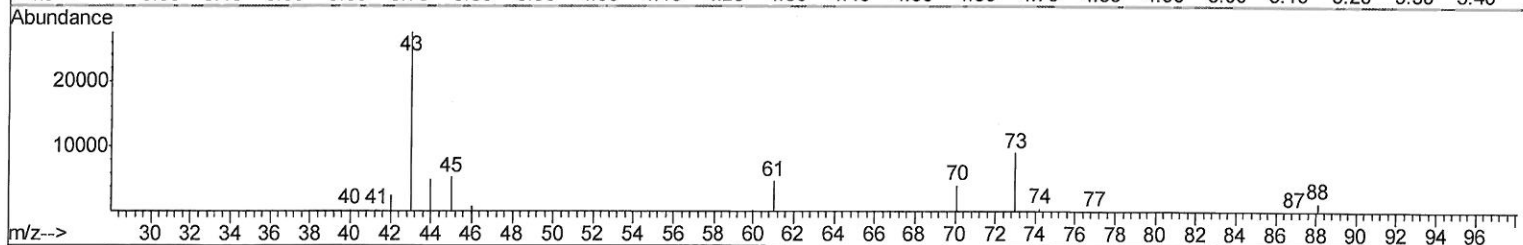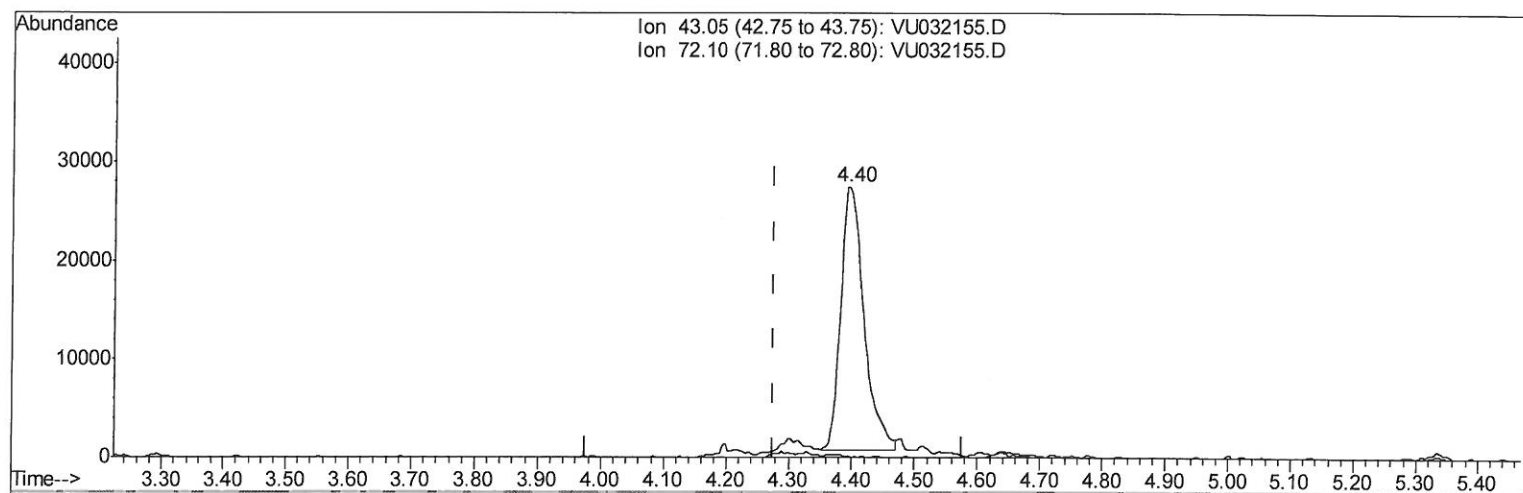

TIC: VU032155.D

(21) 2-Butanone (T)

4.395min (+0.119) 25.07ug/L

response 68482

Ion	Exp%	Act%
43.05	100	100
72.10	33.50	0.84#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU052019\
Quantitation Report (Qedit)




Data File : VU032155.D
Acq On : 20 May 2019 15:17
Operator : JC/SP
Sample : K2860-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9W38

Manual Integrations
APPROVED

MMDadoda
5/21/2019 11:11:07 AM

Quant Time: May 21 06:43:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 21 06:39:31 2019
Response via : Initial Calibration

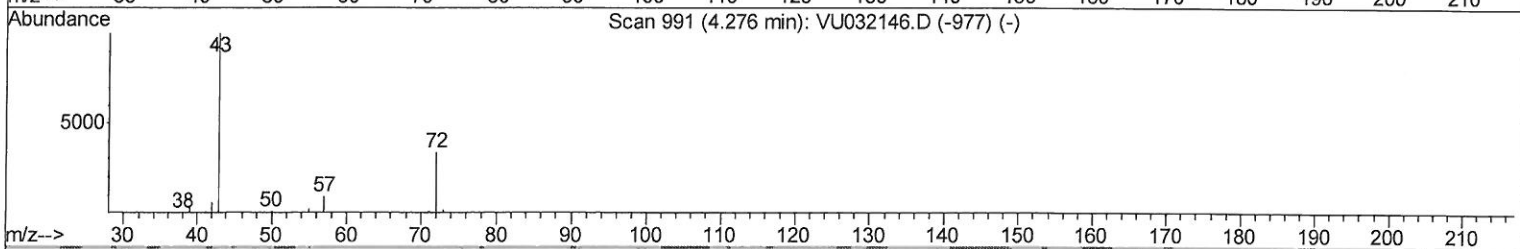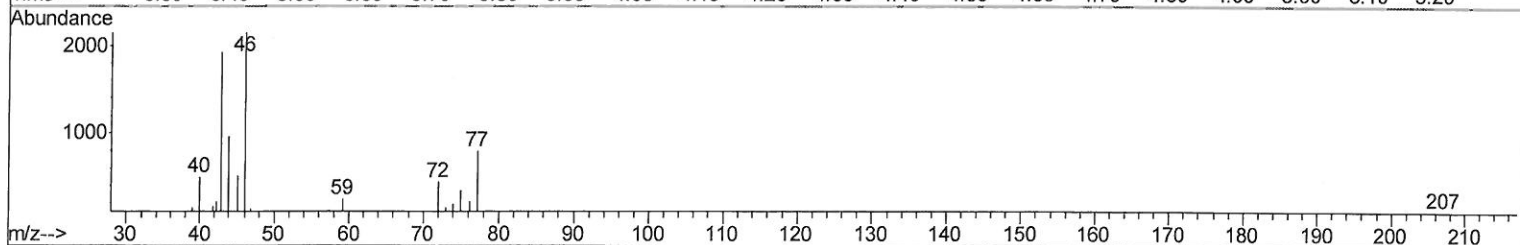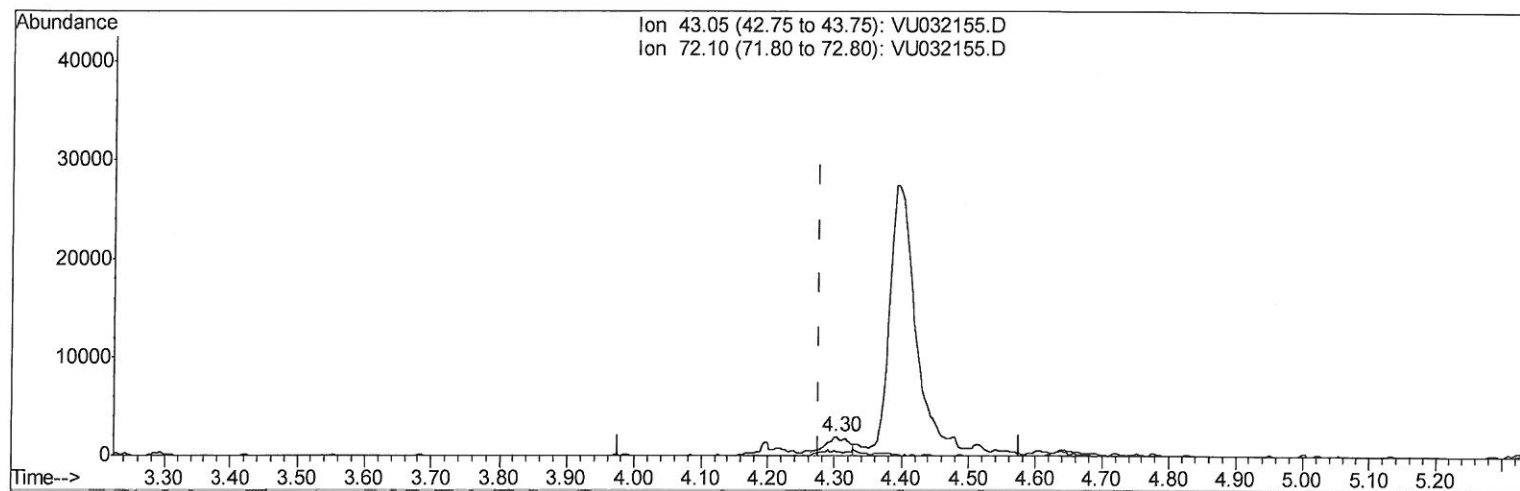

TIC: VU032155.D

(21) 2-Butanone (T)

4.302min (+0.026) 1.76ug/L m

response 4801

Ion	Exp%	Act%
43.05	100	100
72.10	33.50	11.96#
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten: 2ME
5/23/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU052019\
Quantitation Report (QT Reviewed)

Data File : VU032155.D
Acq On : 20 May 2019 15:17
Operator : JC/SP
Sample : K2860-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9W38

Manual Integrations
APPROVED

MMDadoda
5/21/2019 11:11:07 AM

Quant Time: May 21 08:25:43 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue May 21 06:39:31 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	350499	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	371964	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	148761	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	109939	3.72	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.40%
7) Chloroethane-d5	1.68	69	94616	3.75	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.00%
11) 1,1-Dichloroethene-d2	2.27	63	156109	3.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.40%
20) 2-Butanone-d5	4.20	46	253126	43.67	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.34%
24) Chloroform-d	4.64	84	220596	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.00%
26) 1,2-Dichloroethane-d4	5.31	65	115247	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.00%
32) Benzene-d6	5.33	84	432687	3.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.20%
36) 1,2-Dichloropropane-d6	6.33	67	133223	4.02	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.40%
41) Toluene-d8	7.56	98	354776	3.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.00%
43) trans-1,3-Dichloropropene-	7.85	79	43689	3.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.20%
46) 2-Hexanone-d5	8.31	63	216403	40.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.28%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	113733	4.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.00%
64) 1,2-Dichlorobenzene-d4	11.86	152	141090	4.48	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.60%

Target Compounds

					Qvalue
13) Acetone	2.34	43	63202	33.213	ug/L 99
17) Methyl tert-butyl Ether	3.00	73	4051	0.122	ug/L # 93
21) 2-Butanone	4.30	43	4801m	1.758	ug/L 95
34) Trichloroethene	6.18	95	9070	0.585	ug/L 95
47) Tetrachloroethene	8.22	164	8596	0.742	ug/L 87

7 MF
5/23/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed