


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052019\
 Data File : VU032145.D
 Acq On : 20 May 2019 10:06
 Operator : JC/SP
 Sample : BFB10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR051619WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue May 21 13:16:17 2019

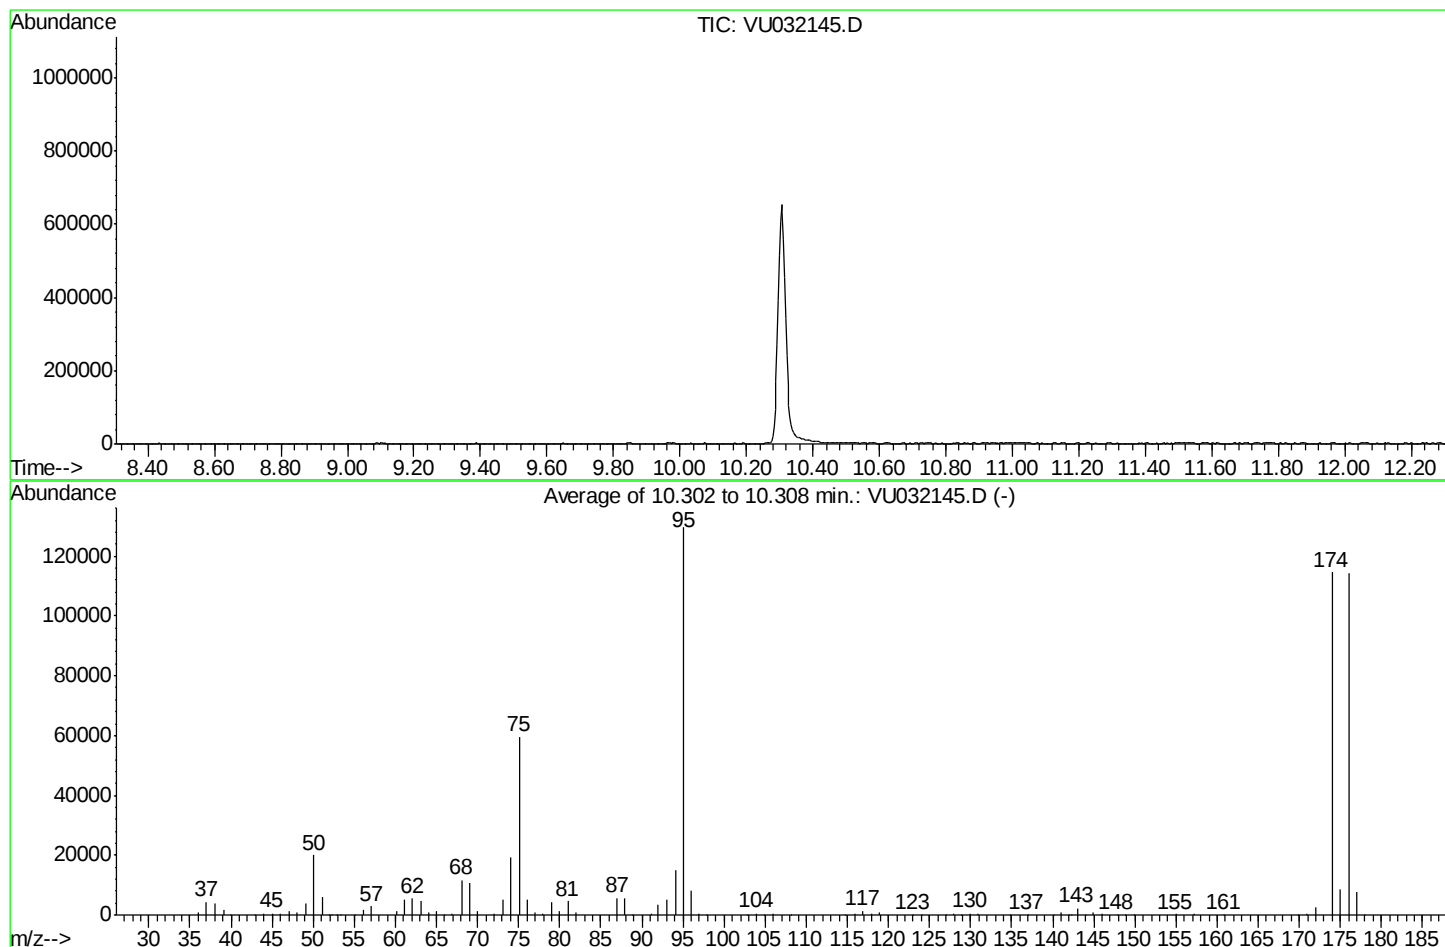

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	19981	PASS
75	95	30	80	46.0	59634	PASS
95	95	100	100	100.0	129637	PASS
96	95	5	9	6.2	7999	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.5	114682	PASS
175	174	5	9	7.4	8515	PASS
176	174	95	101	99.5	114144	PASS
177	176	5	9	6.7	7656	PASS

Scan 2852 (10.260 min): VU032145.D
BFB10

m/z	Abundance
39.90	875.0
43.90	835.0
64.00	101.0
206.90	269.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	782.0
37.00	4312.0
38.00	3945.0
39.10	1867.0
40.00	817.0
42.90	102.0
44.00	1107.0
45.00	591.0
46.00	329.0
47.00	1046.0
48.00	730.0
49.10	3995.0
50.10	19480.0
51.10	5360.0
51.90	302.0
52.90	165.0
53.30	102.0
55.00	244.0
56.00	1556.0
57.10	3024.0
60.10	1163.0
61.10	5092.0
62.10	5085.0
63.10	4650.0
64.00	1217.0
64.90	1316.0
65.80	115.0
66.90	240.0
68.00	11816.0
69.00	10517.0
70.00	1317.0
72.10	518.0
73.10	5167.0
74.10	19240.0
75.10	57944.0
76.00	5365.0
77.10	774.0
77.90	521.0
79.00	4372.0
79.90	1509.0
81.00	4749.0
81.90	1146.0
87.00	5480.0
87.90	5511.0
88.80	251.0
91.10	627.0
91.90	2996.0
93.10	4689.0
94.10	14545.0
95.10	126488.0
96.10	8161.0
97.00	430.0
104.00	499.0
105.90	429.0
108.10	124.0
114.70	153.0
116.00	560.0
116.90	1191.0
118.00	495.0
119.00	850.0
123.00	134.0
127.00	118.0
127.90	435.0
128.80	125.0
129.90	589.0
131.00	258.0
137.00	228.0
141.10	987.0
142.00	232.0
143.00	2152.0
144.00	147.0
144.90	1006.0
146.10	323.0
147.90	171.0
148.80	117.0
154.90	385.0
157.10	261.0
171.00	370.0
172.00	2178.0
174.00	106976.0
175.00	8156.0
176.00	108896.0
177.00	7436.0
177.90	138.0
206.90	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	807.0
37.00	4602.0
38.00	4182.0
39.10	1767.0
40.00	1058.0
44.00	1170.0
45.10	702.0
46.00	369.0
47.00	1263.0
48.00	834.0
49.00	3915.0
50.10	20816.0
51.10	6095.0
51.90	268.0
52.80	150.0
53.30	134.0
55.00	247.0
56.00	1699.0
57.10	3037.0
60.10	1185.0
61.10	5055.0
62.10	5741.0
63.10	4951.0
64.00	1229.0
65.00	1277.0
65.80	110.0
66.80	315.0
68.10	11983.0
69.00	10847.0
70.00	1277.0
72.00	521.0
73.10	5475.0
74.00	20104.0
75.10	61648.0
76.00	5525.0
77.10	962.0
78.00	661.0
79.00	4676.0
80.00	1567.0
81.00	4809.0
81.90	1056.0
87.00	5861.0
87.90	5882.0
88.80	240.0
91.10	568.0
92.00	3425.0
93.00	5160.0
94.10	15334.0
95.10	134080.0
96.00	8213.0
97.00	431.0
97.80	114.0
102.80	138.0
104.00	461.0
104.80	128.0
105.90	441.0
114.70	163.0
116.00	565.0
116.90	1455.0
118.00	417.0
119.00	884.0
123.00	160.0
123.90	106.0
127.00	129.0
127.90	434.0
128.80	158.0
130.00	505.0
131.00	243.0
134.80	160.0
137.00	194.0
140.00	105.0
141.10	1054.0
141.90	230.0
143.00	2399.0
144.00	150.0
144.90	1075.0
146.10	338.0
147.80	180.0
149.90	113.0
155.00	396.0
157.10	235.0
160.80	110.0
169.90	116.0
170.90	532.0
172.00	2505.0
174.00	118376.0
175.00	8911.0
176.00	118248.0
177.00	7922.0
177.90	136.0
206.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.10	824.0
37.00	4350.0
38.00	3730.0
39.10	1514.0
40.00	1110.0
44.00	1069.0
45.10	661.0
46.00	306.0
47.00	1472.0
48.00	802.0
49.00	3757.0
50.10	19648.0
51.00	6188.0
52.20	242.0
52.90	161.0
53.30	128.0
55.00	189.0
56.10	1745.0
57.00	2895.0
60.10	1029.0
61.00	5065.0
62.10	5616.0
63.10	4892.0
64.00	1057.0
65.10	1283.0
65.90	121.0
66.90	336.0
68.10	11341.0
69.00	10543.0
70.00	970.0
71.90	483.0
73.10	5000.0
74.00	19136.0
75.10	59312.0
76.10	4983.0
77.00	969.0
78.00	785.0
79.00	4418.0
80.00	1323.0
81.00	4367.0
81.90	816.0
87.00	5800.0
88.00	5645.0
88.80	134.0
91.10	414.0
92.00	3790.0
93.00	5363.0
94.10	15109.0
95.10	128344.0
96.00	7624.0
97.00	298.0
102.80	153.0
104.00	353.0
104.80	218.0
105.90	402.0
114.70	128.0
116.00	585.0
116.90	1380.0
118.00	346.0
118.90	872.0
124.00	109.0
127.90	409.0
128.80	199.0
130.10	439.0
130.90	197.0
134.80	232.0
136.90	170.0
140.10	118.0
141.00	977.0
142.20	204.0
143.00	2426.0
144.90	1003.0
146.00	322.0
147.80	227.0
149.90	117.0
155.10	464.0
157.20	203.0
160.90	195.0
169.80	102.0
170.90	651.0
172.00	2565.0
174.00	118696.0
175.00	8478.0
176.00	115288.0
177.00	7610.0
177.90	106.0
207.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10