

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU052020\
 Data File : VU038243.D
 Acq On : 20 May 2020 13:27
 Operator : JC/MD
 Sample : L2724-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE4T5

Quant Time: May 21 01:38:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu May 21 01:14:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	356145	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	346115	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	164518	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	107290	3.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.80%
7) Chloroethane-d5	1.93	69	104593	3.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	74.20%
11) 1,1-Dichloroethene-d2	2.59	63	135953	2.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	50.00%#
20) 2-Butanone-d5	4.68	46	478276	59.51	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.02%
24) Chloroform-d	5.10	84	211803	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
26) 1,2-Dichloroethane-d4	5.74	65	133442	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.20%
32) Benzene-d6	5.76	84	418427	4.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.60%
36) 1,2-Dichloropropane-d6	6.72	67	146610	4.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.60%
41) Toluene-d8	7.93	98	350092	3.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.20%
43) trans-1,3-Dichloropropene-	8.20	79	55286	4.12	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.40%
46) 2-Hexanone-d5	8.66	63	361896	57.15	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	114.30%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	135048	5.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.20%
64) 1,2-Dichlorobenzene-d4	12.21	152	146614	4.58	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.60%


Target Compounds					Ovalue
13) Acetone	2.69	43	20748	4.114 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU052020\
Data File : VU038243.D
Acq On : 20 May 2020 13:27
Operator : JC/MD
Sample : L2724-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE4T5

Quant Time: May 21 01:38:58 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu May 21 01:14:05 2020
Response via : Initial Calibration

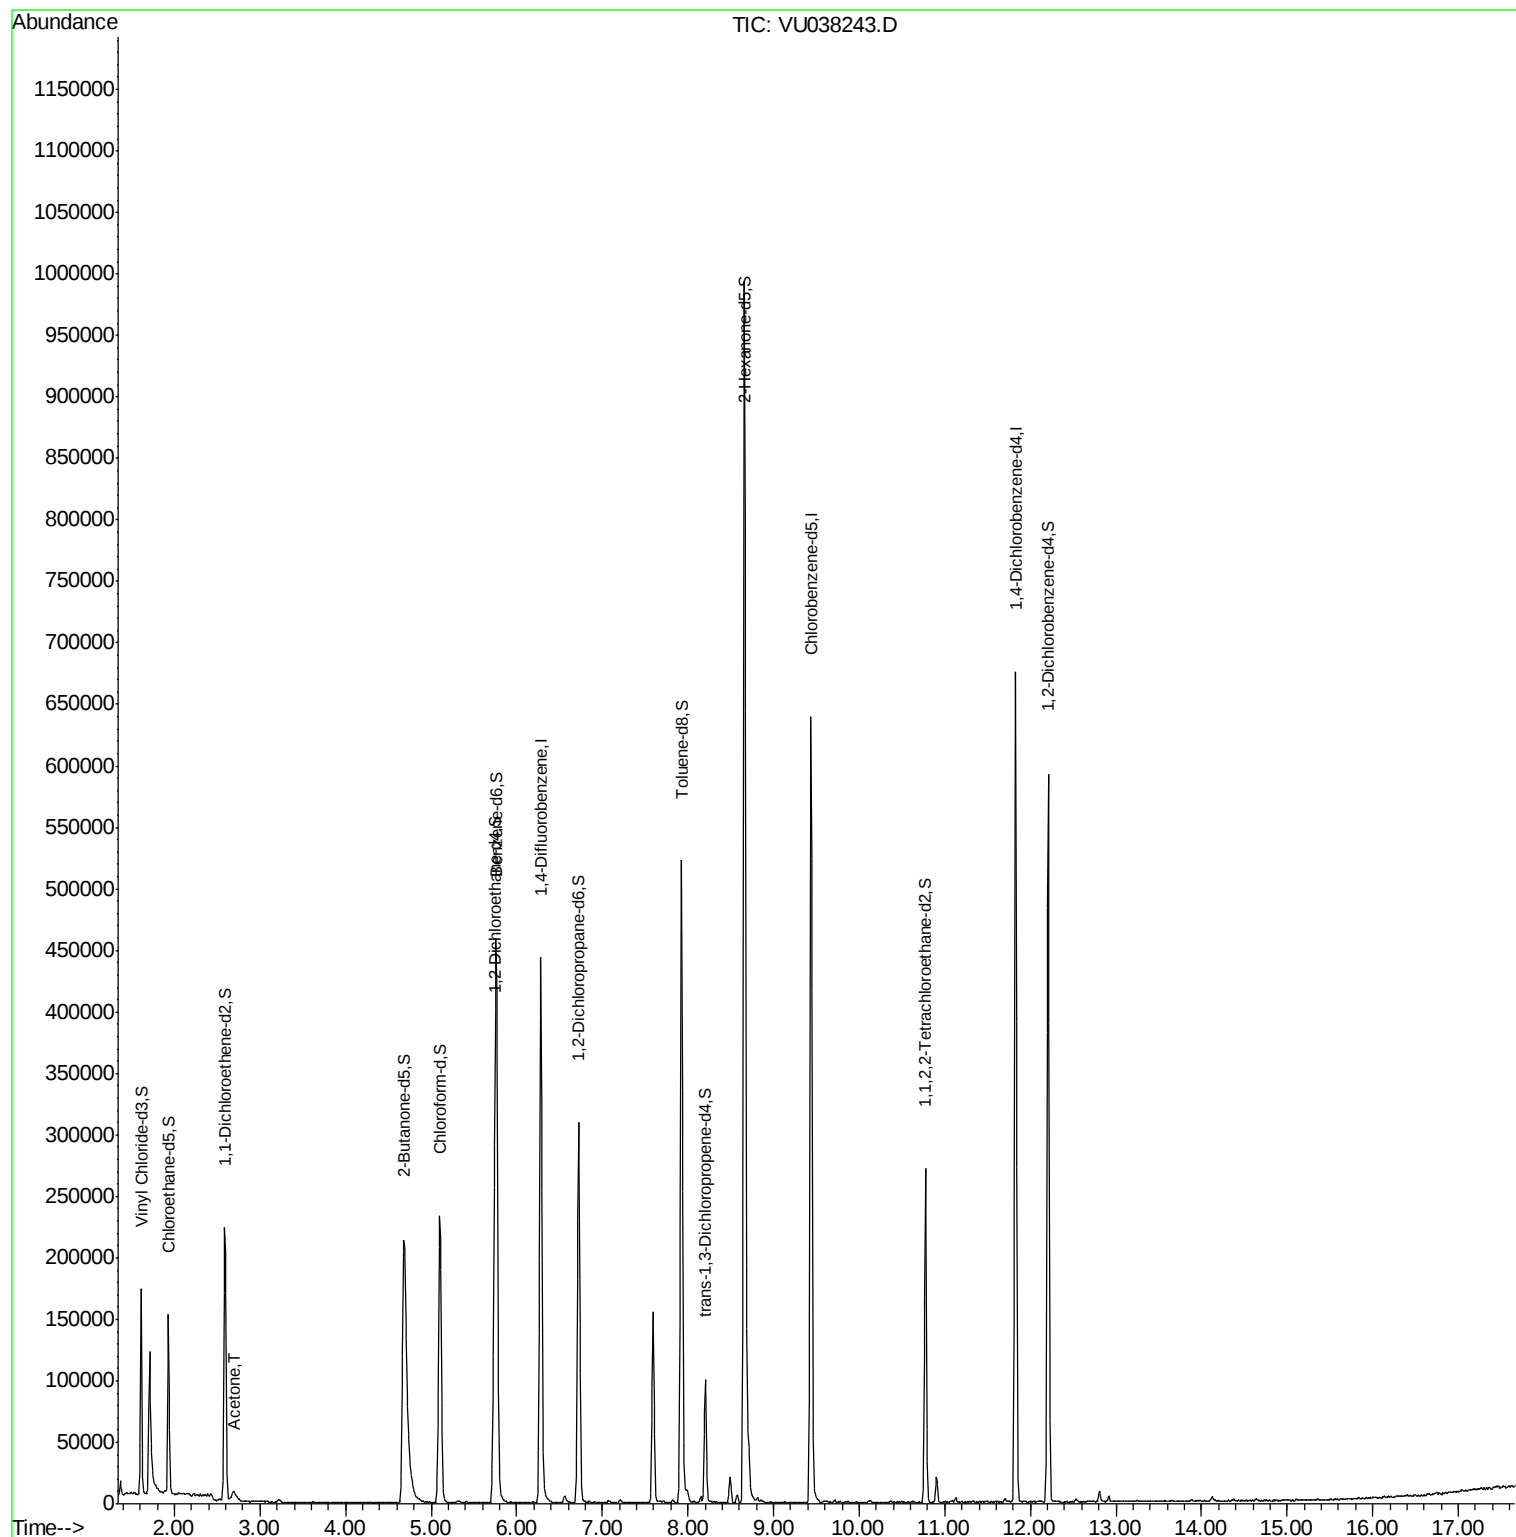

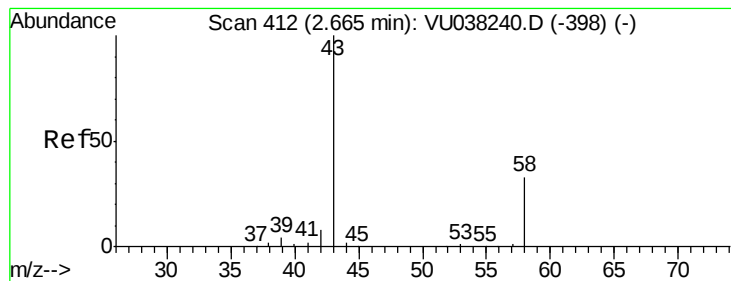

#13
 Acetone
 Concen: 4.114 ug/L
 RT: 2.69 min Scan# 421
 Delta R.T. 0.03 min
 Lab File: VU038243.D
 Acq: 20 May 2020 13:27

Instrument :
 MSVOA_U
 ClientSampleId :
 BE4T5

Tot Ion: 43 Resp: 20748
 Ion Ratio Lower Upper
 43 100
 58 23.5 0.0 63.6

