

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043828.D
 Acq On : 19 May 2021 15:47
 Operator : SY/MD
 Sample : M2459-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GK1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	93	rBV	98383	112326	15.36%	1.791%
2	1.691	103	109	118	rBV	7310	9399	1.29%	0.150%
3	1.916	170	179	191	rVB	65665	82925	11.34%	1.322%
4	2.568	371	382	398	rBV	168304	273614	37.42%	4.362%
5	2.649	398	407	429	rVV2	9308	24598	3.36%	0.392%
6	3.054	520	533	546	rVB2	8881	16530	2.26%	0.264%
7	3.707	722	736	746	rVB7	3913	8759	1.20%	0.140%
8	4.649	1012	1029	1052	rBV2	71987	222675	30.45%	3.550%
9	5.073	1144	1161	1184	rBV	138207	304733	41.67%	4.858%
10	5.732	1345	1366	1395	rBV2	288881	731233	100.00%	11.657%
11	6.256	1511	1529	1555	rBV	276598	521373	71.30%	8.312%
12	6.700	1653	1667	1686	rBV	174726	336175	45.97%	5.359%
13	7.575	1926	1939	1960	rBV	81587	148074	20.25%	2.361%
14	7.906	2028	2042	2057	rBV	348879	589566	80.63%	9.399%
15	7.977	2059	2064	2073	rVB	5621	8552	1.17%	0.136%
16	8.186	2115	2129	2146	rBV2	50588	88116	12.05%	1.405%
17	8.645	2259	2272	2317	rBV	330046	714079	97.65%	11.384%
18	9.423	2501	2514	2531	rBV	401731	657750	89.95%	10.486%
19	9.510	2531	2541	2554	rVB2	44653	69965	9.57%	1.115%
20	9.697	2590	2599	2611	rBV2	5097	7414	1.01%	0.118%
21	10.764	2919	2931	2949	rBV	133550	214403	29.32%	3.418%
22	11.819	3244	3259	3281	rBV	375974	597259	81.68%	9.522%
23	12.066	3326	3336	3348	rBV3	9524	15039	2.06%	0.240%
24	12.202	3363	3378	3402	rBV	316066	518090	70.85%	8.260%




Sum of corrected areas: 6272647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043828.D
Acq On : 19 May 2021 15:47
Operator : SY/MD
Sample : M2459-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

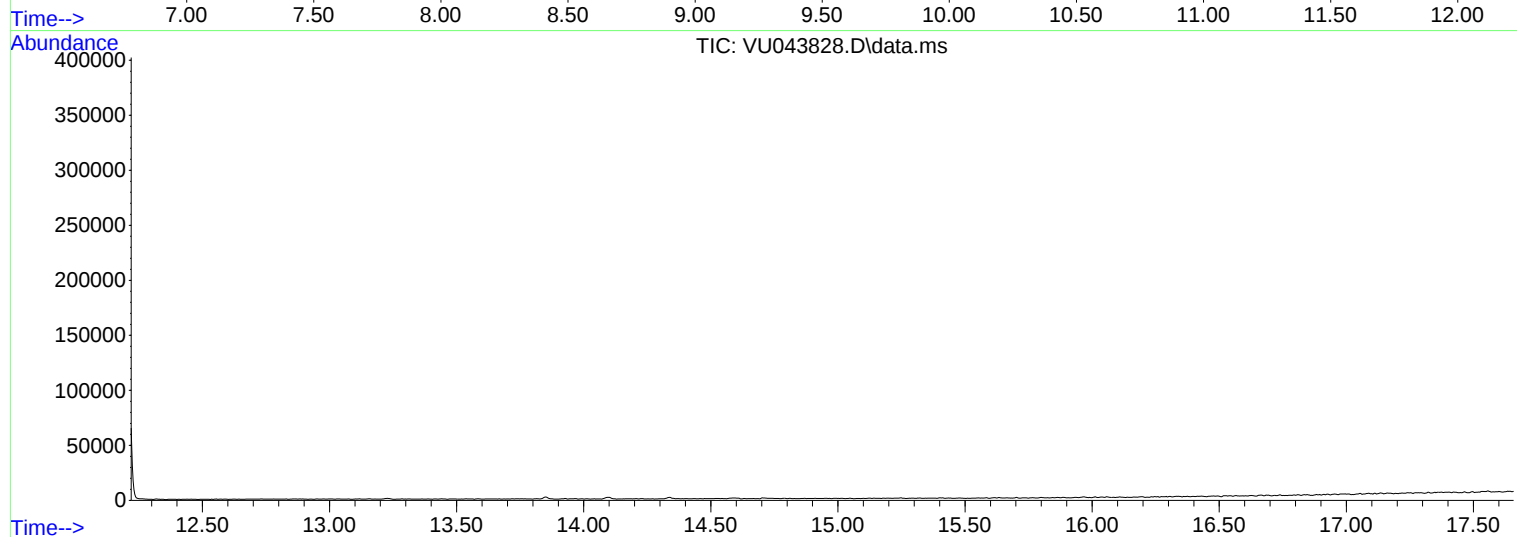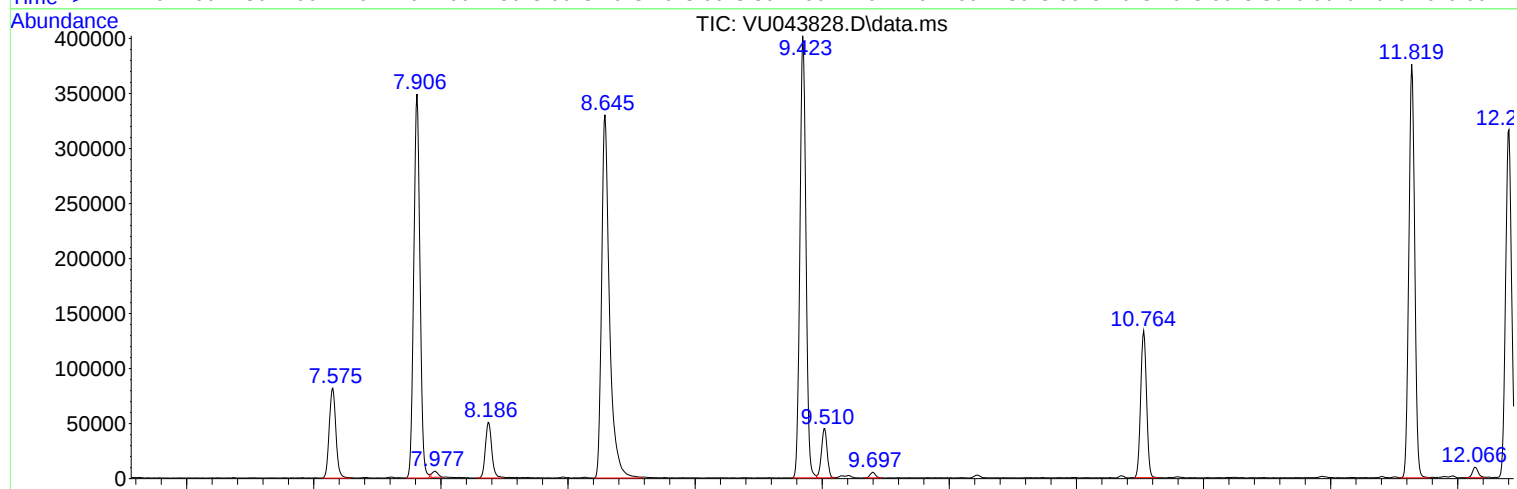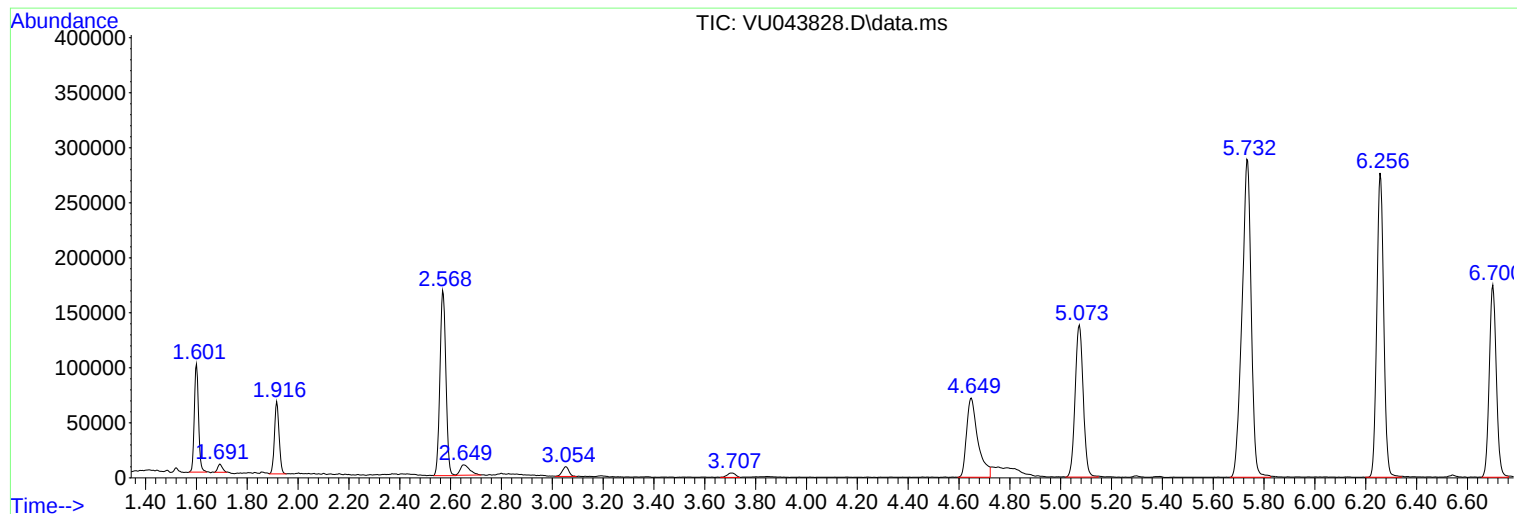

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043828.D
Acq On : 19 May 2021 15:47
Operator : SY/MD
Sample : M2459-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzene, 1-chloro-4-(triflu... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.510	0.53 ug/L	69965	Chlorobenzene-d5	9.423

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-chloro-4-(trifluorome...	180	C7H4ClF3	000098-56-6	98
2			Benzene, 1-chloro-4-(trifluorome...	180	C7H4ClF3	000098-56-6	98
3			Benzene, 1-chloro-4-(trifluorome...	180	C7H4ClF3	000098-56-6	98
4			Benzene, 1-chloro-2-(trifluorome...	180	C7H4ClF3	000088-16-4	95
5			Benzene, 1-chloro-2-(trifluorome...	180	C7H4ClF3	000088-16-4	94

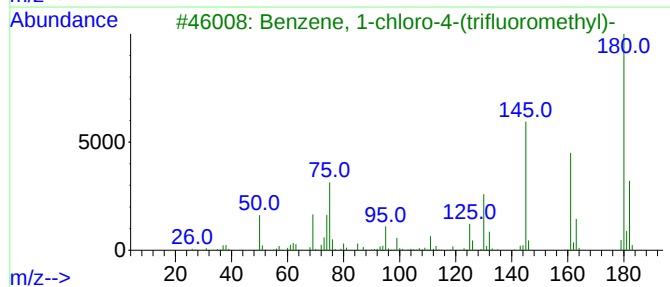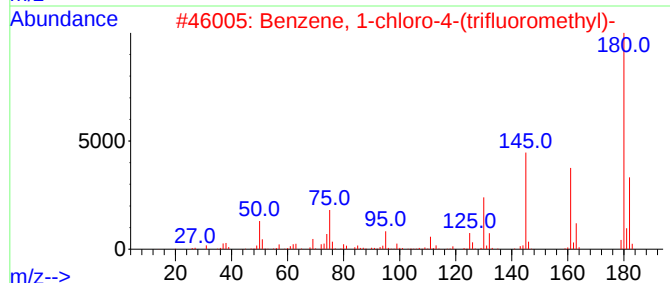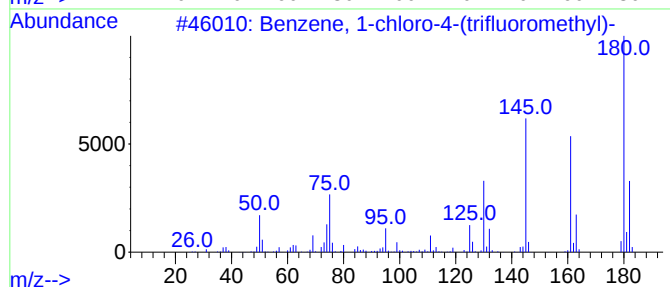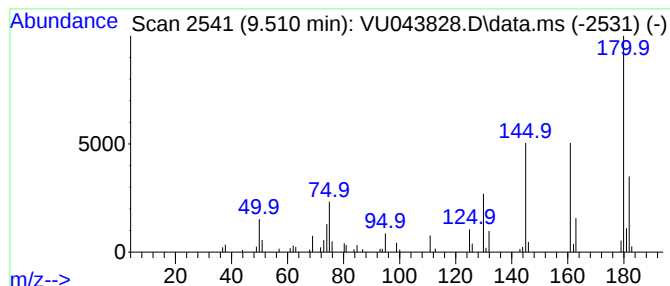

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043828.D
Acq On : 19 May 2021 15:47
Operator : SY/MD
Sample : M2459-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1-chlo...	9.510	0.5	ug/L	69965	2	9.423	657750	5.0