

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043830.D
 Acq On : 19 May 2021 16:36
 Operator : SY/MD
 Sample : M2460-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AR3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	70	81	92	rBV	101748	127749	17.42%	1.938%
2	1.916	171	179	194	rVB	67777	89702	12.23%	1.361%
3	2.571	369	383	398	rBV	165689	269457	36.74%	4.089%
4	2.800	443	454	467	rBV	12495	21863	2.98%	0.332%
5	3.054	522	533	544	rBV2	4786	8818	1.20%	0.134%
6	4.645	1010	1028	1064	rBV	84731	271743	37.05%	4.123%
7	5.092	1144	1167	1191	rBV4	229802	704322	96.03%	10.687%
8	5.735	1344	1367	1385	rBV2	287394	726601	99.07%	11.025%
9	6.259	1514	1530	1548	rBV	267997	507146	69.15%	7.695%
10	6.700	1652	1667	1684	rBV	174523	337225	45.98%	5.117%
11	7.574	1926	1939	1963	rBV	82878	147216	20.07%	2.234%
12	7.906	2029	2042	2056	rBV	336091	581797	79.33%	8.828%
13	7.973	2057	2063	2075	rVB	9507	16881	2.30%	0.256%
14	8.189	2117	2130	2147	rBV	49860	86370	11.78%	1.311%
15	8.645	2255	2272	2309	rBV	347839	733431	100.00%	11.129%
16	9.423	2501	2514	2534	rBV	375790	639351	87.17%	9.701%
17	10.764	2918	2931	2947	rBV	132387	216959	29.58%	3.292%
18	11.819	3247	3259	3276	rBV	362072	576862	78.65%	8.753%
19	12.201	3365	3378	3395	rBV	320067	516677	70.45%	7.840%
20	13.848	3880	3890	3902	rVB2	6584	10113	1.38%	0.153%




Sum of corrected areas: 6590283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043830.D
Acq On : 19 May 2021 16:36
Operator : SY/MD
Sample : M2460-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

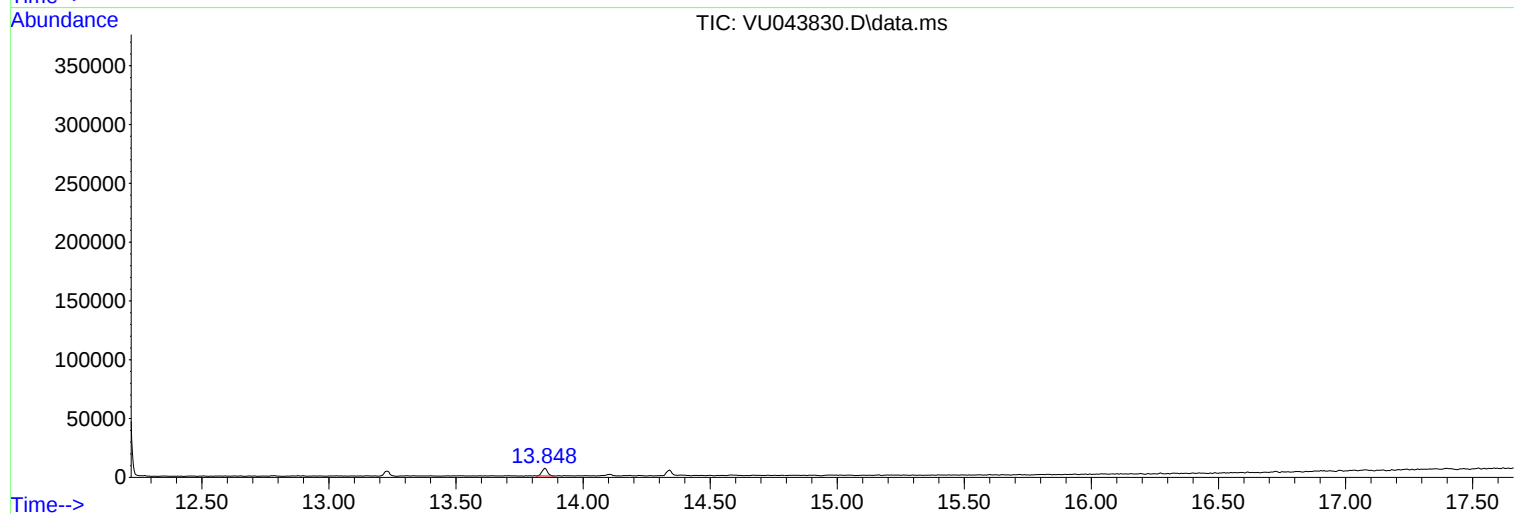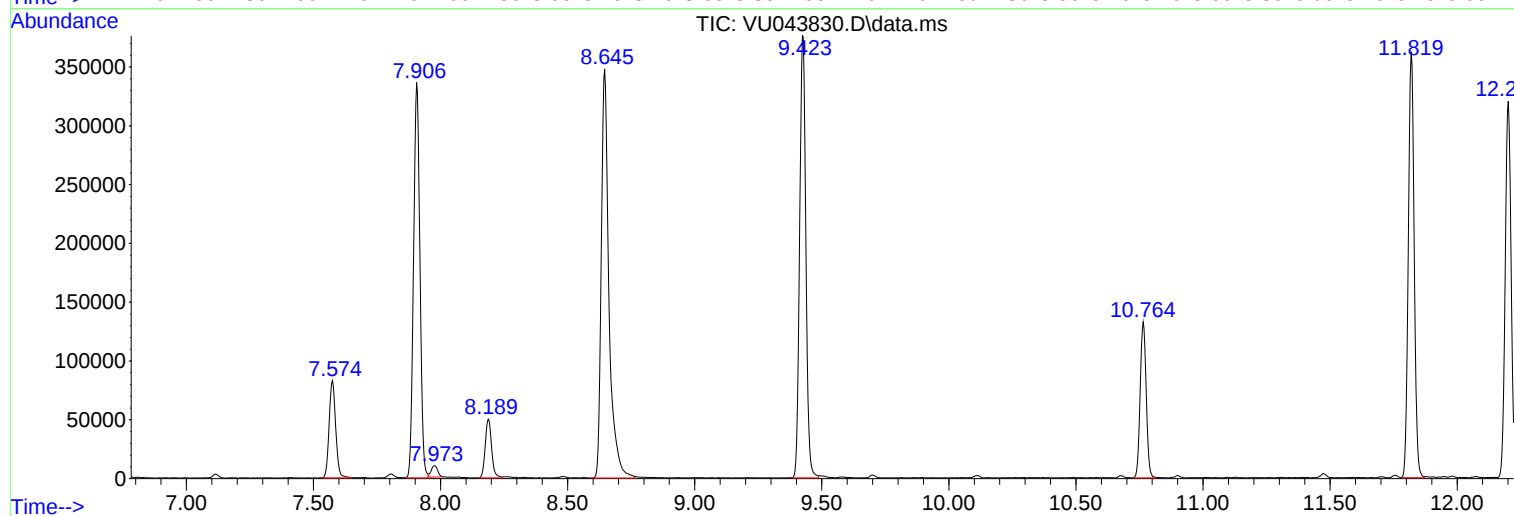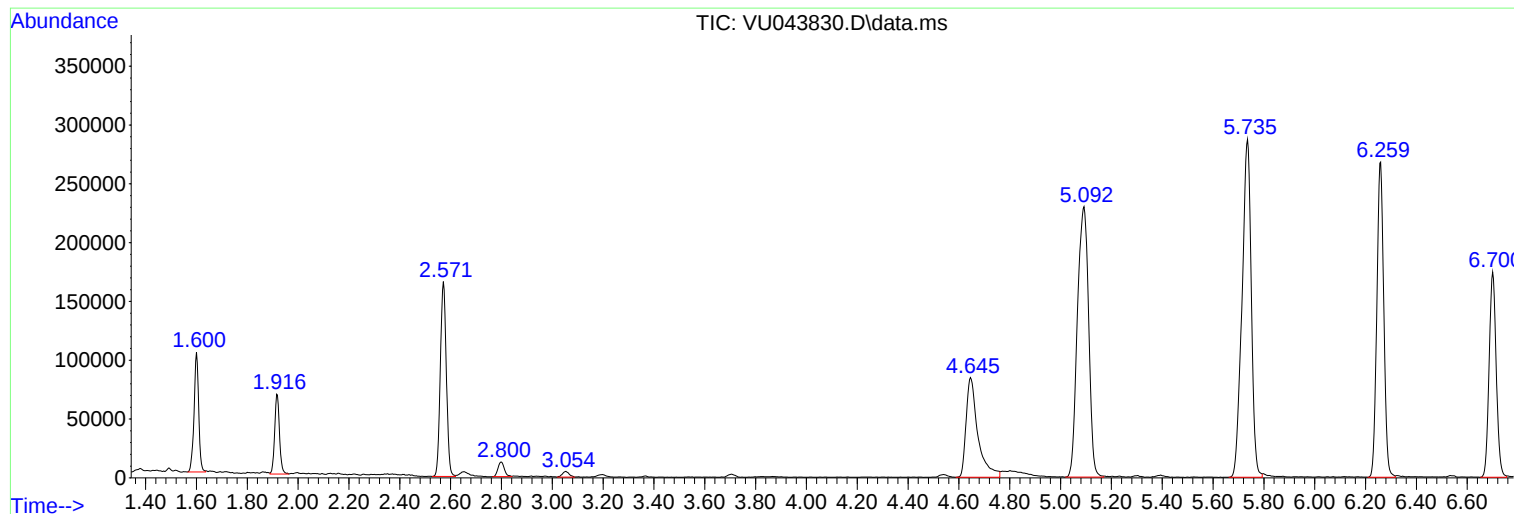

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043830.D
Acq On : 19 May 2021 16:36
Operator : SY/MD
Sample : M2460-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043830.D
Acq On : 19 May 2021 16:36
Operator : SY/MD
Sample : M2460-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
