

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043842.D
 Acq On : 19 May 2021 21:27
 Operator : SY/MD
 Sample : M2464-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB3Z1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	93	rBV	93262	104409	7.08%	1.232%
2	1.915	171	179	192	rVB	61729	78540	5.33%	0.926%
3	2.571	370	383	398	rBV2	160237	276836	18.77%	3.266%
4	4.642	1011	1027	1075	rBV	117516	332428	22.54%	3.921%
5	5.073	1143	1161	1191	rBV2	138259	303882	20.61%	3.585%
6	5.327	1219	1240	1269	rBV	654339	1474596	100.00%	17.395%
7	5.735	1341	1367	1395	rBV2	280658	716143	48.57%	8.448%
8	6.259	1514	1530	1551	rBV	264004	506363	34.34%	5.973%
9	6.700	1653	1667	1685	rBV	173741	333871	22.64%	3.938%
10	7.574	1924	1939	1964	rVB	79840	142432	9.66%	1.680%
11	7.906	2028	2042	2057	rBV	326832	560898	38.04%	6.616%
12	7.976	2057	2064	2076	rVB	9133	15310	1.04%	0.181%
13	8.185	2115	2129	2148	rBV	50593	85907	5.83%	1.013%
14	8.562	2232	2246	2259	rBV	460831	771621	52.33%	9.102%
15	8.645	2259	2272	2303	rVB	428395	819615	55.58%	9.668%
16	9.423	2502	2514	2536	rBV	381183	640086	43.41%	7.551%
17	10.764	2917	2931	2949	rBV	143917	229385	15.56%	2.706%
18	11.819	3247	3259	3275	rBV	362058	573424	38.89%	6.764%
19	12.201	3365	3378	3394	rBV	323331	511537	34.69%	6.034%




Sum of corrected areas: 8477283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043842.D
Acq On : 19 May 2021 21:27
Operator : SY/MD
Sample : M2464-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3Z1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

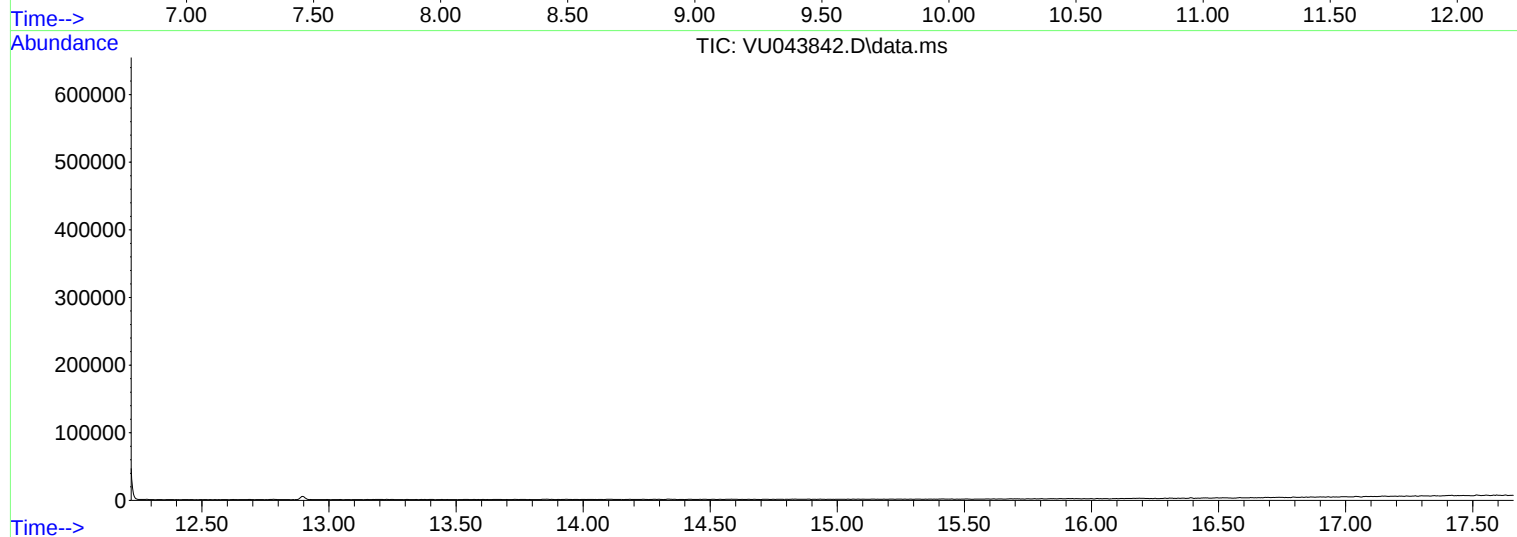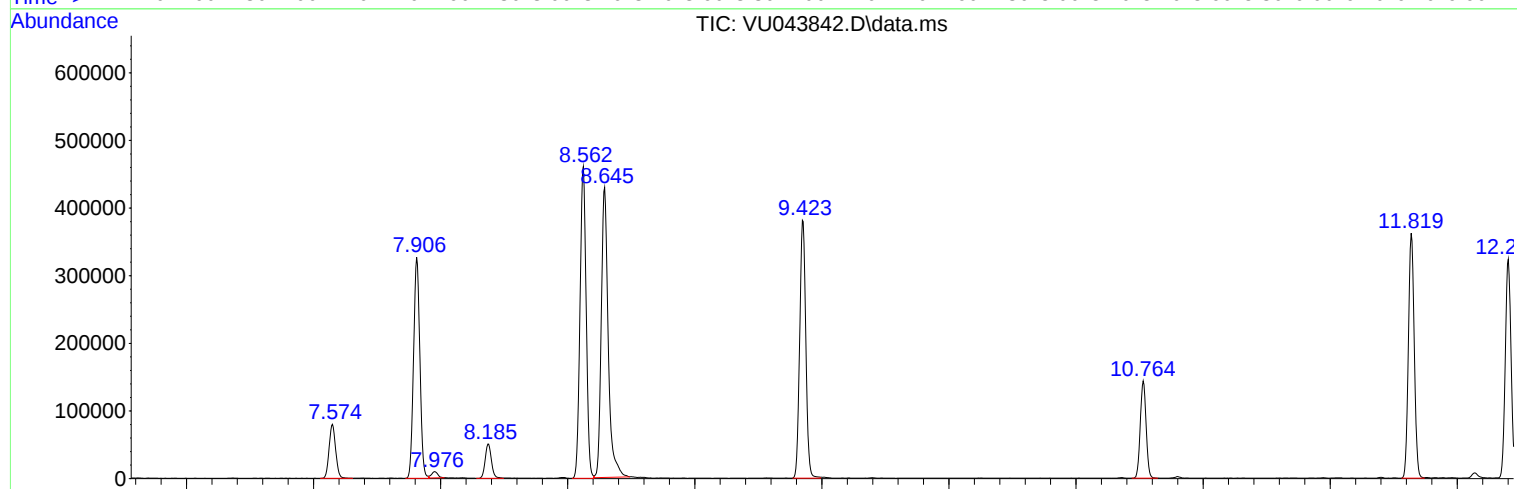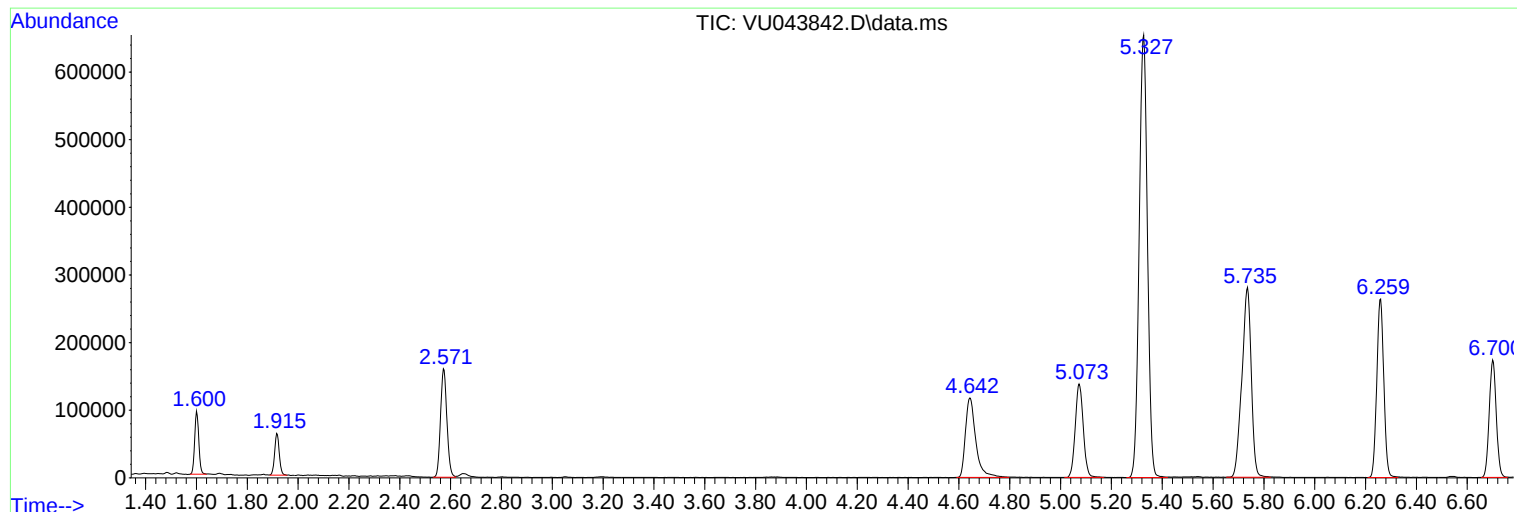

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043842.D
Acq On : 19 May 2021 21:27
Operator : SY/MD
Sample : M2464-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3Z1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043842.D
Acq On : 19 May 2021 21:27
Operator : SY/MD
Sample : M2464-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3Z1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
