

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043846.D
 Acq On : 19 May 2021 23:04
 Operator : SY/MD
 Sample : M2459-03 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GK2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rBV	88517	99195	12.62%	1.660%
2	1.916	171	179	194	rVB	62448	79657	10.14%	1.333%
3	2.572	370	383	401	rBV	153890	250190	31.84%	4.188%
4	3.054	522	533	549	rBV	12632	23347	2.97%	0.391%
5	4.645	1011	1028	1093	rBV	93866	326030	41.49%	5.458%
6	5.073	1145	1161	1186	rBV	132256	292195	37.19%	4.891%
7	5.735	1344	1367	1385	rBV2	264454	680056	86.55%	11.384%
8	6.256	1515	1529	1553	rBV	243955	463589	59.00%	7.760%
9	6.552	1608	1621	1637	rVB	36248	68847	8.76%	1.152%
10	6.700	1653	1667	1689	rBV	162640	320162	40.75%	5.359%
11	7.575	1926	1939	1956	rBV	76371	133630	17.01%	2.237%
12	7.906	2027	2042	2058	rBV	305597	528562	67.27%	8.848%
13	8.189	2117	2130	2153	rBV	46758	80710	10.27%	1.351%
14	8.645	2259	2272	2314	rBV	385787	785715	100.00%	13.152%
15	8.925	2349	2359	2379	rVB3	3949	8016	1.02%	0.134%
16	9.423	2501	2514	2533	rBV	362348	596602	75.93%	9.987%
17	10.764	2918	2931	2946	rVB	138193	221633	28.21%	3.710%
18	11.819	3247	3259	3274	rBV	338933	529101	67.34%	8.857%
19	12.201	3360	3378	3401	rBV	296873	486709	61.94%	8.147%




Sum of corrected areas: 5973946

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043846.D
Acq On : 19 May 2021 23:04
Operator : SY/MD
Sample : M2459-03 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

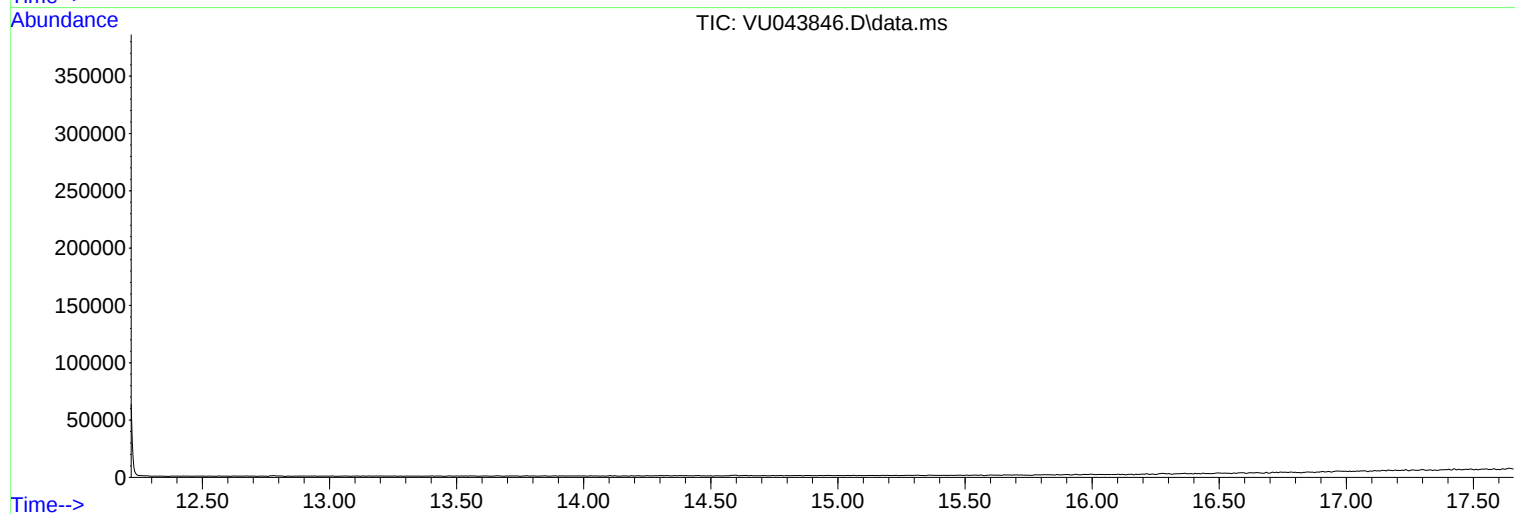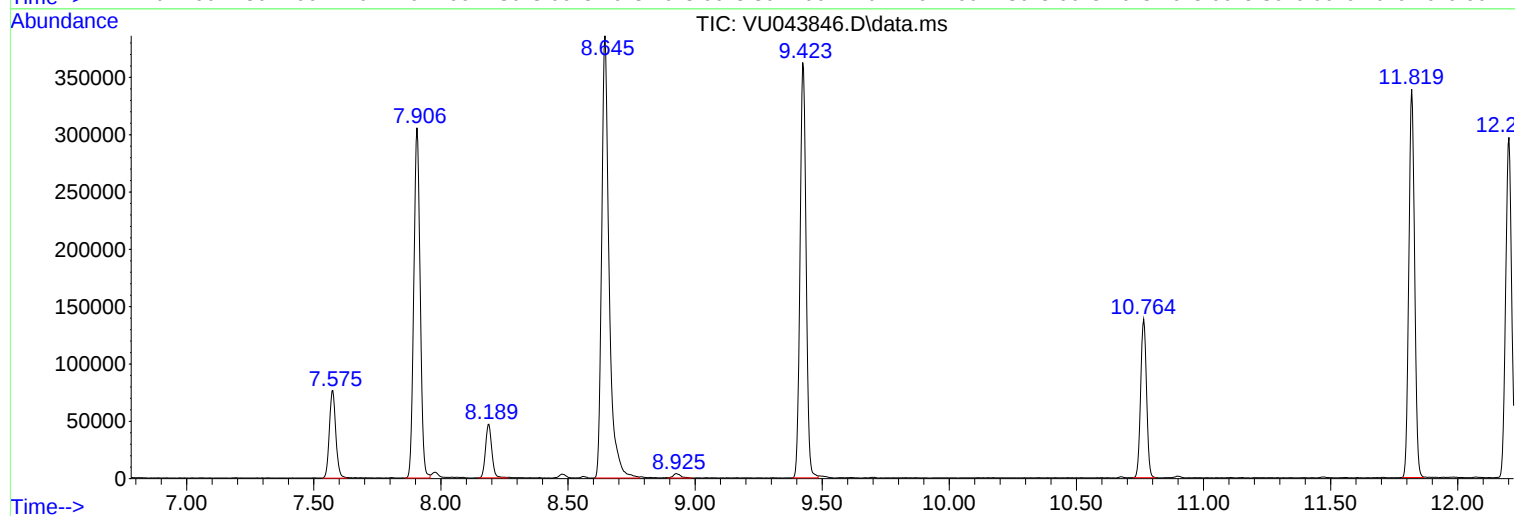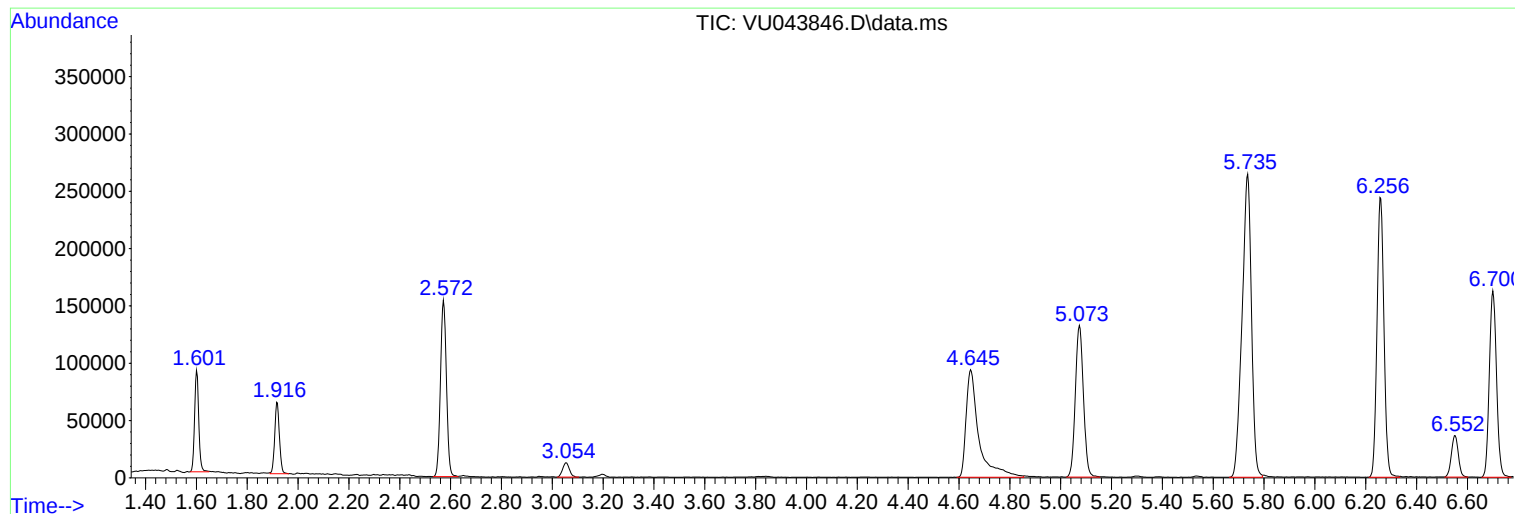

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043846.D
Acq On : 19 May 2021 23:04
Operator : SY/MD
Sample : M2459-03 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043846.D
Acq On : 19 May 2021 23:04
Operator : SY/MD
Sample : M2459-03 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
