

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043847.D
 Acq On : 19 May 2021 23:28
 Operator : SY/MD
 Sample : M2459-04 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GK4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	94	rBV	90191	99460	12.73%	1.672%
2	1.916	170	179	190	rBV	63042	80772	10.34%	1.358%
3	2.571	371	383	399	rBV	151279	248494	31.82%	4.178%
4	3.054	523	533	548	rVB2	10511	20102	2.57%	0.338%
5	4.642	1011	1027	1063	rBV	92803	294627	37.72%	4.954%
6	5.073	1141	1161	1184	rBV	133673	293142	37.53%	4.929%
7	5.735	1345	1367	1389	rBV2	268343	689484	88.28%	11.593%
8	6.256	1513	1529	1548	rBV	248371	470461	60.23%	7.910%
9	6.549	1610	1620	1634	rVB6	12654	23876	3.06%	0.401%
10	6.700	1651	1667	1685	rBV	167494	324621	41.56%	5.458%
11	7.575	1927	1939	1955	rBV	74679	133589	17.10%	2.246%
12	7.906	2024	2042	2057	rBV	307826	534511	68.43%	8.987%
13	7.976	2059	2064	2078	rVB	5171	7964	1.02%	0.134%
14	8.185	2117	2129	2149	rBV2	46590	81054	10.38%	1.363%
15	8.645	2254	2272	2309	rBV	375834	781053	100.00%	13.133%
16	9.423	2500	2514	2554	rVB	365205	608772	77.94%	10.236%
17	10.764	2919	2931	2952	rVB	139283	224034	28.68%	3.767%
18	11.819	3247	3259	3283	rBV	345449	542500	69.46%	9.122%
19	12.201	3363	3378	3395	rBV	302276	488895	62.59%	8.220%




Sum of corrected areas: 5947411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043847.D
Acq On : 19 May 2021 23:28
Operator : SY/MD
Sample : M2459-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

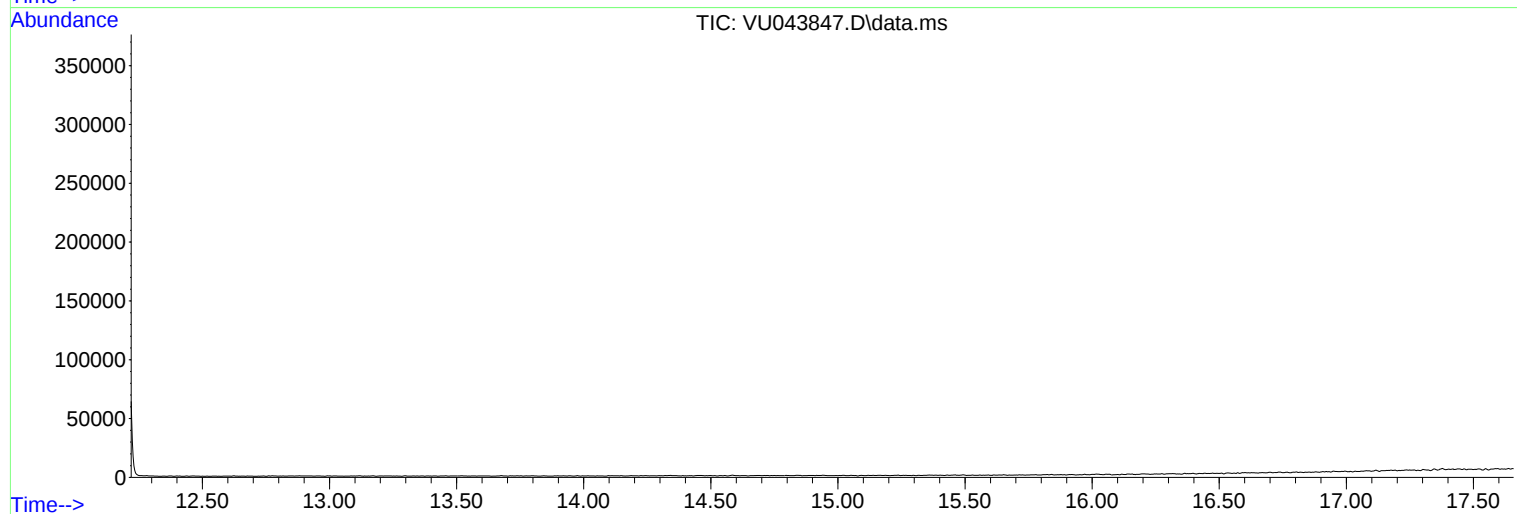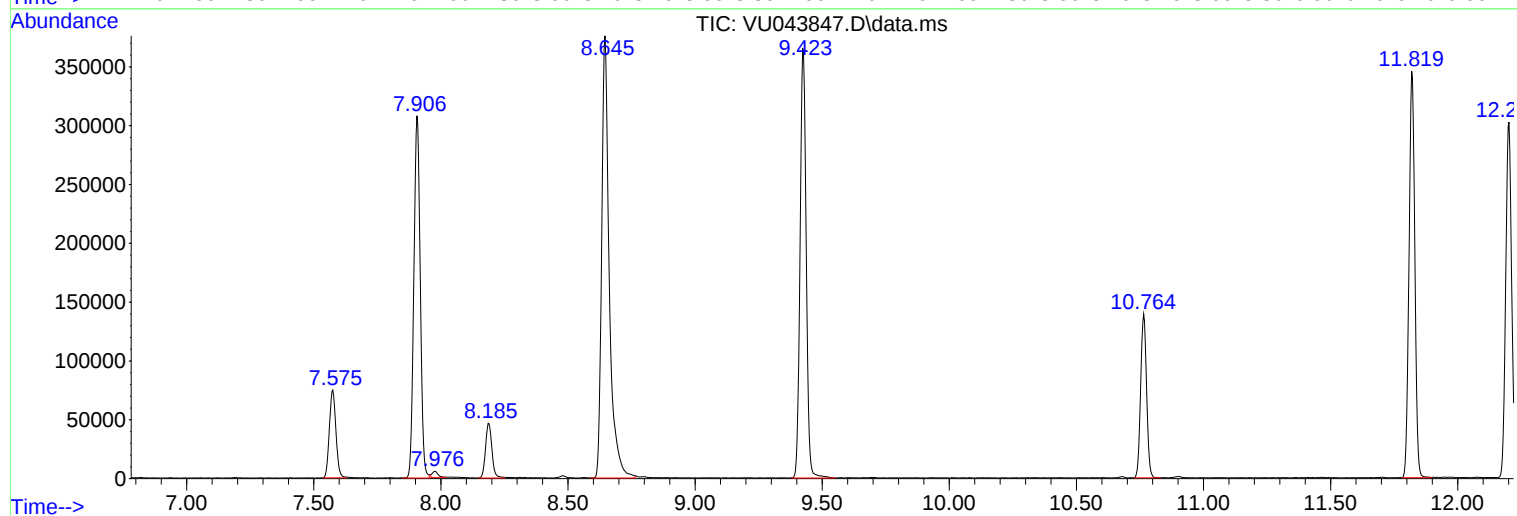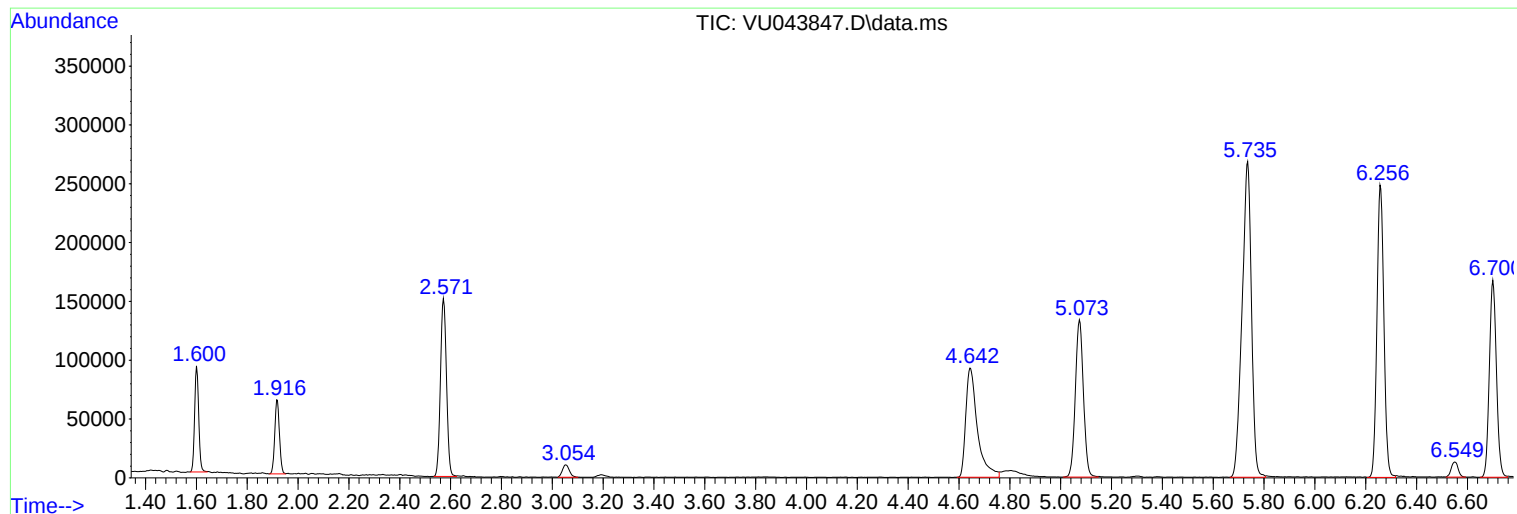

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043847.D
Acq On : 19 May 2021 23:28
Operator : SY/MD
Sample : M2459-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043847.D
Acq On : 19 May 2021 23:28
Operator : SY/MD
Sample : M2459-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
