

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
 Data File : VU043848.D
 Acq On : 19 May 2021 23:52
 Operator : SY/MD
 Sample : M2459-05 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0GK6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	92	rBV	91032	99431	14.12%	1.716%
2	1.919	171	180	190	rVB	64545	81619	11.59%	1.408%
3	2.571	371	383	402	rBV	153581	248179	35.25%	4.282%
4	3.054	523	533	546	rVB2	8268	15121	2.15%	0.261%
5	4.649	1012	1029	1075	rBV	89267	299658	42.56%	5.170%
6	5.073	1143	1161	1186	rBV	131620	296059	42.05%	5.108%
7	5.735	1346	1367	1388	rBV2	267146	684550	97.23%	11.811%
8	6.256	1514	1529	1549	rBV	236837	456329	64.82%	7.874%
9	6.549	1609	1620	1632	rBV5	7073	13029	1.85%	0.225%
10	6.700	1653	1667	1687	rBV	165812	322464	45.80%	5.564%
11	7.574	1927	1939	1958	rBV	75011	130564	18.55%	2.253%
12	7.906	2029	2042	2056	rBV	312372	536677	76.23%	9.260%
13	8.185	2118	2129	2148	rBV	46726	79812	11.34%	1.377%
14	8.645	2259	2272	2306	rBV	346403	704024	100.00%	12.147%
15	8.928	2349	2360	2372	rBV4	4482	8326	1.18%	0.144%
16	9.423	2499	2514	2536	rBV	355896	592984	84.23%	10.232%
17	10.764	2919	2931	2956	rVB	132127	212126	30.13%	3.660%
18	11.819	3246	3259	3276	rBV	332201	527577	74.94%	9.103%
19	12.201	3364	3378	3396	rBV	298093	487119	69.19%	8.405%




Sum of corrected areas: 5795648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043848.D
Acq On : 19 May 2021 23:52
Operator : SY/MD
Sample : M2459-05 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

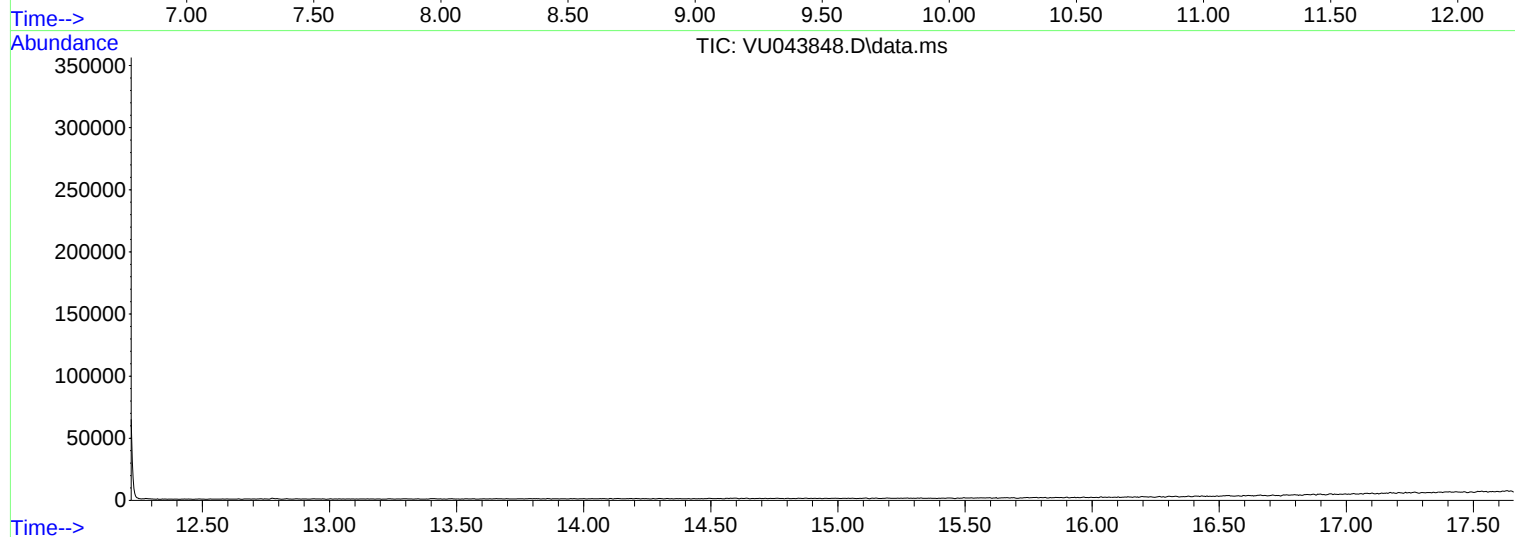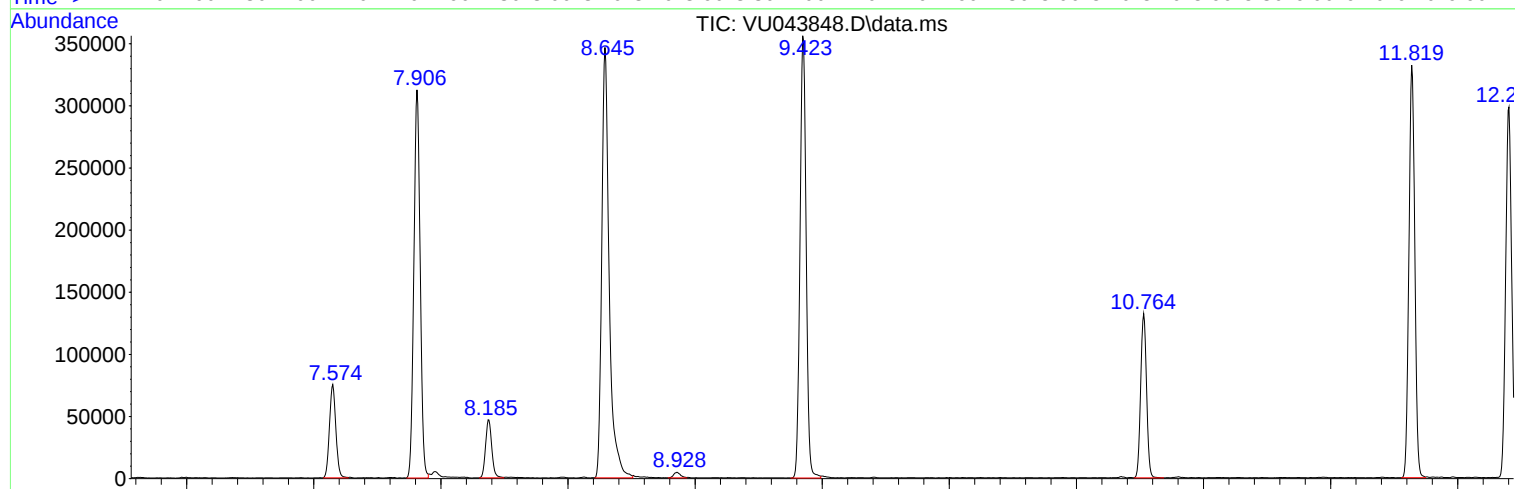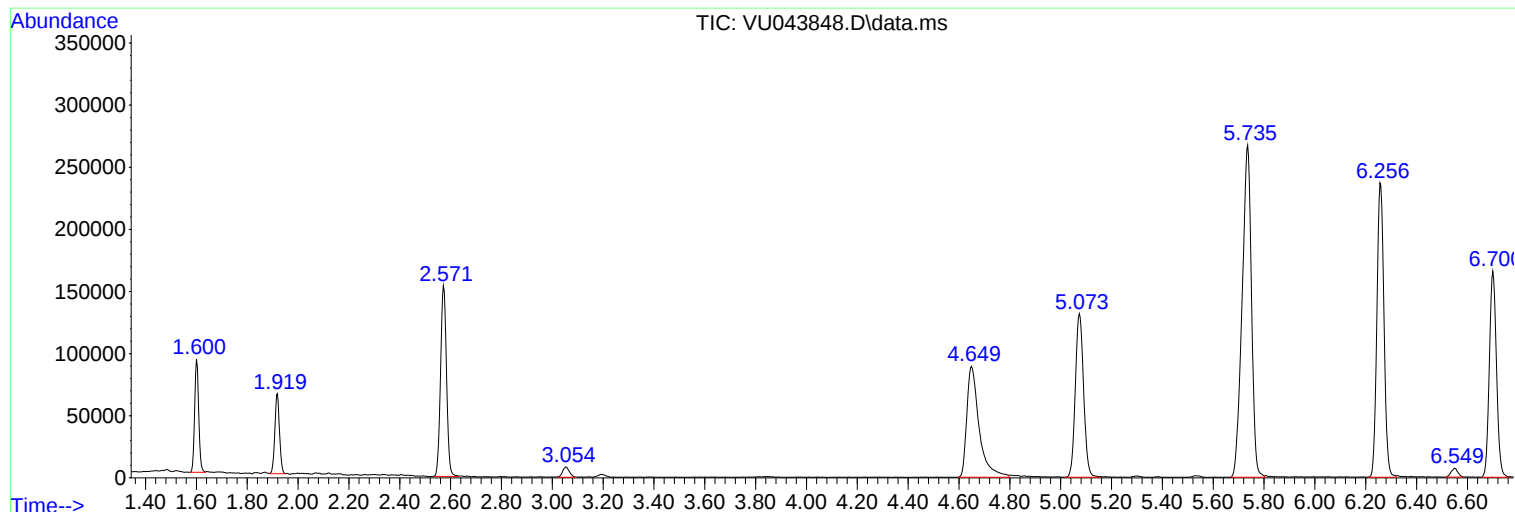

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043848.D
Acq On : 19 May 2021 23:52
Operator : SY/MD
Sample : M2459-05 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052021\
Data File : VU043848.D
Acq On : 19 May 2021 23:52
Operator : SY/MD
Sample : M2459-05 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0GK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
